

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111017\
 Data File : BF100415.D
 Acq On : 11 Nov 2017 2:34
 Operator : SJ/JU
 Sample : I6355-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110317-TIFR-F-D-B

Quant Time: Nov 13 07:44:10 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:44:40 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	150145	20.00	ng	0.00
21) Naphthalene-d8	8.18	136	541912	20.00	ng	0.00
38) Acenaphthene-d10	9.94	164	219873	20.00	ng	0.00
63) Phenanthrene-d10	11.42	188	345925	20.00	ng	0.00
75) Chrysene-d12	14.06	240	298696	20.00	ng	0.00
86) Perylene-d12	15.54	264	229409	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	502730	53.67	ng	0.00
7) Phenol-d6	6.52	99	412737	35.73	ng	-0.01
23) Nitrobenzene-d5	7.47	82	917958	111.99	ng	0.00
41) 2,4,6-Tribromophenol	10.73	330	193103	86.19	ng	0.00
44) 2-Fluorobiphenyl	9.26	172	1509629	104.55	ng	0.00
78) Terphenyl-d14	13.01	244	1117299	85.95	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF111017\
Data File : BF100415.D
Acq On : 11 Nov 2017 2:34
Operator : SJ/JU
Sample : I6355-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110317-TIFR-F-D-B

Quant Time: Nov 13 07:44:10 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:44:40 2017
Response via : Initial Calibration

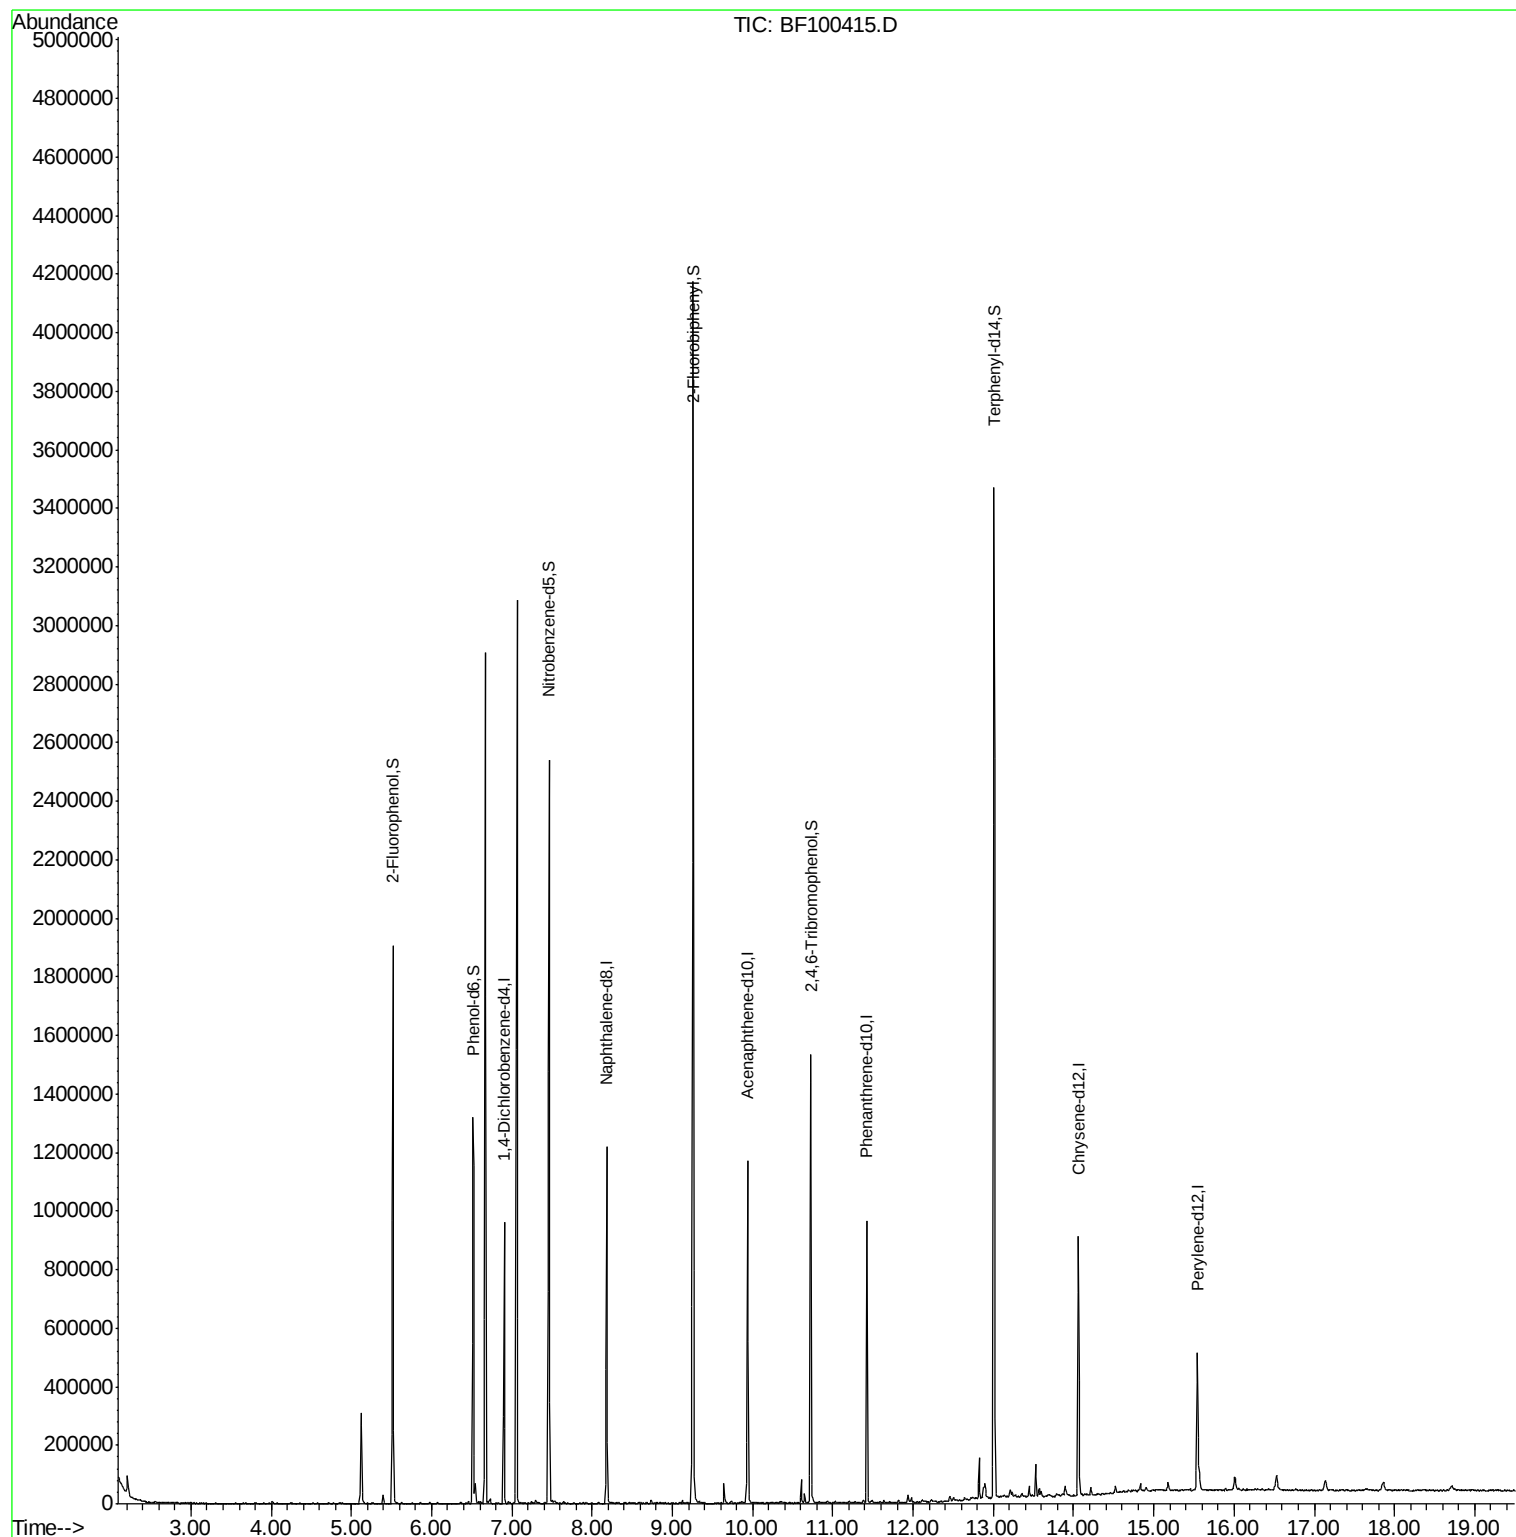







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.90 min Scan# 819
 Delta R.T. -0.00 min
 Lab File: BF100415.D
 Acq: 11 Nov 2017 2:34

Instrument :
 BNA_F
 ClientSampleId :
 110317-TIFR-F-D-B

Tot Ion:152 Resp: 150145
 Ion Ratio Lower Upper
 152 100
 150 155.1 124.6 186.8
 115 56.7 50.1 75.1

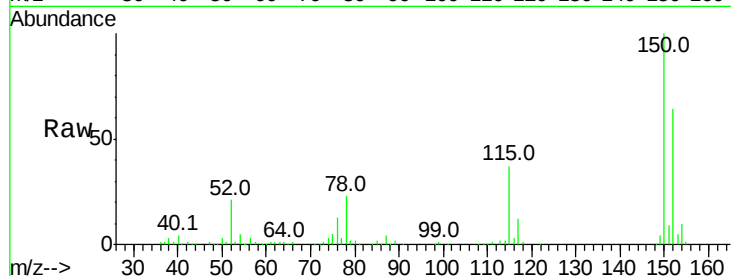


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

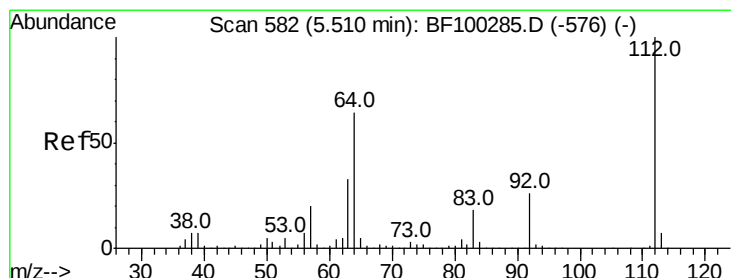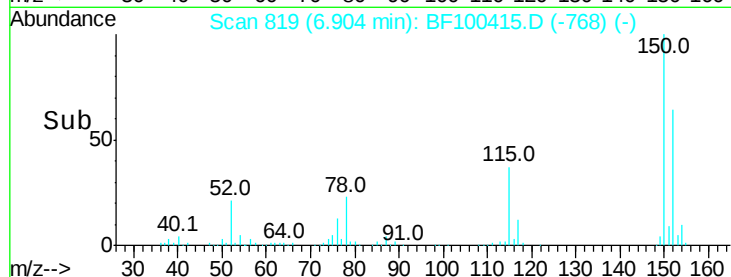
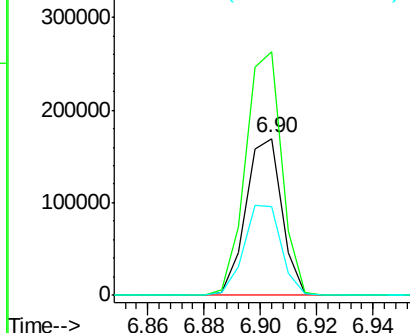


#5
 2-Fluorophenol
 Concen: 53.673 ng
 RT: 5.52 min Scan# 583
 Delta R.T. -0.00 min
 Lab File: BF100415.D
 Acq: 11 Nov 2017 2:34

Tgt Ion:112 Resp: 502730
 Ion Ratio Lower Upper
 112 100
 64 62.7 47.9 71.9
 63 31.9 23.7 35.5

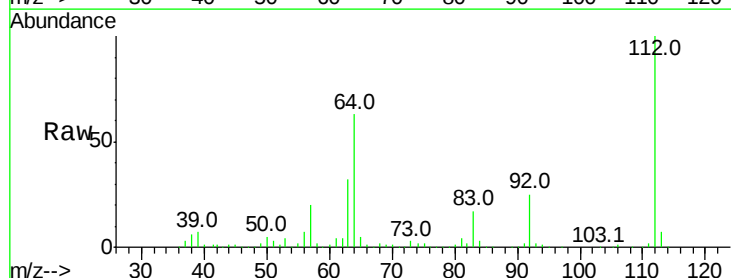

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

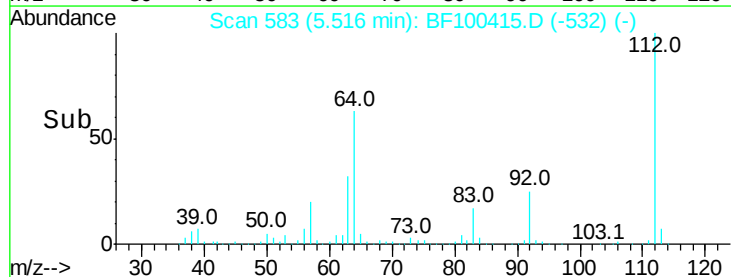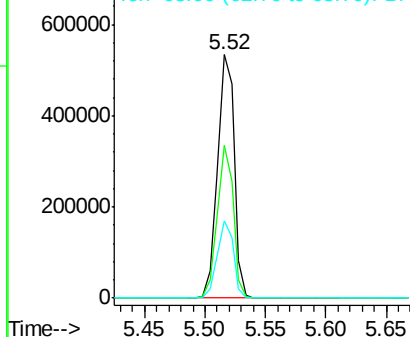



#7

Phenol-d6

Concen: 35.734 ng

RT: 6.52 min Scan# 753

Delta R.T. -0.01 min

Lab File: BF100415.D

Acq: 11 Nov 2017 2:34

Instrument :

BNA_F

ClientSampleId :

110317-TIFR-F-D-B





Tot Ion: 99 Resp: 412737

Ion Ratio Lower Upper

99 100

42 20.4 14.5 21.7

71 31.9 25.4 38.0

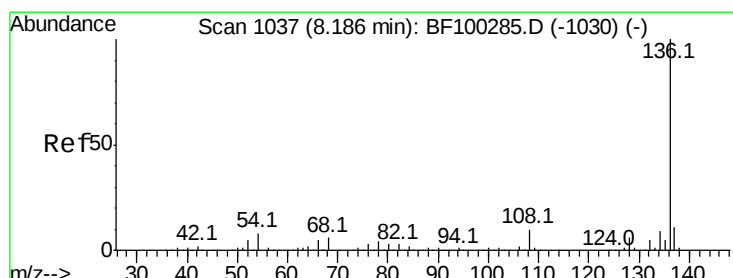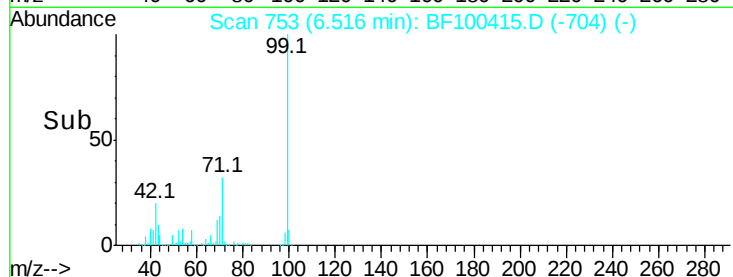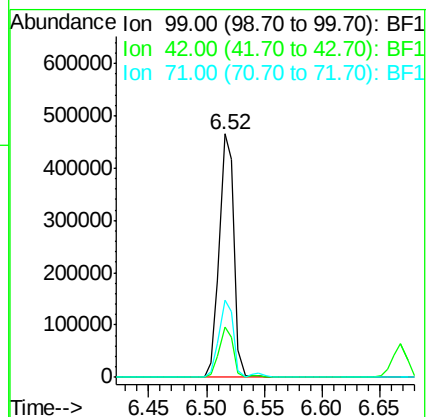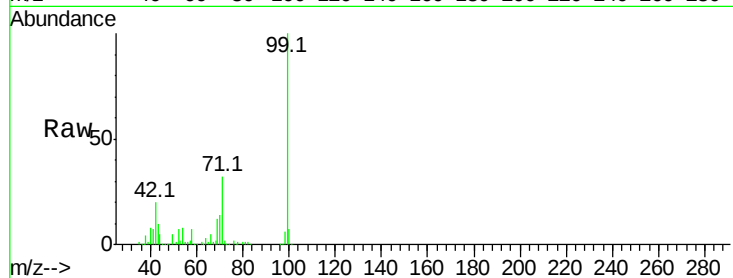

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.18 min Scan# 1036

Delta R.T. -0.01 min

Lab File: BF100415.D

Acq: 11 Nov 2017 2:34

Tgt Ion: 136 Resp: 541912




Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 9.2 6.6 9.8

68 6.5 5.0 7.4

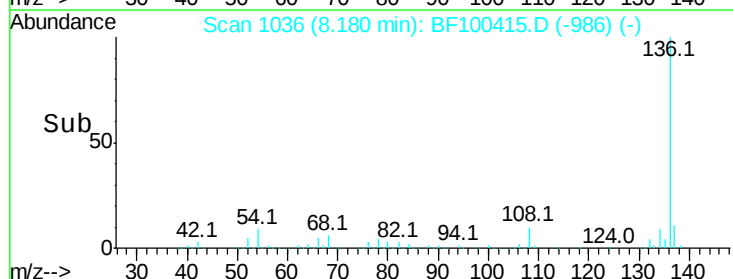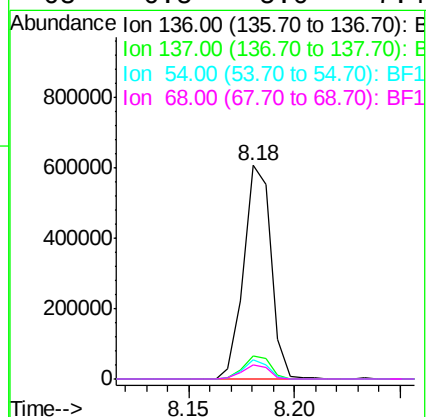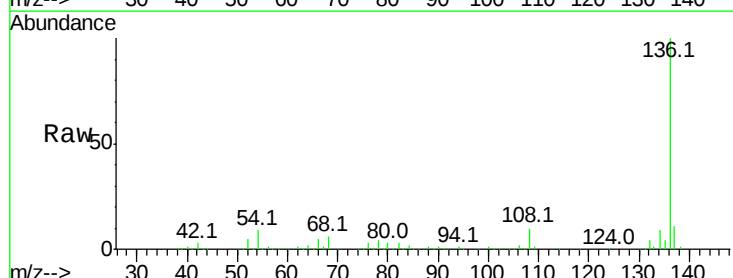







#23
 Nitrobenzene-d5
 Concen: 111.991 ng
 RT: 7.47 min Scan# 915
 Delta R.T. -0.00 min
 Lab File: BF100415.D
 Acq: 11 Nov 2017 2:34

Instrument :
 BNA_F
 ClientSampleId :
 110317-TIFR-F-D-B

Tot Ion	82	Resp	917958
Ion Ratio	100	Lower	Upper
128	47.2	36.1	54.1
54	53.4	41.4	62.2

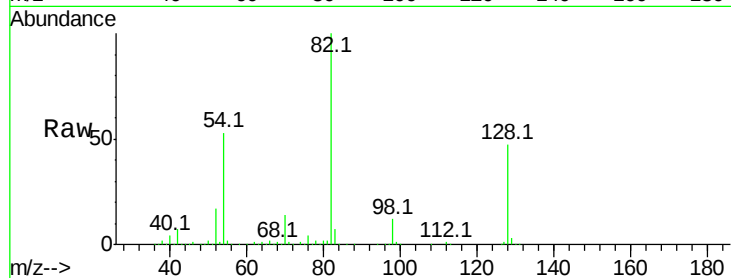


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

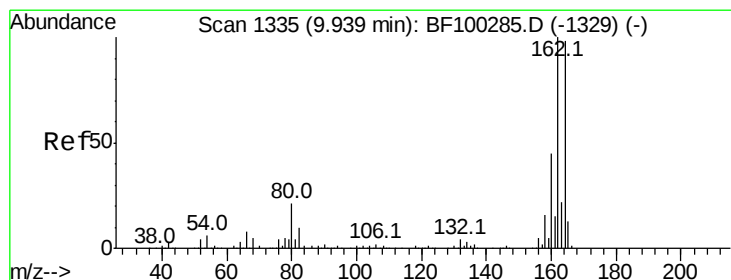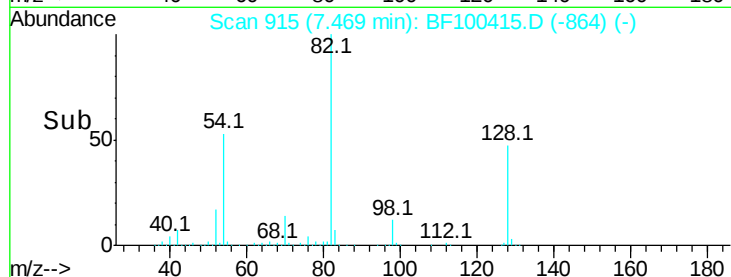
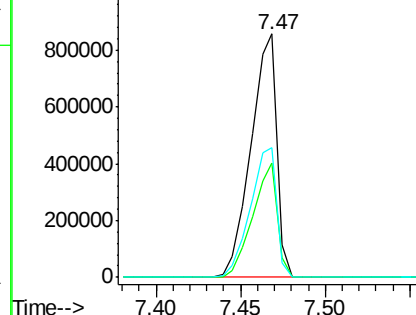


#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.94 min Scan# 1335
 Delta R.T. -0.01 min
 Lab File: BF100415.D
 Acq: 11 Nov 2017 2:34

Tgt Ion	164	Resp	219873
Ion Ratio	100	Lower	Upper
162	106.6	86.1	129.1
160	48.3	38.3	57.5

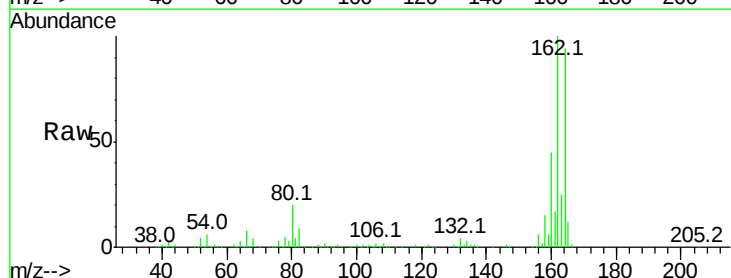

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1


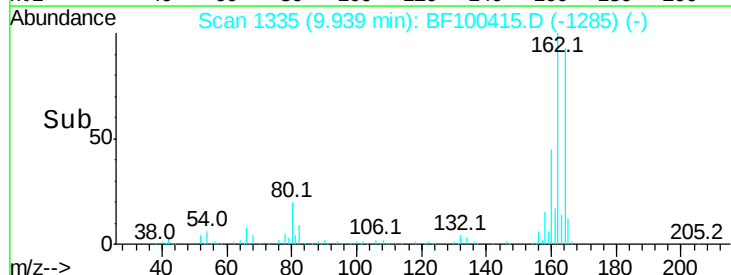
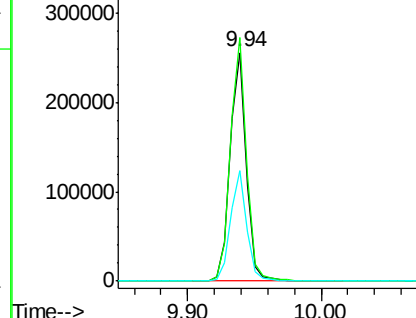




#41
 2,4,6-Tribromophenol
 Concen: 86.187 ng
 RT: 10.73 min Scan# 1469
 Delta R.T. -0.01 min
 Lab File: BF100415.D
 Acq: 11 Nov 2017 2:34




Instrument :
 BNA_F
 ClientSampleId :
 110317-TIFR-F-D-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.0	77.0	115.6
141	31.0	29.9	44.9

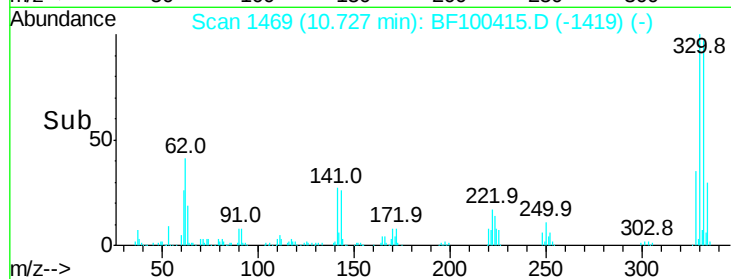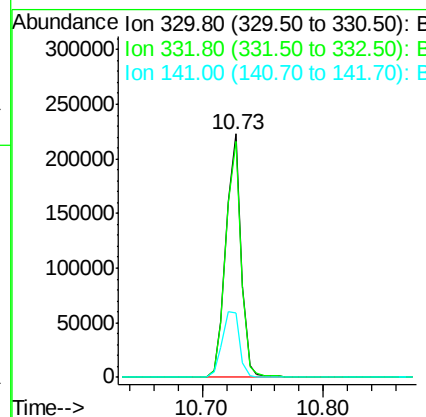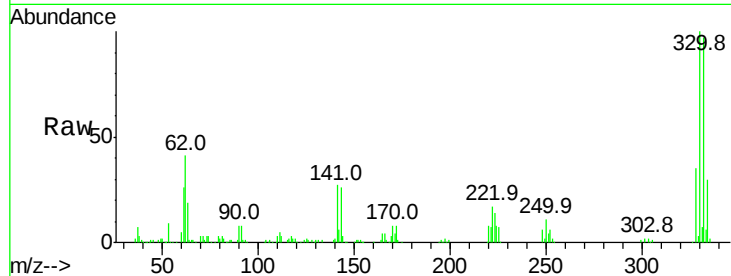

#44
 2-Fluorobiphenyl
 Concen: 104.548 ng
 RT: 9.26 min Scan# 1220
 Delta R.T. -0.00 min
 Lab File: BF100415.D
 Acq: 11 Nov 2017 2:34

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.7	44.5
170	24.5	19.6	29.4


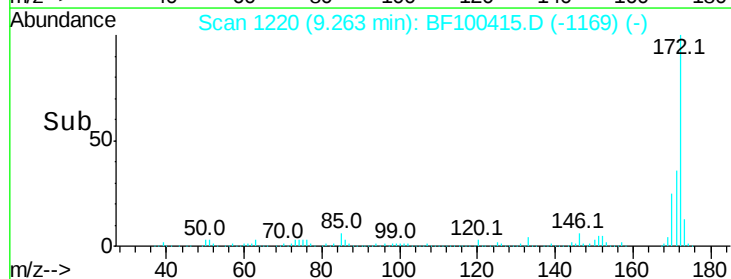
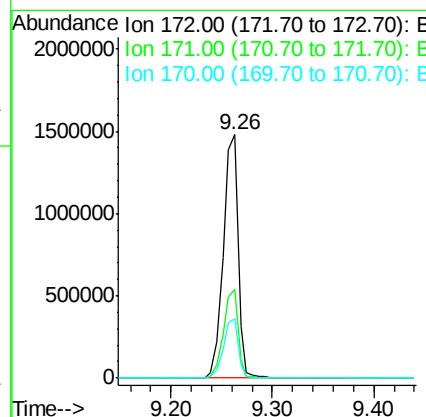
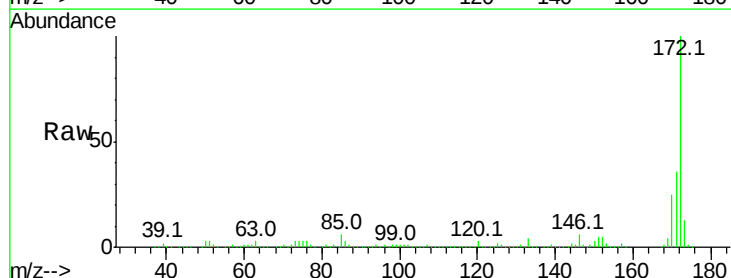




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.42 min Scan# 1587
Delta R.T. -0.01 min
Lab File: BF100415.D
Acq: 11 Nov 2017 2:34




Instrument :
BNA_F
ClientSampleId :
110317-TIFR-F-D-B

Tot Ion:188 Resp: 345925
Ion Ratio Lower Upper
188 100
94 11.6 8.5 12.7
80 11.6 9.2 13.8

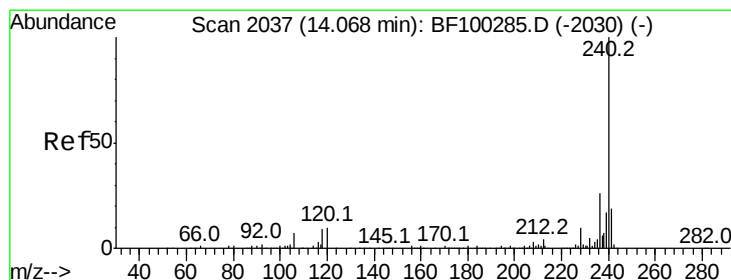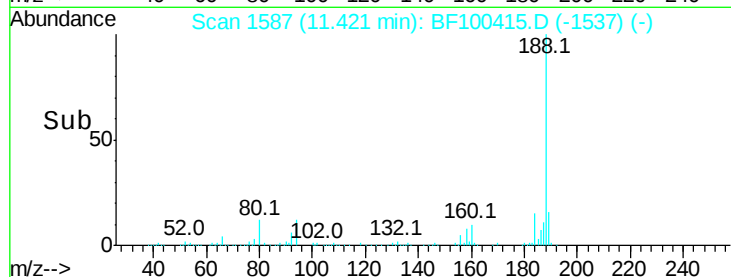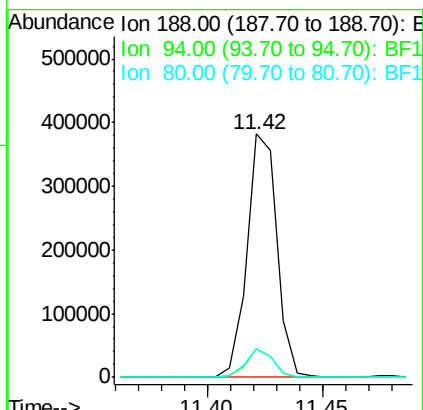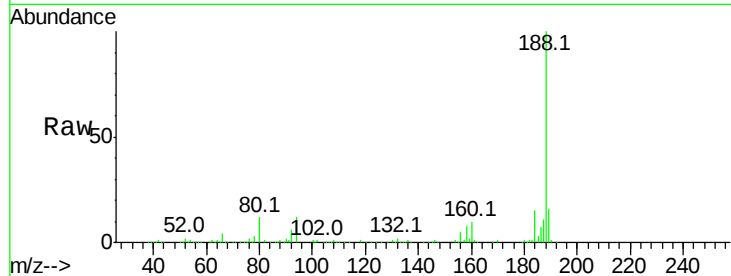

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.06 min Scan# 2036
Delta R.T. -0.01 min
Lab File: BF100415.D
Acq: 11 Nov 2017 2:34

Tgt Ion:240 Resp: 298696
Ion Ratio Lower Upper
240 100
120 11.4 9.5 14.3
236 26.1 20.7 31.1

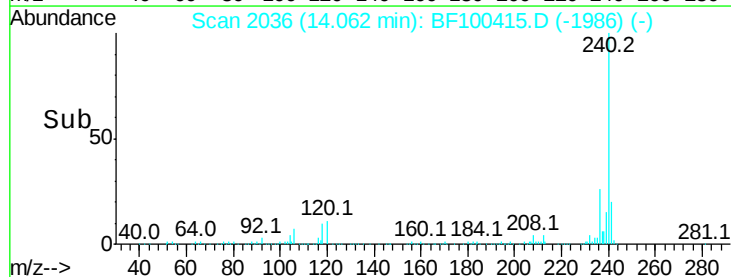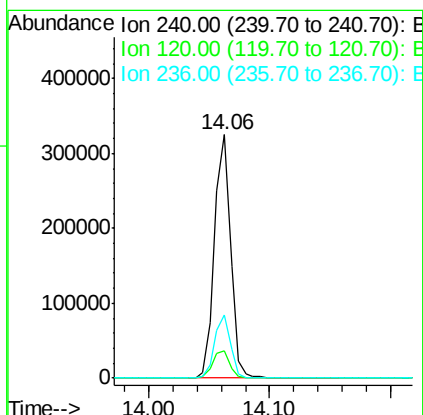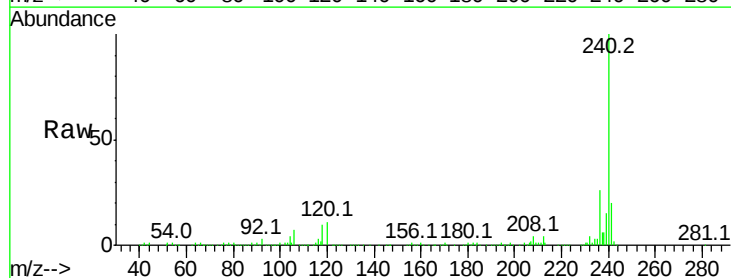



#78

Terphenyl-d14

Concen: 85.948 ng

RT: 13.01 min Scan# 1857

Delta R.T. -0.00 min

Lab File: BF100415.D

Acq: 11 Nov 2017 2:34

Instrument :

BNA_F

ClientSampleId :

110317-TIFR-F-D-B


Tot Ion:244 Resp: 1117299

Ion Ratio Lower Upper

244 100

212 7.4 5.4 8.0




122 11.7 11.0 16.4

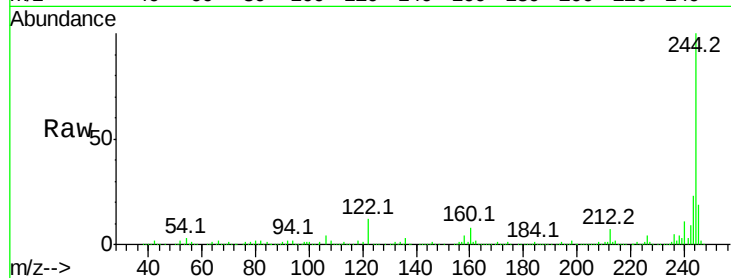

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

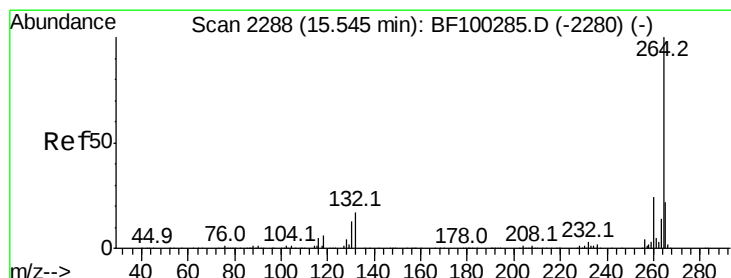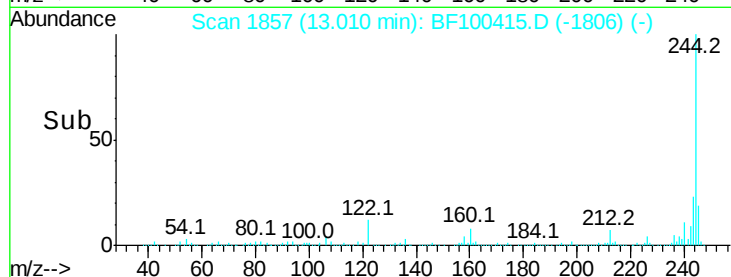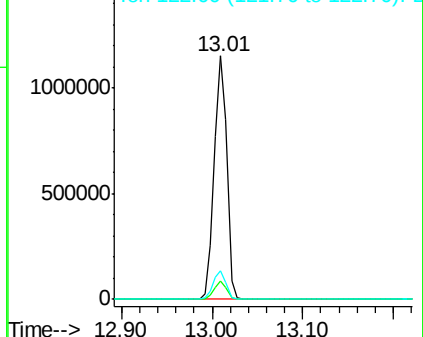

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.54 min Scan# 2288

Delta R.T. -0.00 min

Lab File: BF100415.D

Acq: 11 Nov 2017 2:34


Tgt Ion:264 Resp: 229409

Ion Ratio Lower Upper

264 100

260 22.7 19.2 28.8

265 21.0 17.5 26.3

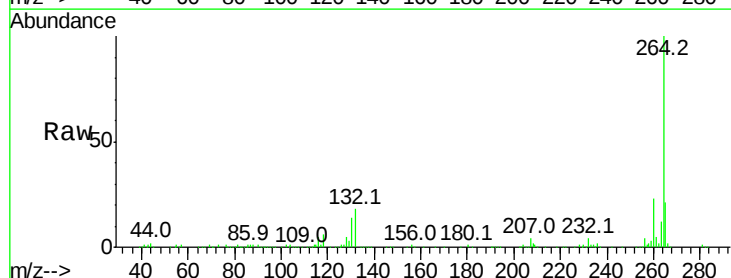

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

