

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF111017\
 Data File : BF100395.D
 Acq On : 10 Nov 2017 17:08
 Operator : SJ/JU
 Sample : I6364-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 N-P001-001-0001-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	511	514	519	rBV	61440	62272	4.32%	0.619%
2	5.504	577	581	584	rBV	405709	382281	26.50%	3.797%
3	6.510	748	752	756	rBV	484952	391898	27.17%	3.893%
4	6.663	774	778	781	rBV	495260	400364	27.76%	3.977%
5	6.898	814	818	822	rBV	1267438	1021686	70.84%	10.149%
6	7.051	841	844	848	rVB	369817	314841	21.83%	3.127%
7	7.457	909	913	916	rBV	252564	228286	15.83%	2.268%
8	8.181	1032	1036	1040	rBV	1646232	1351220	93.68%	13.422%
9	9.251	1215	1218	1226	rBV	573845	477830	33.13%	4.747%
10	9.369	1234	1238	1241	rVB2	18954	17127	1.19%	0.170%
11	9.522	1261	1264	1267	rVB	28019	20317	1.41%	0.202%
12	9.839	1313	1318	1321	rBV5	12723	15804	1.10%	0.157%
13	9.939	1331	1335	1350	rBV	1519263	1442340	100.00%	14.327%
14	10.645	1450	1455	1461	rVB	26774	24923	1.73%	0.248%
15	10.722	1464	1468	1476	rVB	238600	225116	15.61%	2.236%
16	11.074	1524	1528	1531	rBV2	17770	18172	1.26%	0.181%
17	11.422	1583	1587	1591	rBV	1525500	1260967	87.43%	12.526%
18	11.933	1671	1674	1680	rBV	61449	67854	4.70%	0.674%
19	12.721	1805	1808	1813	rBV3	30542	38835	2.69%	0.386%
20	13.004	1852	1856	1859	rBV	389554	343146	23.79%	3.409%
21	13.898	2005	2008	2011	rBV4	20313	24319	1.69%	0.242%
22	14.057	2032	2035	2039	rVB	978587	957498	66.39%	9.511%
23	15.174	2223	2225	2231	rVB	49980	60187	4.17%	0.598%
24	15.545	2283	2288	2297	rVB	682965	919688	63.76%	9.136%


Sum of corrected areas: 10066971

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111017\
Data File : BF100395.D
Acq On : 10 Nov 2017 17:08
Operator : SJ/JU
Sample : I6364-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
N-P001-001-0001-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

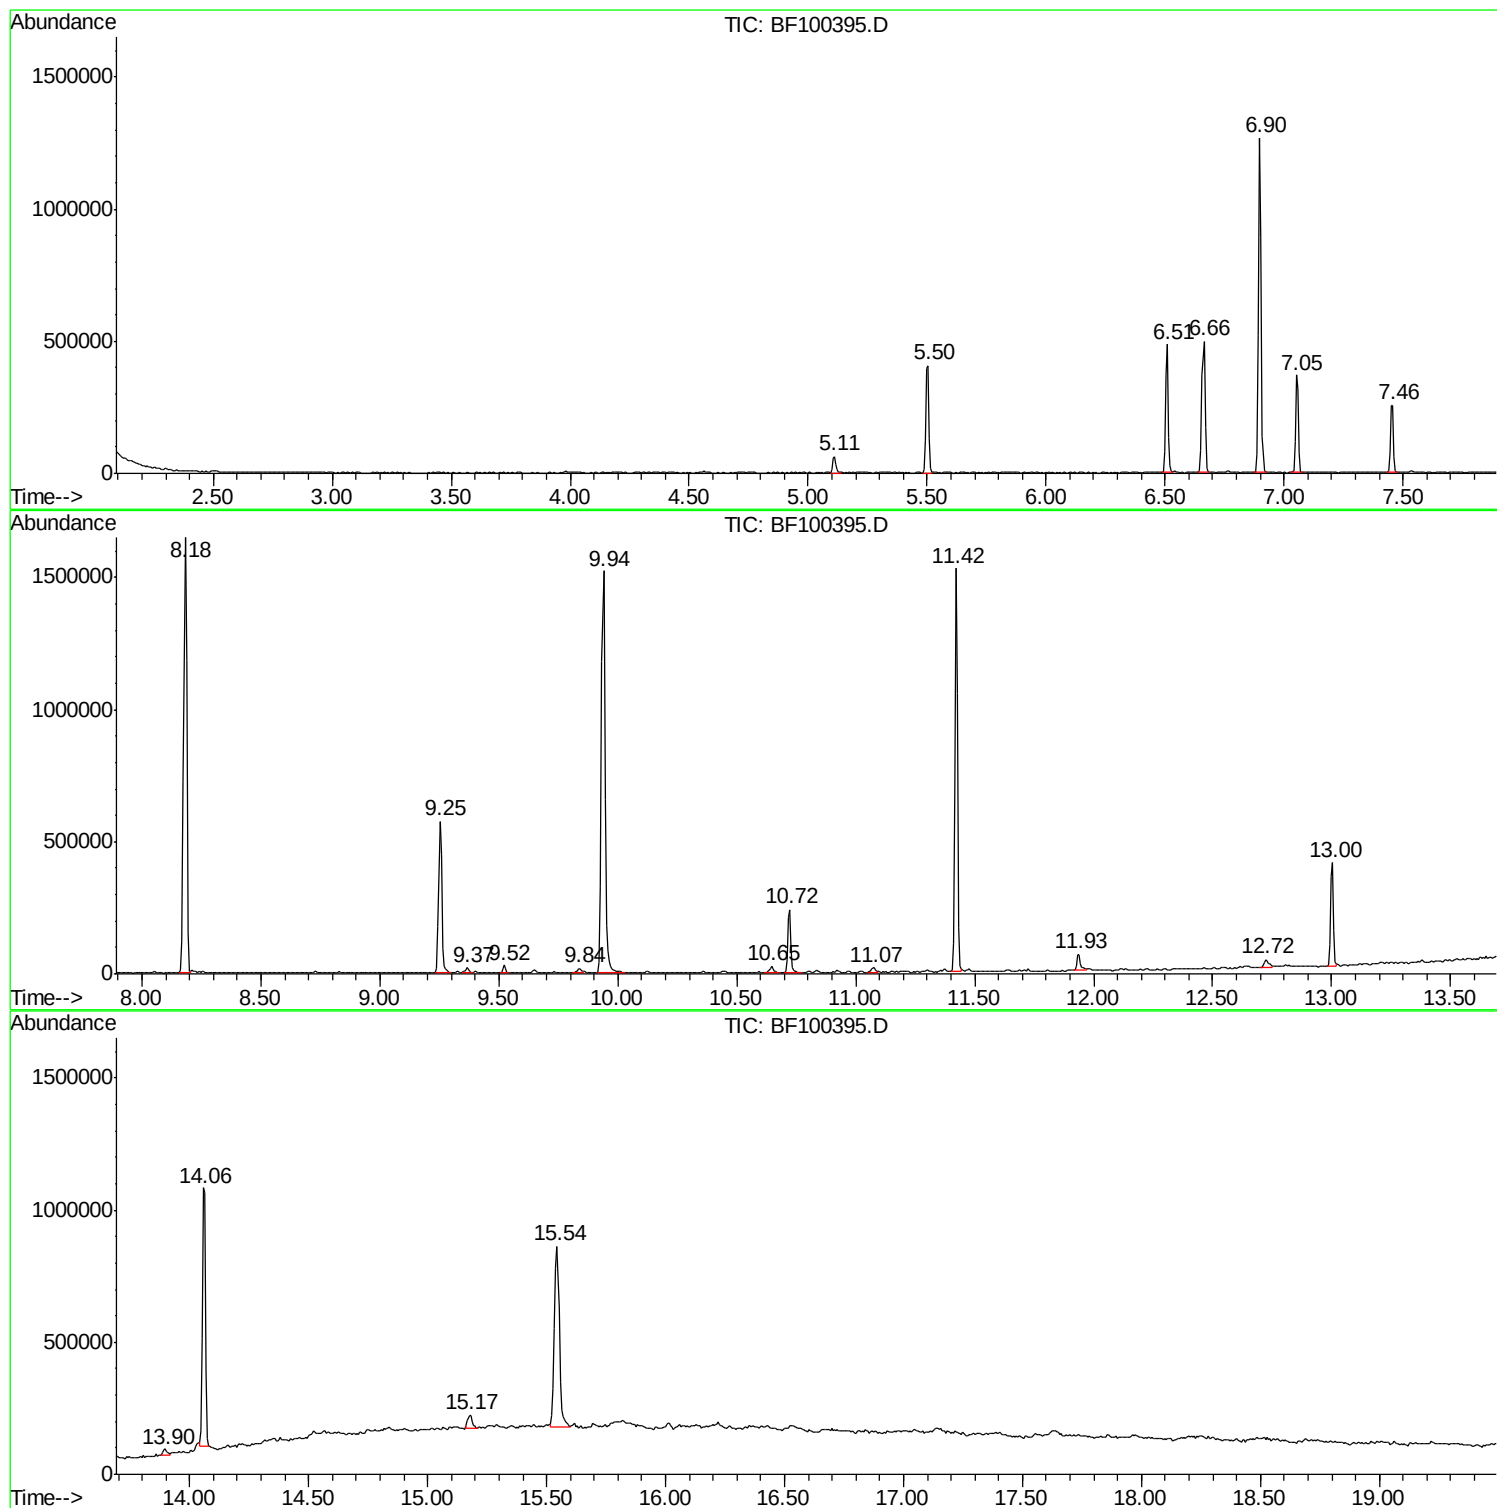

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF111017\
Data File : BF100395.D
Acq On : 10 Nov 2017 17:08
Operator : SJ/JU
Sample : I6364-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
N-P001-001-0001-01










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	7.84 ng	400364	1,4-Dichlorobenzene-d4	6.90

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

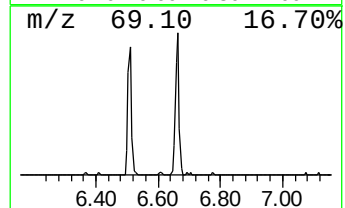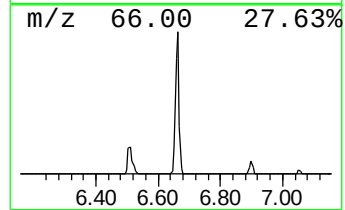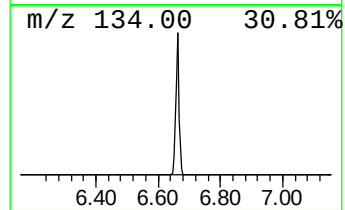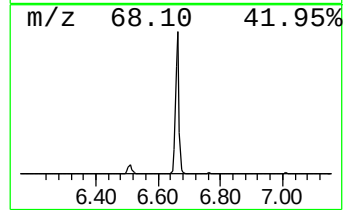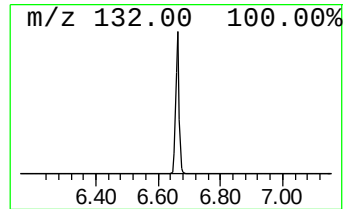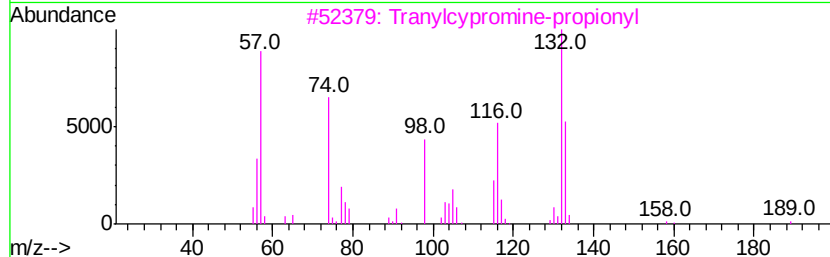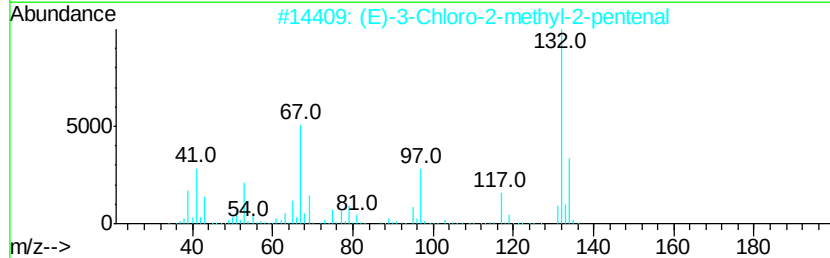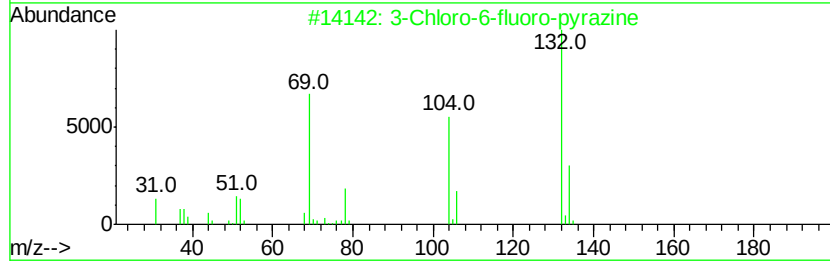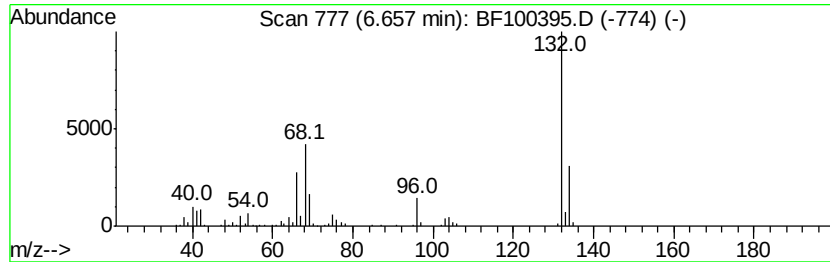

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF111017\
Data File : BF100395.D
Acq On : 10 Nov 2017 17:08
Operator : SJ/JU
Sample : I6364-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
N-P001-001-0001-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.66	6.66	7.8	ng	400364	1	6.90	1021690	20.0