


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111017\
 Data File : BF100407.D
 Acq On : 10 Nov 2017 22:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:44:40 2017

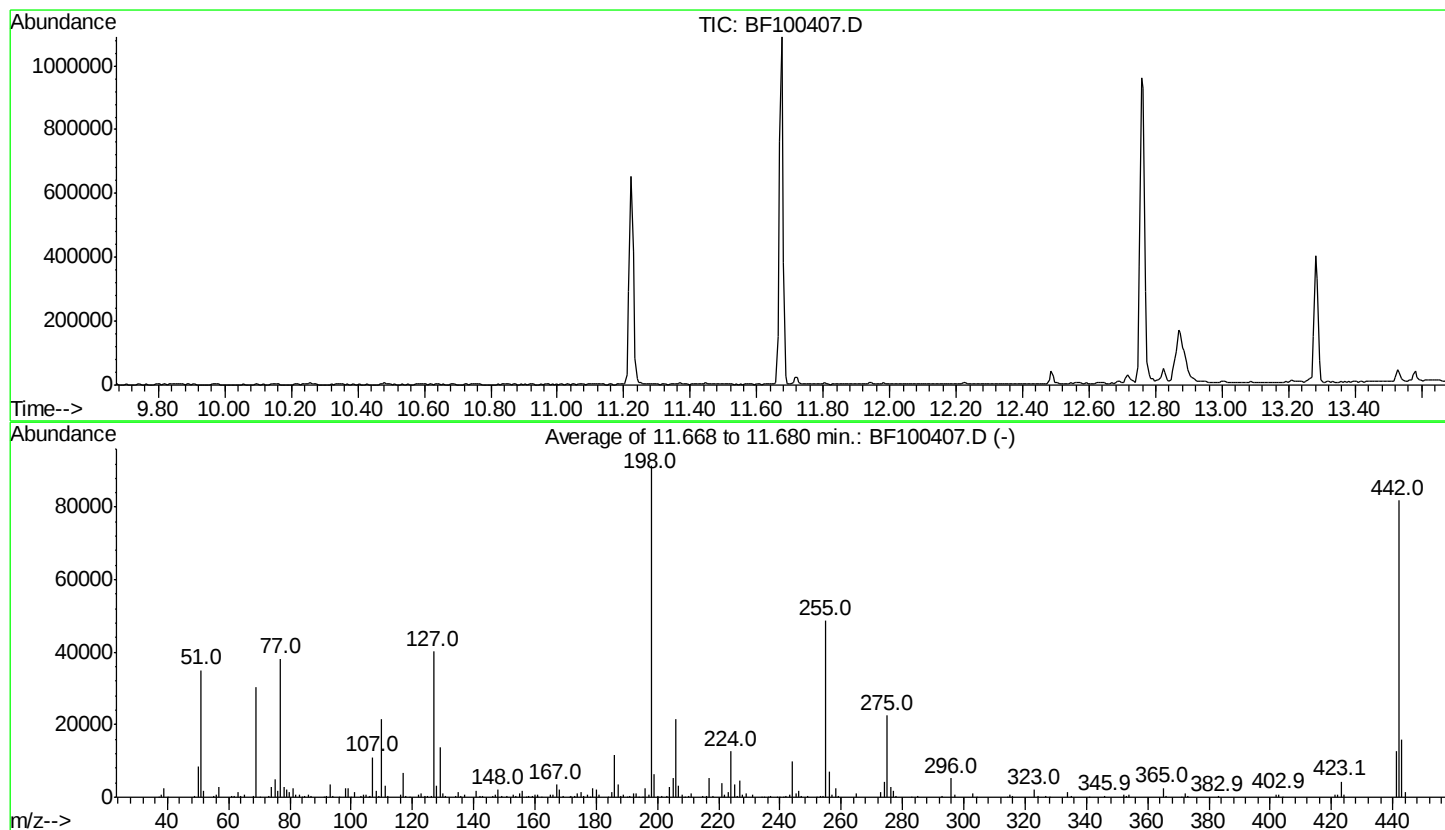

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	35098	PASS
68	69	0.00	2	1.4	424	PASS
69	198	0.00	100	33.1	30264	PASS
70	69	0.00	2	0.4	106	PASS
127	198	10	80	43.8	40110	PASS
197	198	0.00	2	0.6	565	PASS
198	198	100	100	100.0	91482	PASS
199	198	5	9	7.0	6393	PASS
275	198	10	60	24.6	22511	PASS
365	198	1	100	2.9	2644	PASS
441	443	0.01	100	80.5	12827	PASS
442	198	50	100	89.4	81773	PASS
443	442	15	24	19.5	15944	PASS