


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111021\
 Data File : BF126097.D
 Acq On : 10 Nov 2021 9:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 13:31:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 17:21:25 2021
 Response via : Initial Calibration

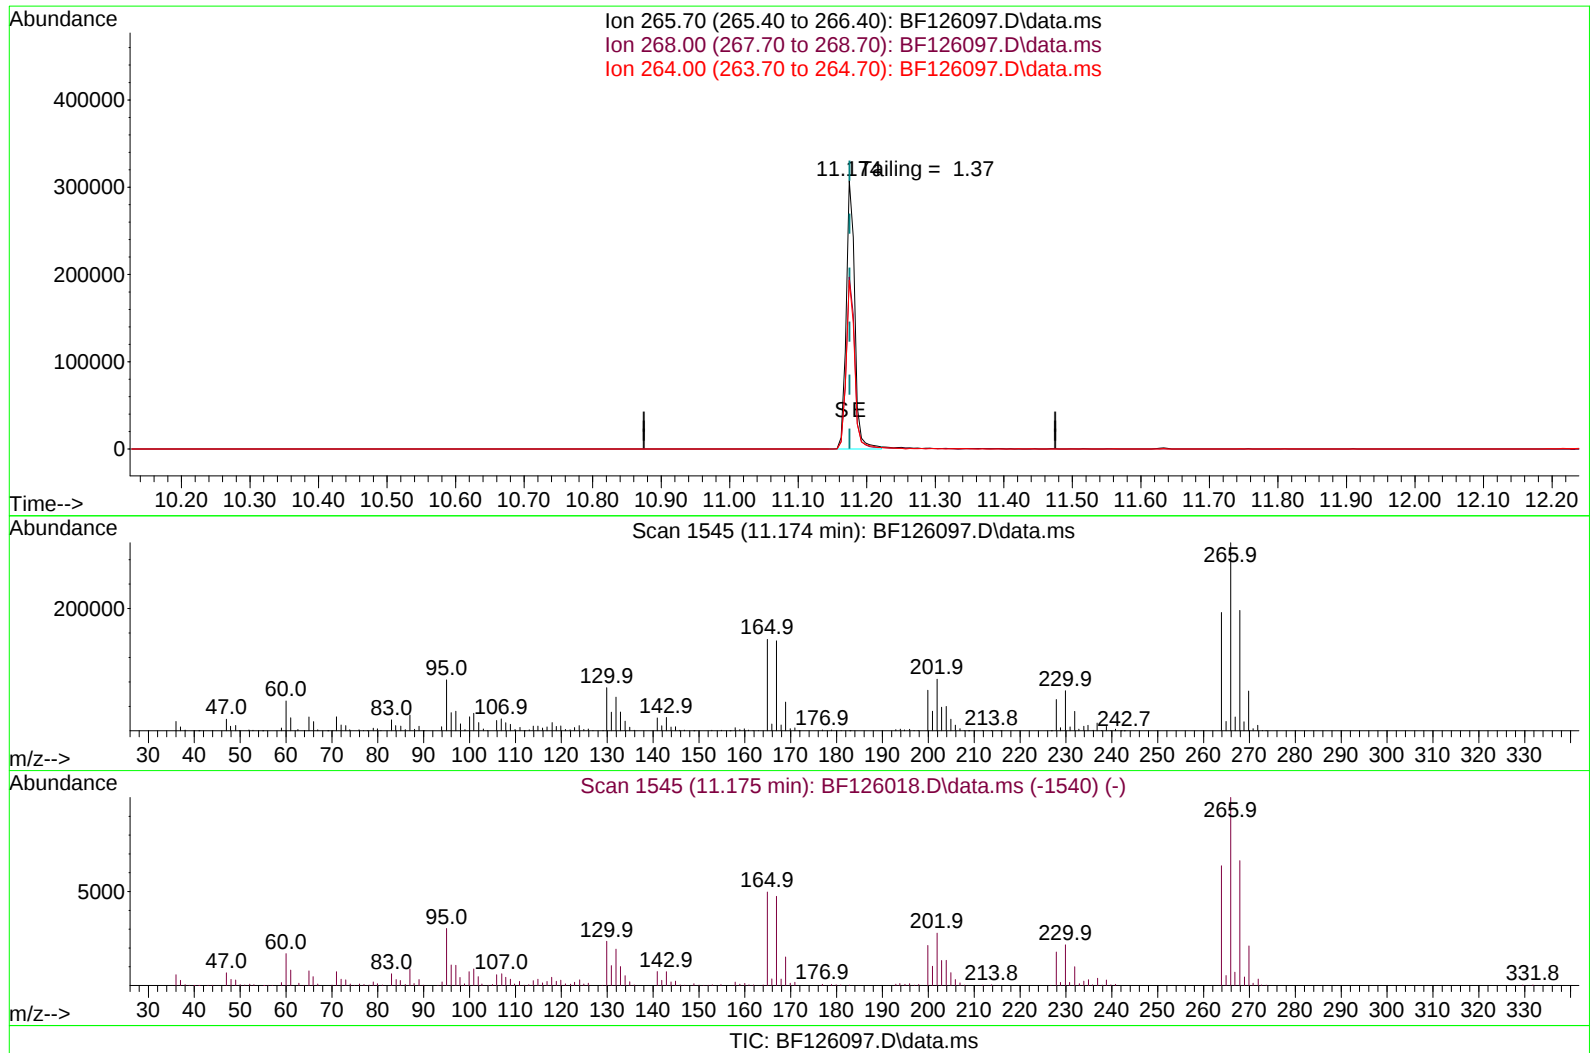

(70) Pentachlorophenol (C)

11.174min (-0.001) 29802.36 ng

response 269232

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.04
264.00	69.90	62.92
0.00	0.00	0.00