
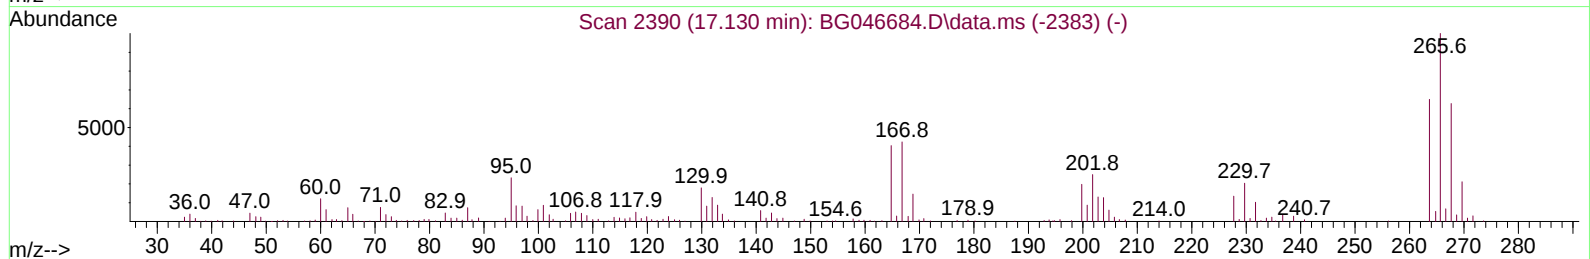
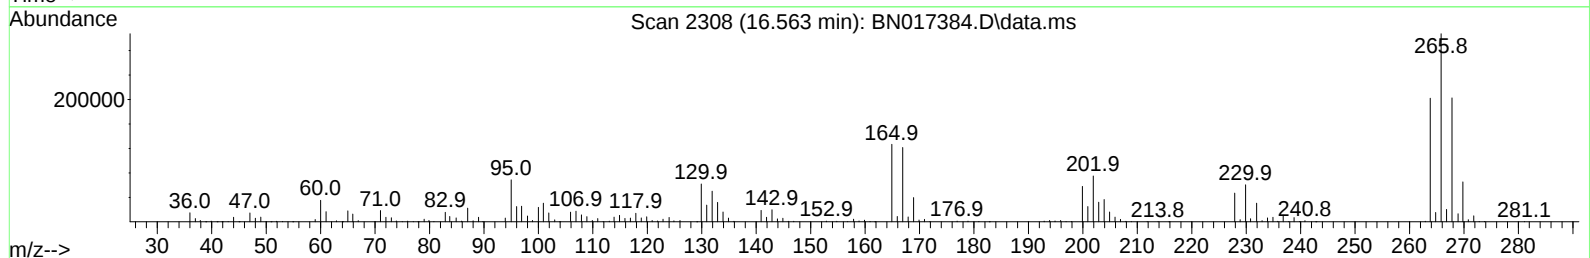


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111121\
Data File : BN017384.D
Acq On : 10 Nov 2021 17:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 07:08:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

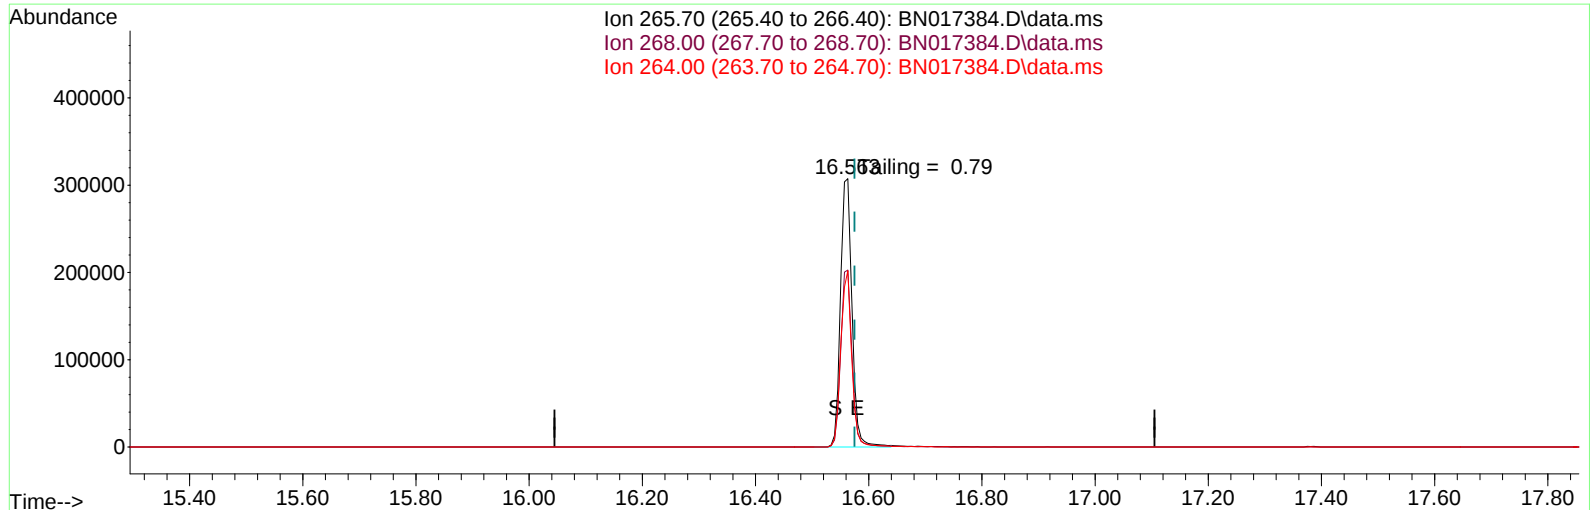

TIC: BN017384.D\data.ms

(70) Pentachlorophenol (C)

16.563min (-0.012) 24757.27 ng

response 433847

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.95
264.00	61.60	65.70
0.00	0.00	0.00