
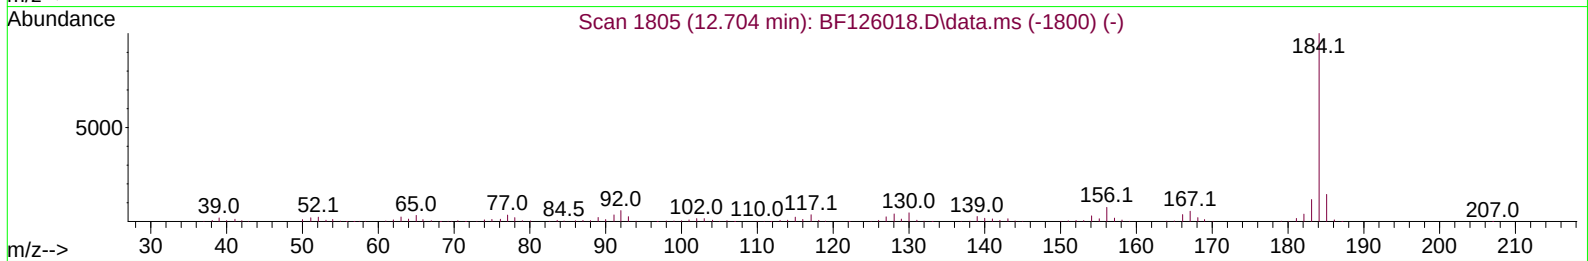
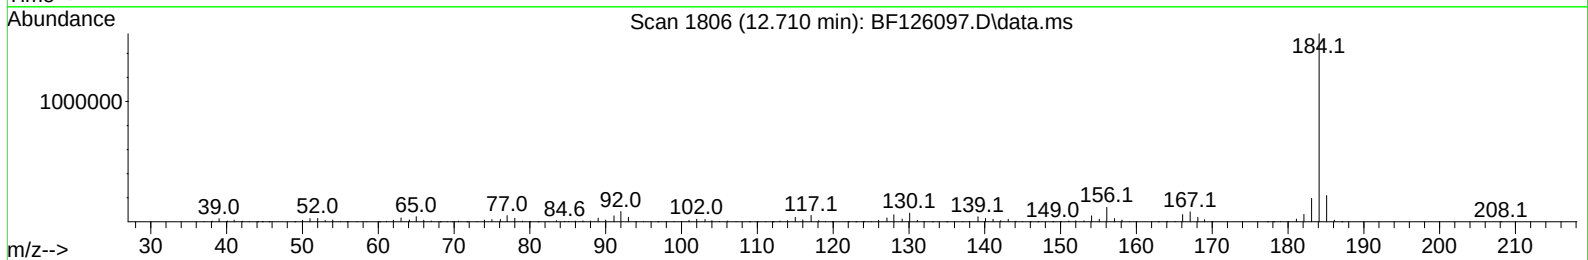


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111021\
Data File : BF126097.D
Acq On : 10 Nov 2021 9:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 13:31:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

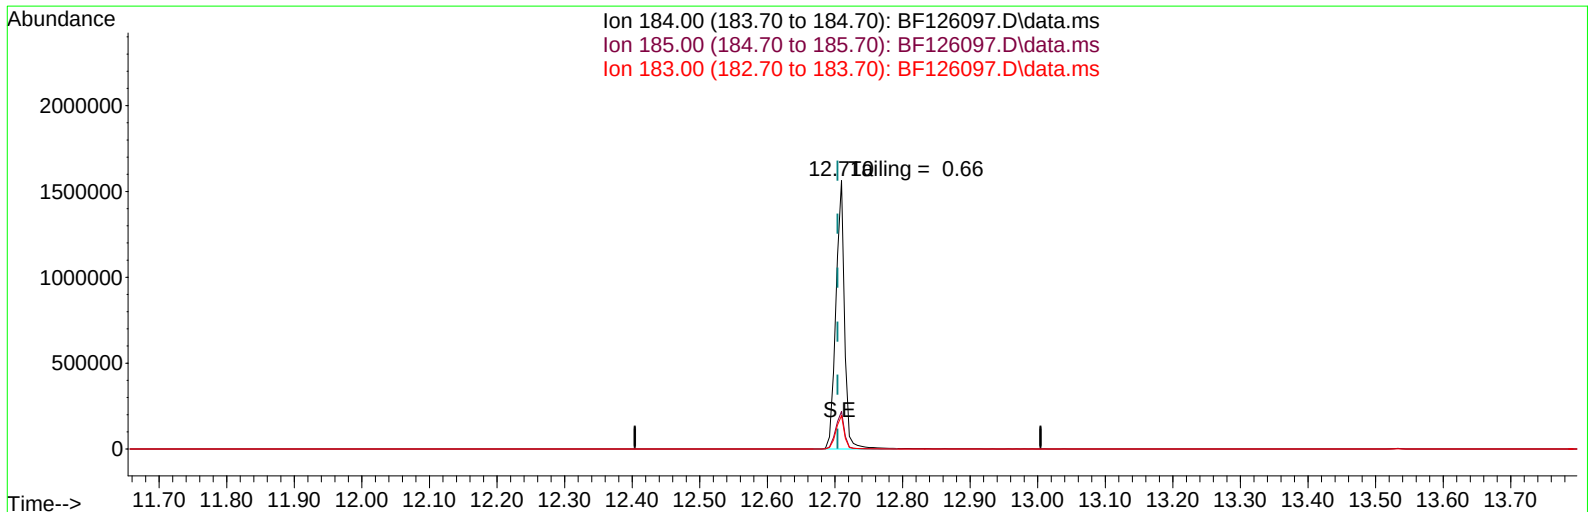

TIC: BF126097.D\data.ms

(77) Benzidine


12.710min (+ 0.006) 350422.47 ng

response 1393997

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.01
183.00	10.10	12.48#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111021\
Data File : BF126097.D
Acq On : 10 Nov 2021 9:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 13:31:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

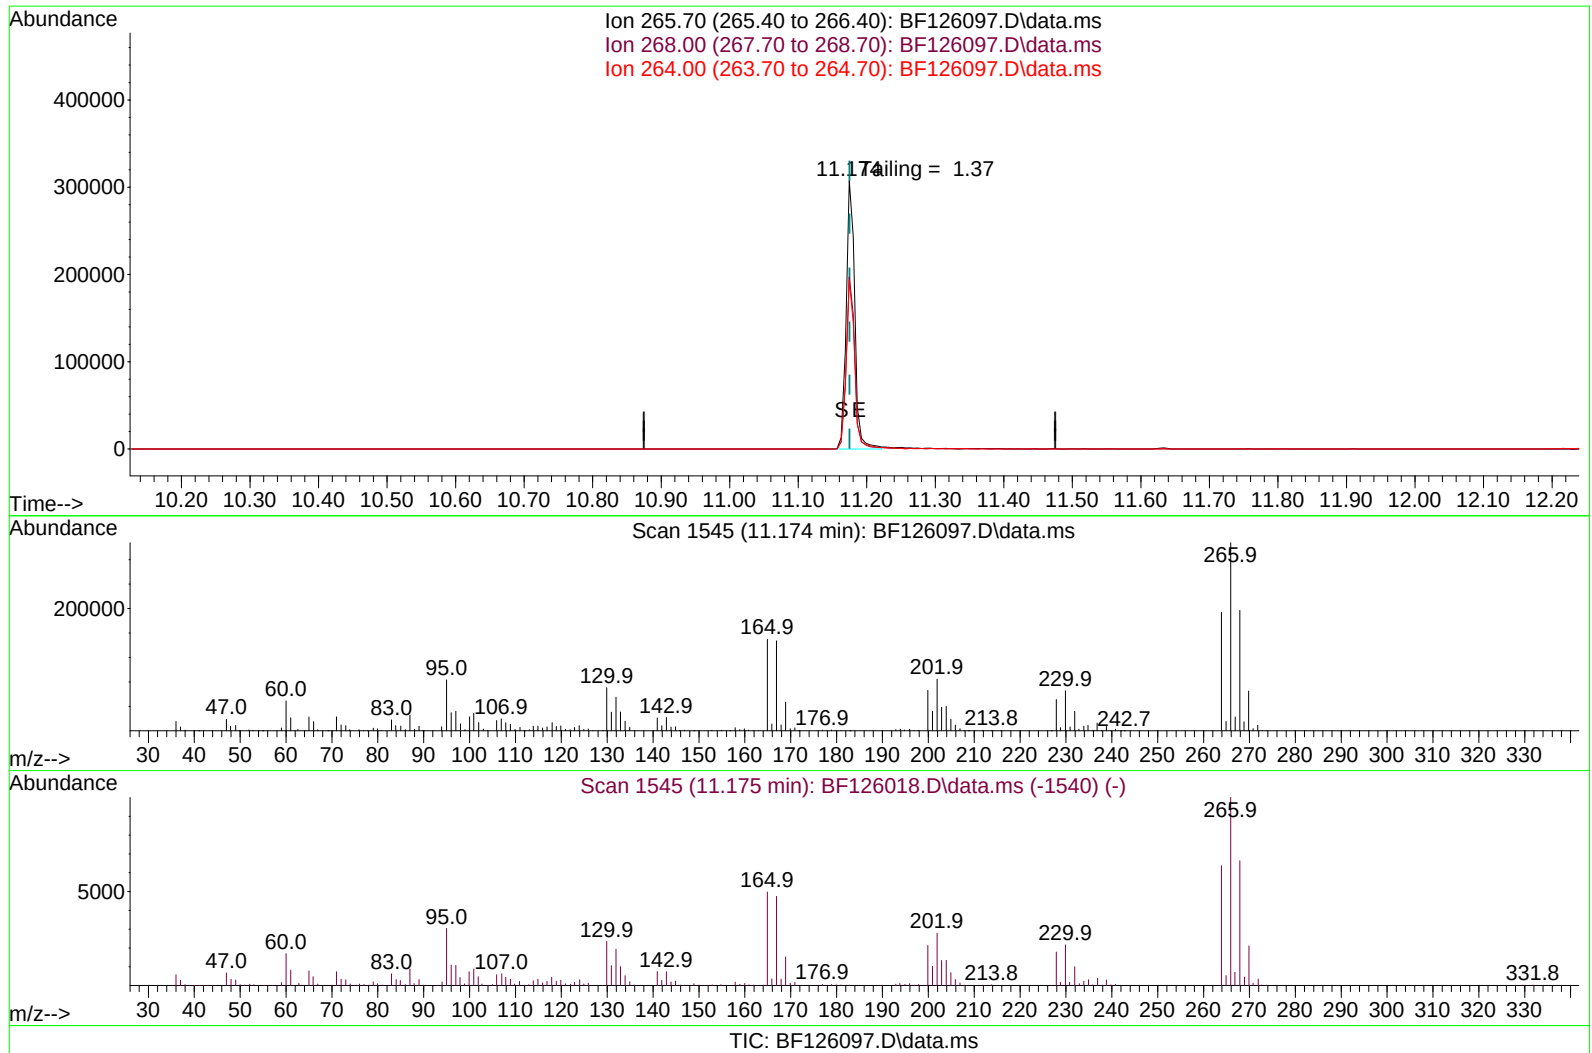**(70) Pentachlorophenol (C)****11.174min (-0.001) 29802.36 ng****response 269232**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.04
264.00	69.90	62.92
0.00	0.00	0.00