

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111021\
 Data File : BF126099.D
 Acq On : 10 Nov 2021 10:15
 Operator : JU/CG
 Sample : PB140520BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB140520BL

Quant Time: Nov 10 13:33:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 17:21:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.851	152	225789	20.000	ng	0.00
21) Naphthalene-d8	8.134	136	840729	20.000	ng	# 0.00
39) Acenaphthene-d10	9.886	164	508383	20.000	ng	0.00
64) Phenanthrene-d10	11.375	188	944668	20.000	ng	0.00
76) Chrysene-d12	14.010	240	724873	20.000	ng	# 0.00
86) Perylene-d12	15.474	264	554517	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	1623038	123.443	ng	0.02
7) Phenol-d6	6.487	99	2045999	110.389	ng	0.00
23) Nitrobenzene-d5	7.416	82	1525728	85.585	ng	0.00
42) 2,4,6-Tribromophenol	10.680	330	762420	130.863	ng	0.00
45) 2-Fluorobiphenyl	9.216	172	2891945	76.872	ng	0.00
79) Terphenyl-d14	12.963	244	3557611	79.142	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111021\
Data File : BF126099.D
Acq On : 10 Nov 2021 10:15
Operator : JU/CG
Sample : PB140520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB140520BL

Quant Time: Nov 10 13:33:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration




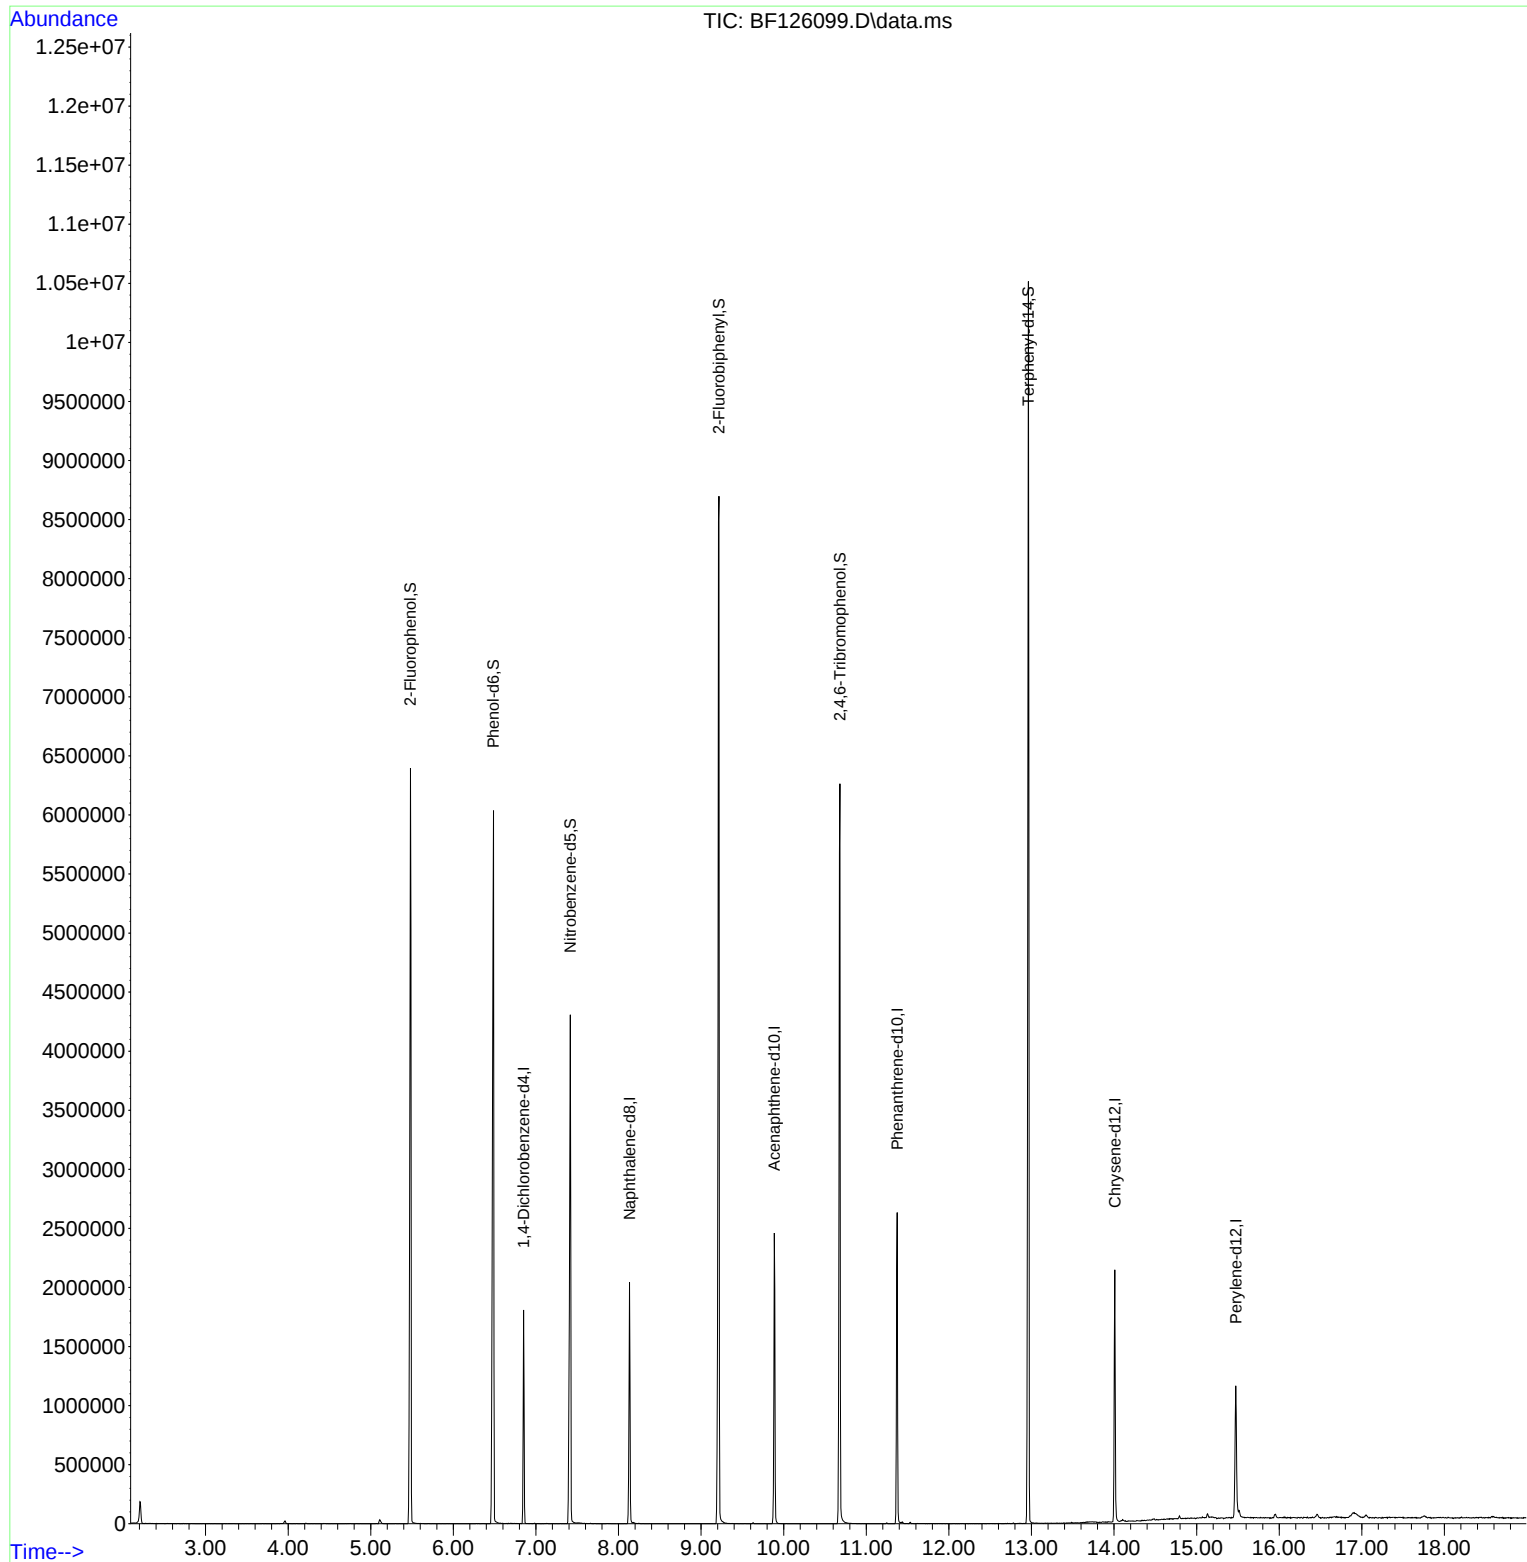




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.851 min Scan# 811
Delta R.T. -0.006 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15




Instrument :
BNA_F
ClientSampleId :
PB140520BL


Tgt Ion:152 Resp: 225789
Ion Ratio Lower Upper
152 100
150 150.0 117.6 176.4
115 65.5 47.1 70.7

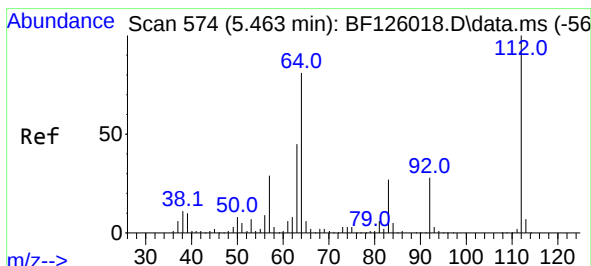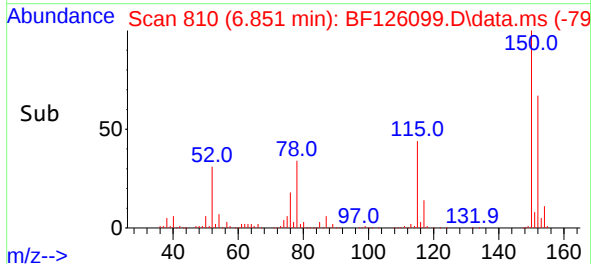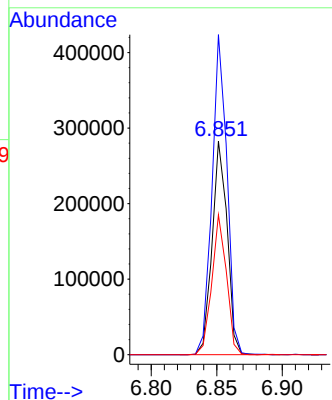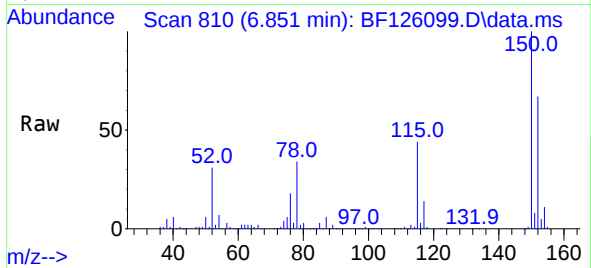

#5
2-Fluorophenol
Concen: 123.443 ng
RT: 5.481 min Scan# 577
Delta R.T. 0.018 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15

Tgt Ion:112 Resp: 1623038
Ion Ratio Lower Upper
112 100
64 73.6 44.2 66.2#
63 42.3 26.2 39.2#


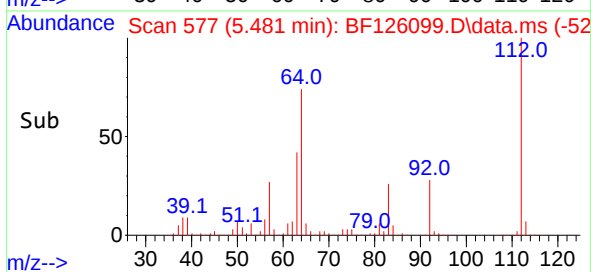
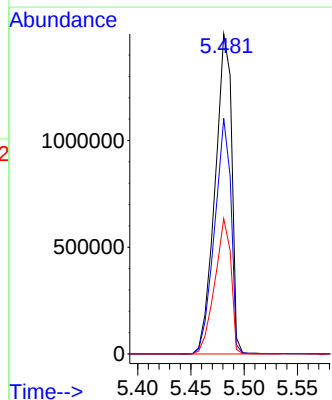
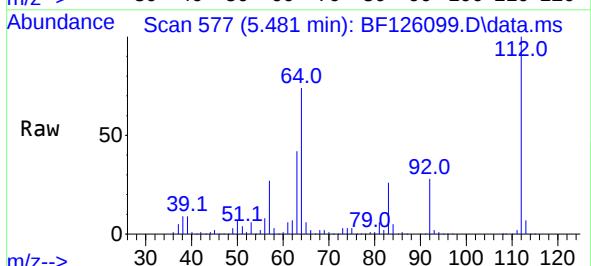


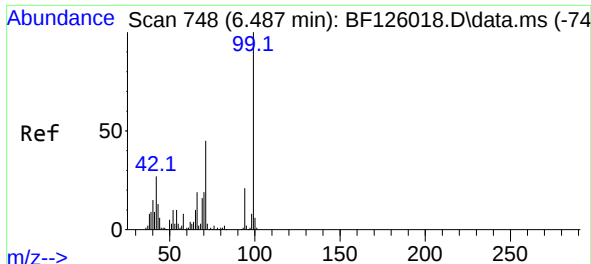

#7
Phenol-d6
Concen: 110.389 ng
RT: 6.487 min Scan# 74
Delta R.T. -0.000 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15




Instrument :
BNA_F
ClientSampleId :
PB140520BL


Tgt Ion: 99 Resp: 2045999
Ion Ratio Lower Upper
99 100
42 25.6 23.5 35.3
71 44.1 25.6 38.4#

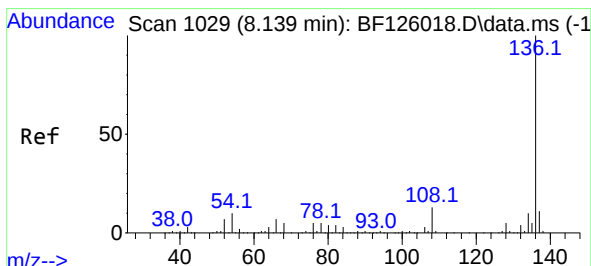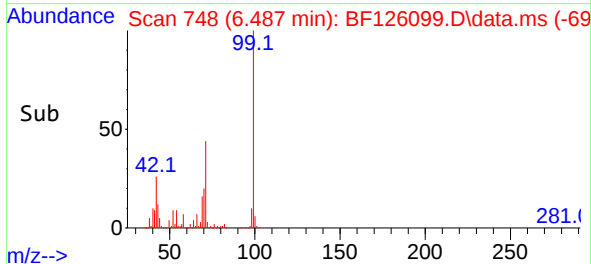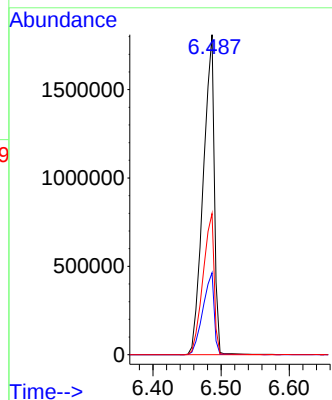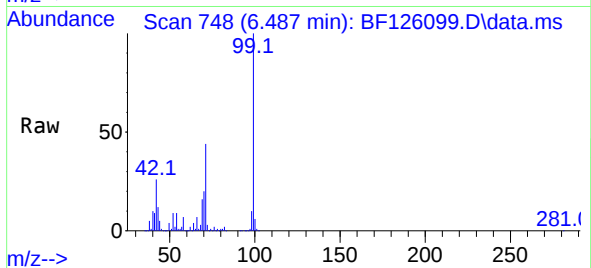

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.134 min Scan# 1028
Delta R.T. -0.005 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15

Tgt Ion:136 Resp: 840729
Ion Ratio Lower Upper
136 100
137 10.6 9.8 14.6
54 9.4 6.4 9.6
68 5.3 3.3 4.9#


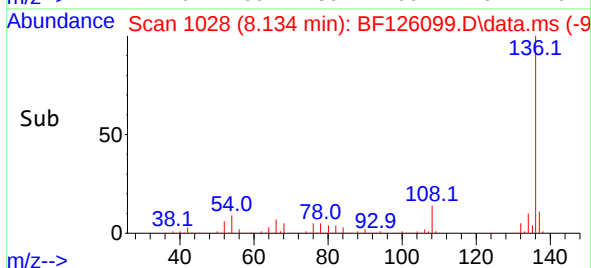
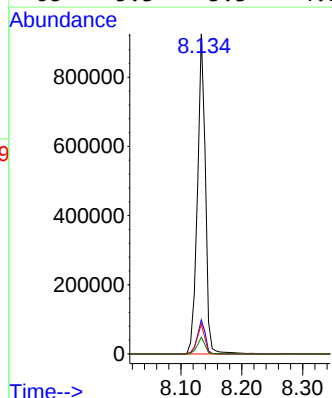
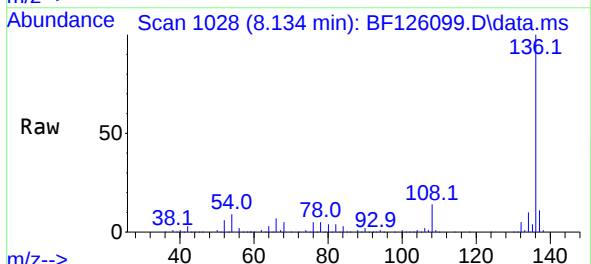


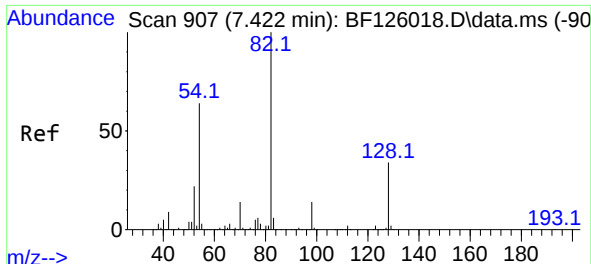

#23
Nitrobenzene-d5
Concen: 85.585 ng
RT: 7.416 min Scan# 907
Delta R.T. -0.006 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15




Instrument :
BNA_F
ClientSampleId :
PB140520BL


Tgt Ion: 82 Resp: 1525728
Ion Ratio Lower Upper
82 100
128 36.2 40.6 60.8#
54 59.6 49.6 74.4

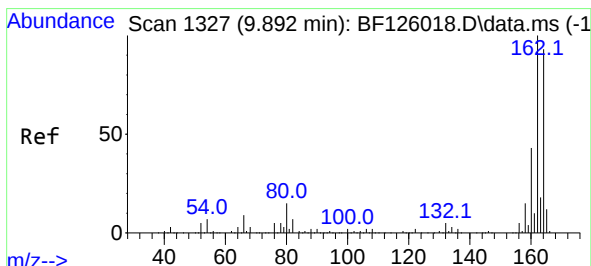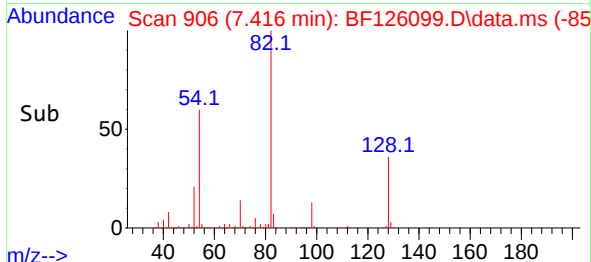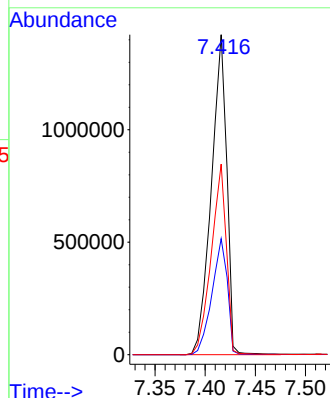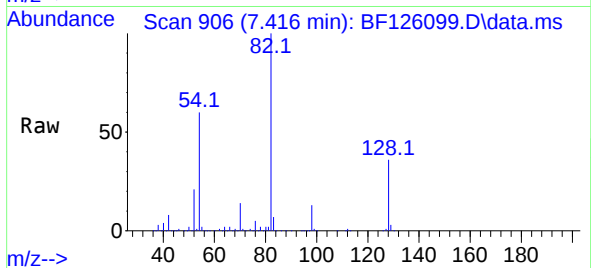

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.886 min Scan# 1326
Delta R.T. -0.006 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15


Tgt Ion:164 Resp: 508383
Ion Ratio Lower Upper
164 100
162 104.2 81.3 121.9
160 45.6 38.0 57.0

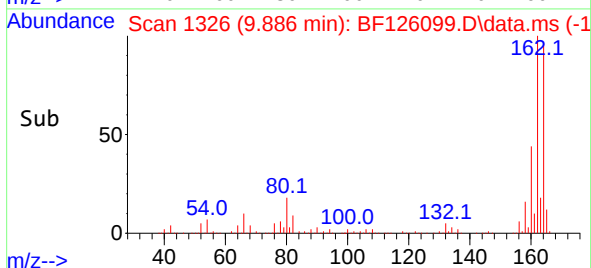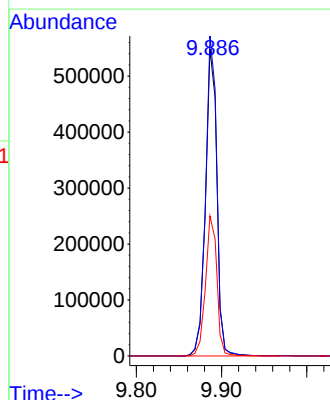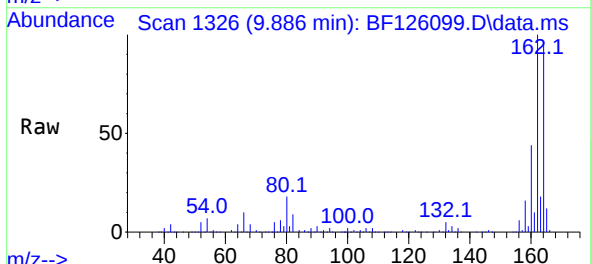



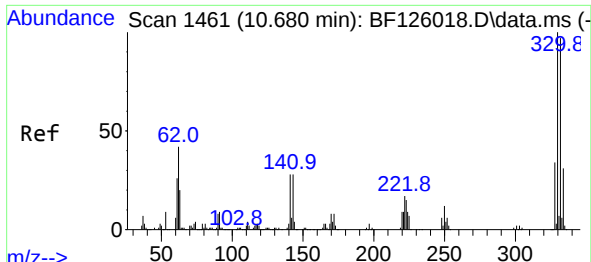


#42
2,4,6-Tribromophenol
Concen: 130.863 ng
RT: 10.680 min Scan# 1461
Delta R.T. -0.000 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15


Instrument :
BNA_F
ClientSampleId :
PB140520BL

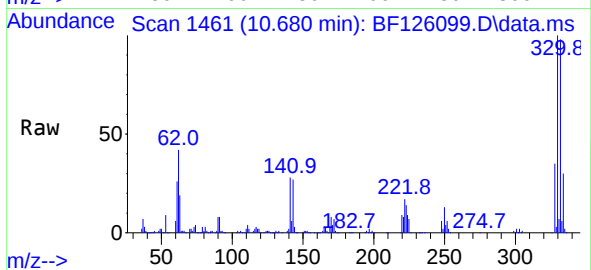



Tgt Ion: 330 Resp: 762420
Ion Ratio Lower Upper
330 100
332 97.1 76.2 114.4
141 35.2 44.6 66.8#

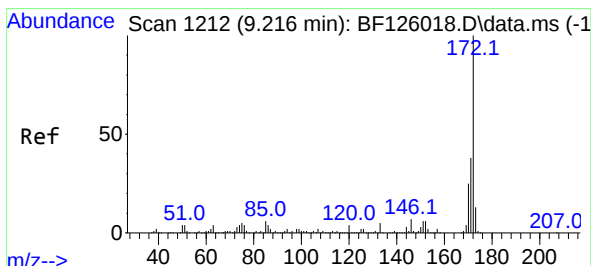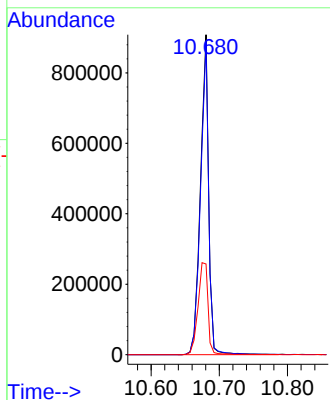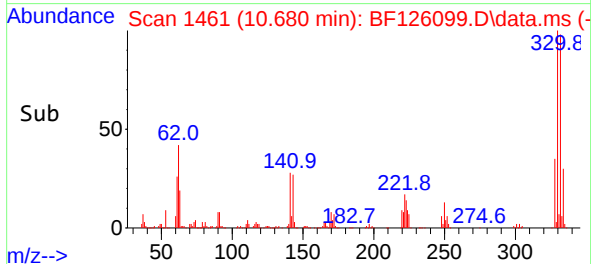

#45
2-Fluorobiphenyl
Concen: 76.872 ng
RT: 9.216 min Scan# 1212
Delta R.T. -0.000 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15

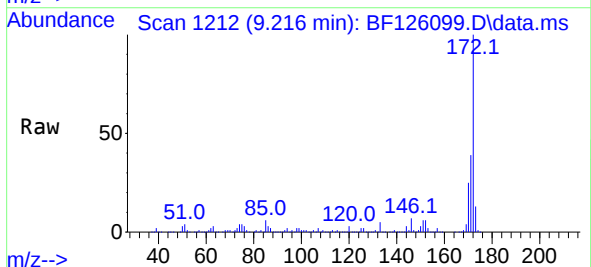

Tgt Ion: 172 Resp: 2891945
Ion Ratio Lower Upper
172 100
171 38.6 26.5 39.7
170 25.4 18.8 28.2



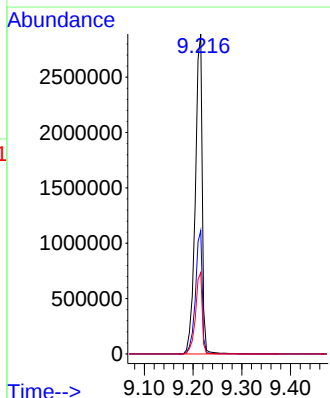
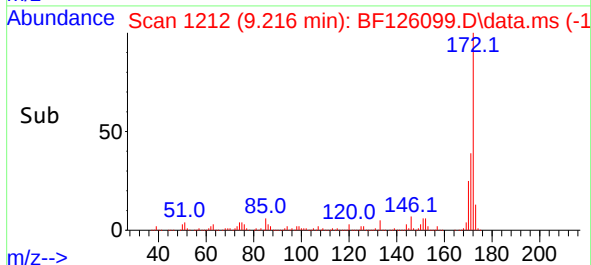




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.375 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15




Instrument :
BNA_F
ClientSampleId :
PB140520BL

Tgt Ion:188 Resp: 944668
Ion Ratio Lower Upper
188 100
94 6.7 6.7 10.1
80 7.8 7.5 11.3

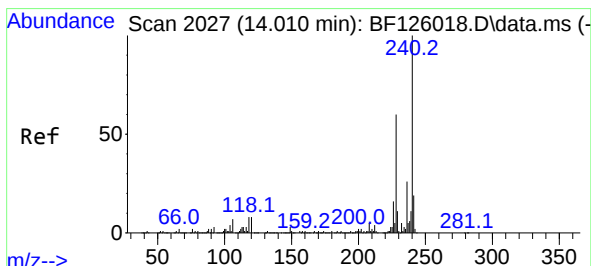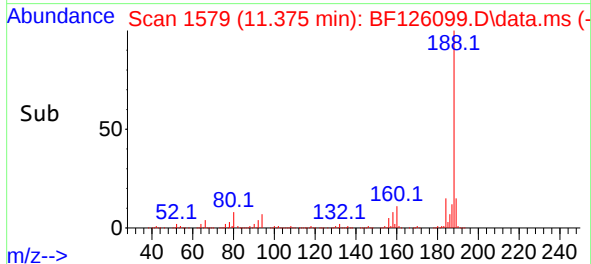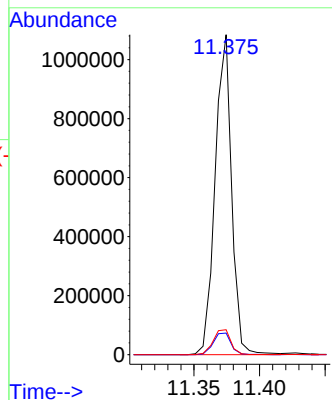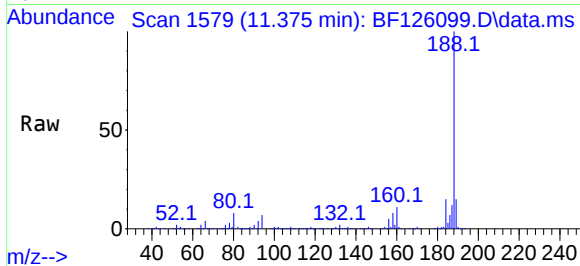

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.010 min Scan# 2027
Delta R.T. -0.000 min
Lab File: BF126099.D
Acq: 10 Nov 2021 10:15


Tgt Ion:240 Resp: 724873
Ion Ratio Lower Upper
240 100
120 7.2 10.8 16.2#
236 26.3 21.6 32.4

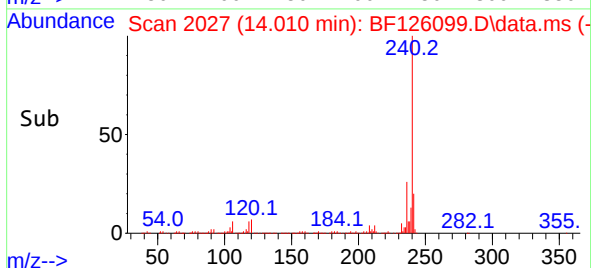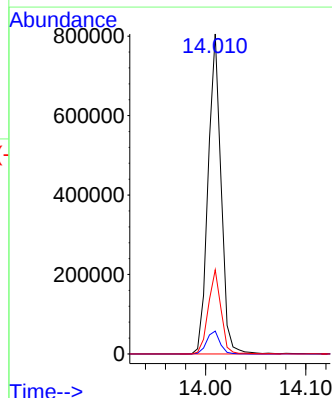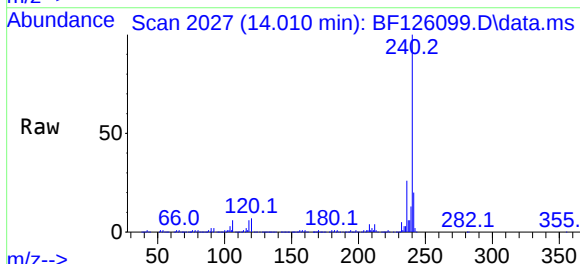






#79
 Terphenyl-d14
 Concen: 79.142 ng
 RT: 12.963 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BF126099.D
 Acq: 10 Nov 2021 10:15

Instrument :
 BNA_F
 ClientSampleId :
 PB140520BL

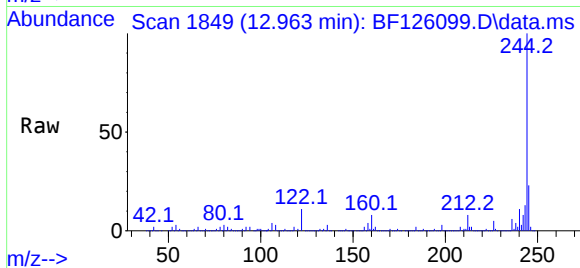

Tgt Ion:244 Resp: 3557611

Ion	Ratio	Lower	Upper
244	100		
212	8.3	5.9	8.9
122	11.0	9.0	13.4

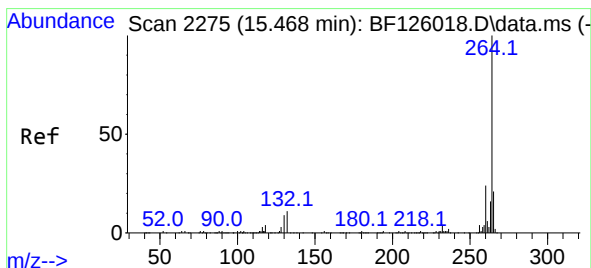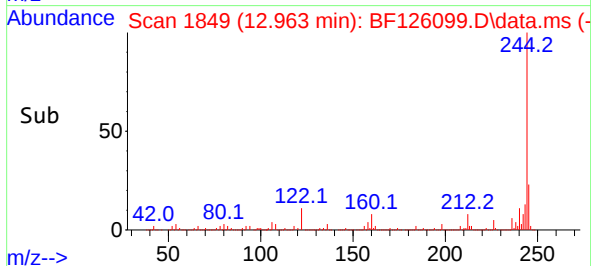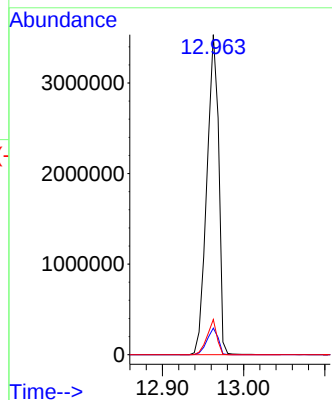

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.474 min Scan# 2276
 Delta R.T. 0.006 min
 Lab File: BF126099.D
 Acq: 10 Nov 2021 10:15

Tgt Ion:264 Resp: 554517

Ion	Ratio	Lower	Upper
264	100		
260	25.5	19.6	29.4
265	21.4	17.2	25.8

