


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111021\
 Data File : BF126097.D
 Acq On : 10 Nov 2021 9:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 03 17:21:25 2021

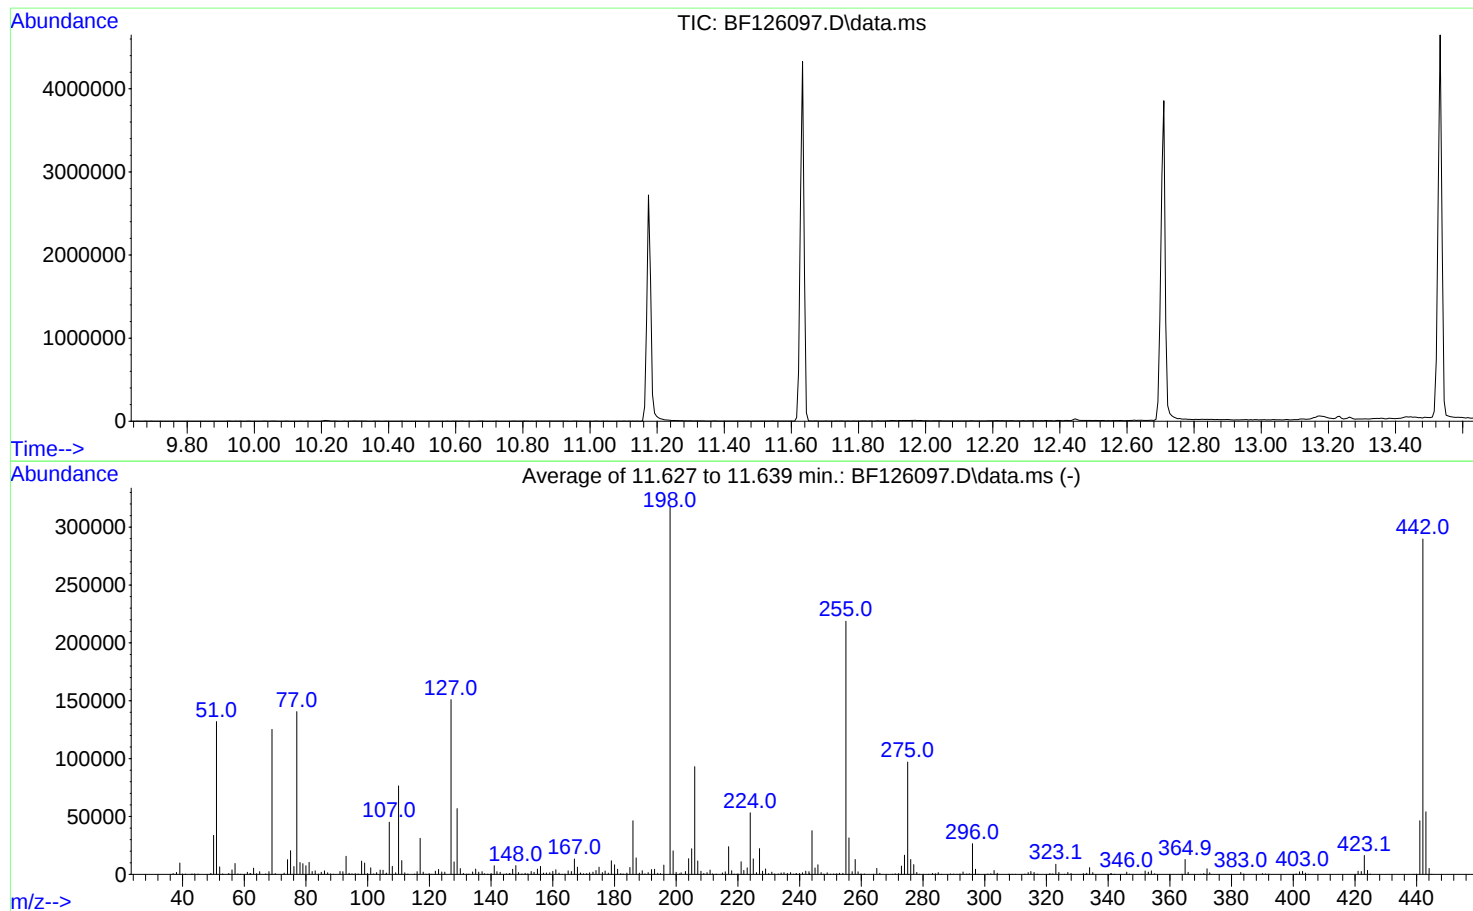




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	132043	PASS
68	69	0.00	2	1.9	2378	PASS
69	198	0.00	100	39.4	125216	PASS
70	69	0.00	2	0.5	684	PASS
127	198	10	80	47.5	150960	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	317824	PASS
199	198	5	9	6.4	20399	PASS
275	198	10	60	30.5	97080	PASS
365	198	1	100	4.1	12908	PASS
441	198	0.01	100	14.6	46341	PASS
442	442	50	100	100.0	289813	PASS
443	442	15	24	18.7	54107	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111021\
Data File : BF126097.D
Acq On : 10 Nov 2021 9:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 10 13:31:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

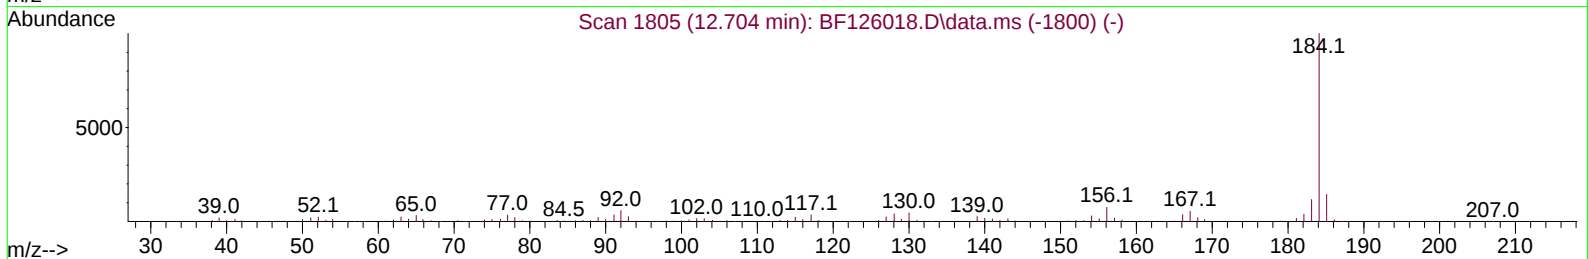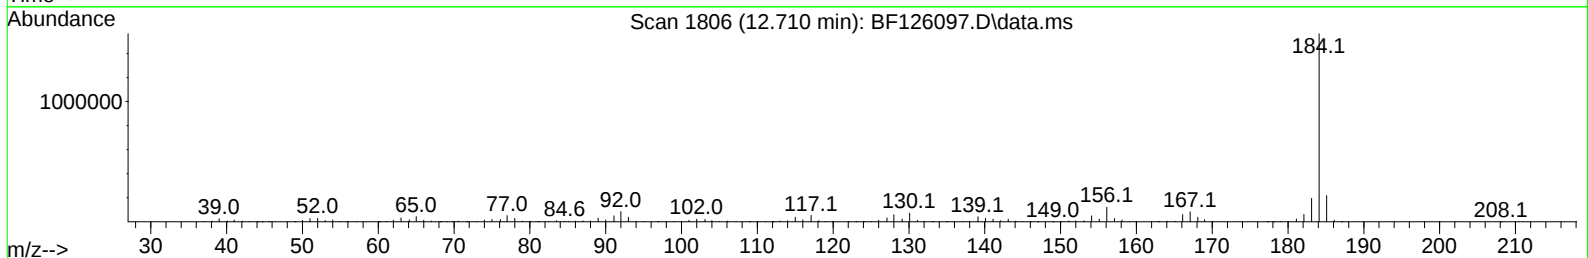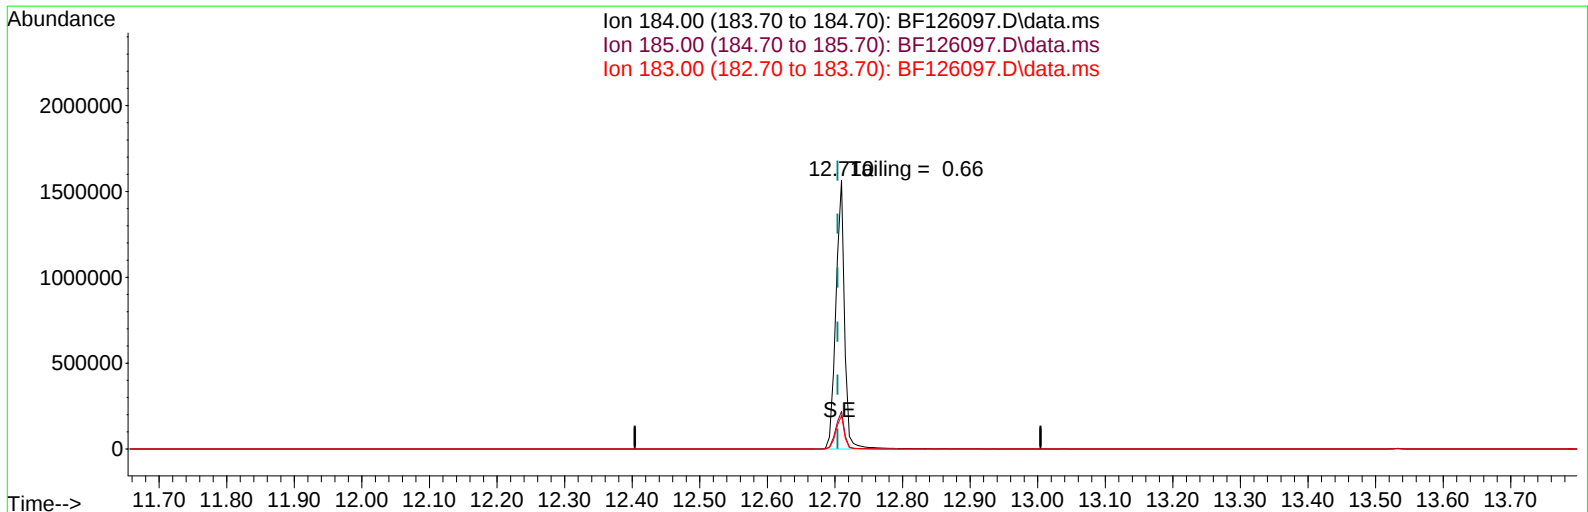

TIC: BF126097.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 350422.47 ng




response 1393997

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.01
183.00	10.10	12.48#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111021\
 Data File : BF126097.D
 Acq On : 10 Nov 2021 9:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 10 13:31:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 17:21:25 2021
 Response via : Initial Calibration

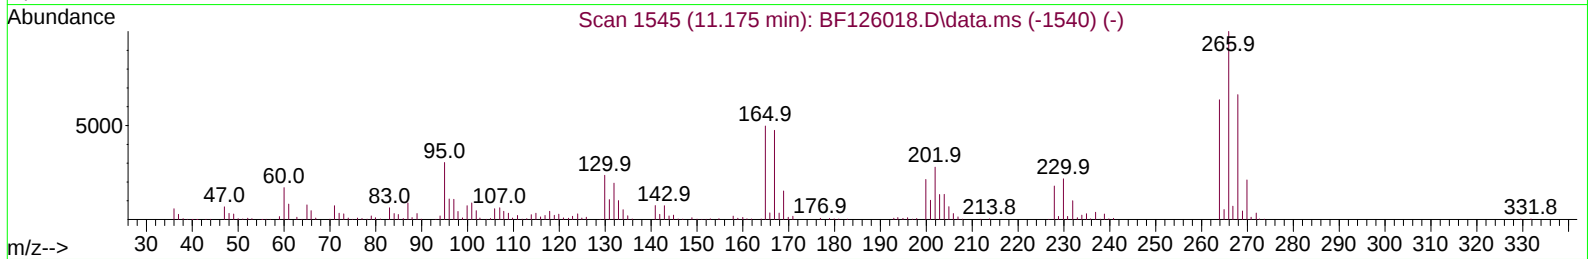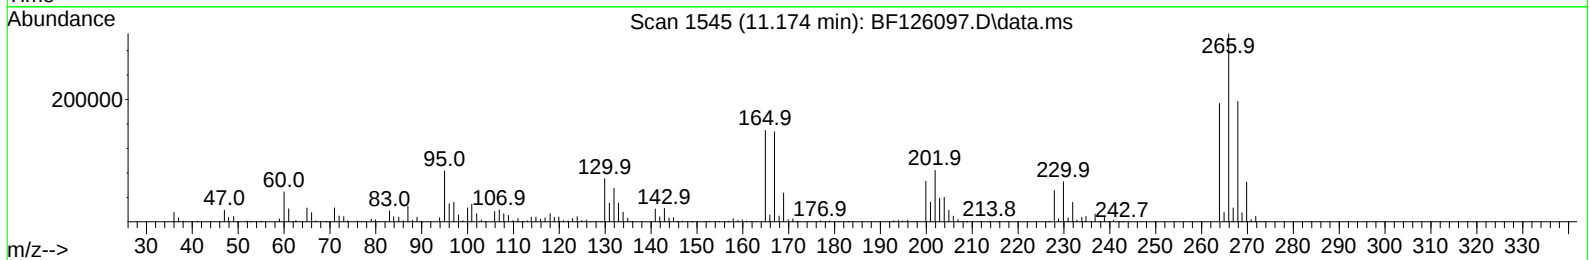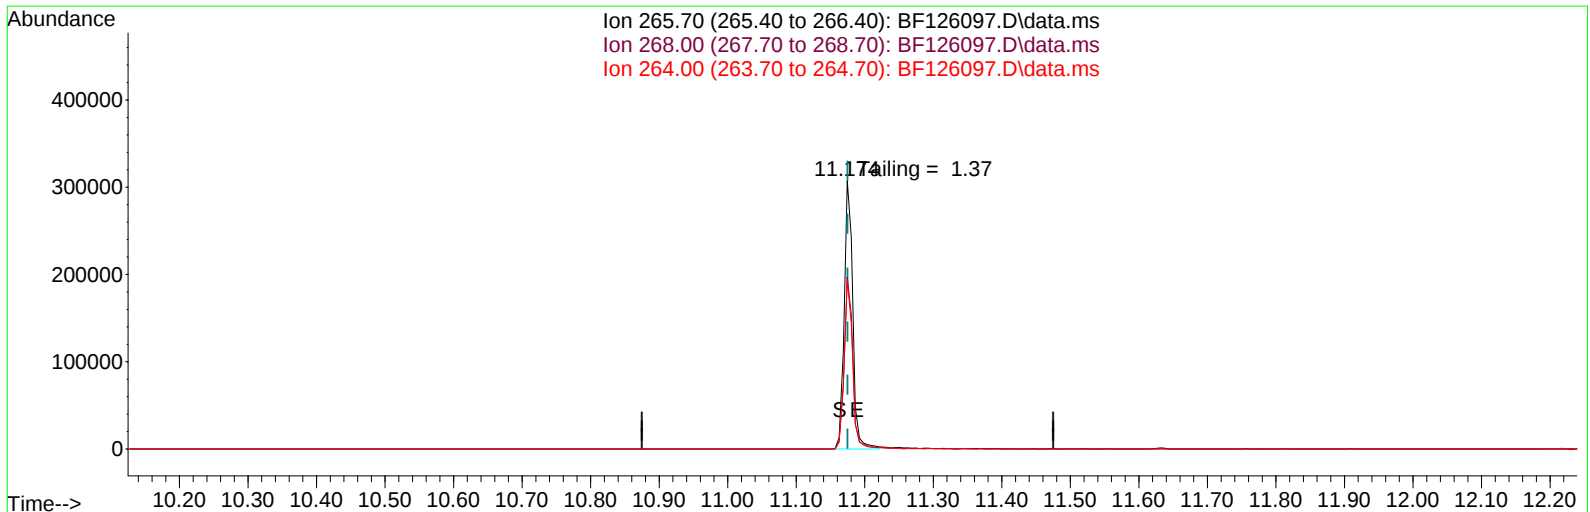

TIC: BF126097.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.001) 29802.36 ng

response 269232

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.04
264.00	69.90	62.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/10/2021	BNA_F	<u>BF126097.D</u>
Compound Name	Response	Retention Time
DDT	687816	13.53
DDD	7540	13.23
DDE	867	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8407	696223	1.21

Instrument :
BNA_F
ClientSampleId :
DFTPP