
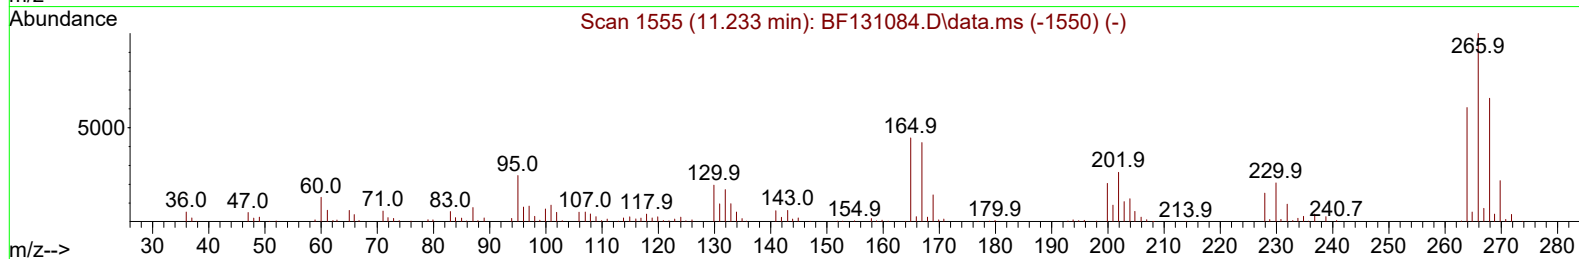
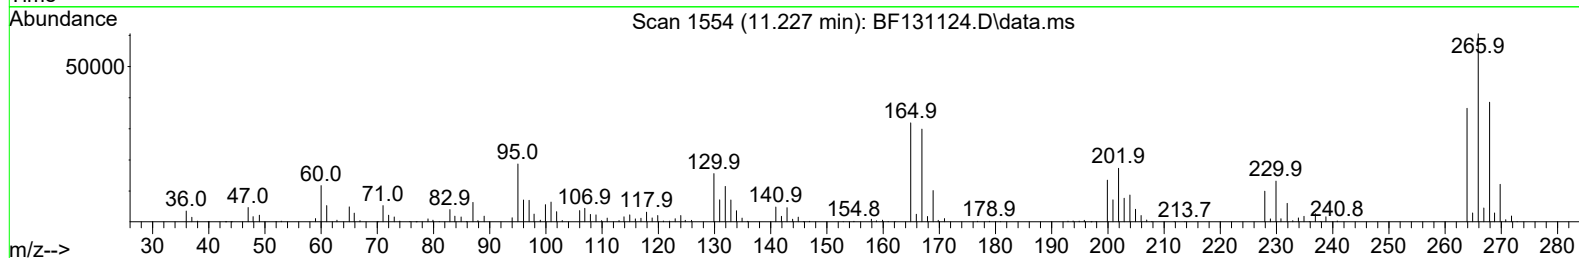


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111022\
Data File : BF131124.D
Acq On : 10 Nov 2022 15:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 04:49:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

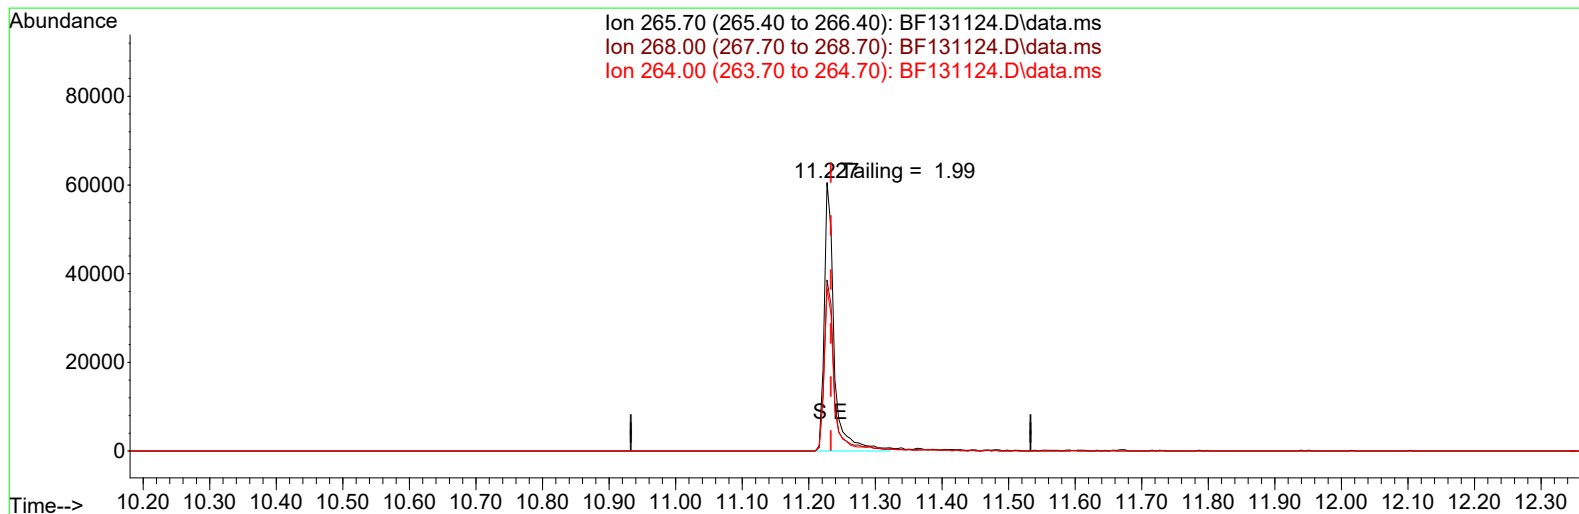




TIC: BF131124.D\data.ms

(70) Pentachlorophenol (C)**11.227min (-0.006) 33428.14 ng****response 62989**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	63.71
264.00	60.70	60.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111022\
Data File : BF131124.D
Acq On : 10 Nov 2022 15:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 04:49:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

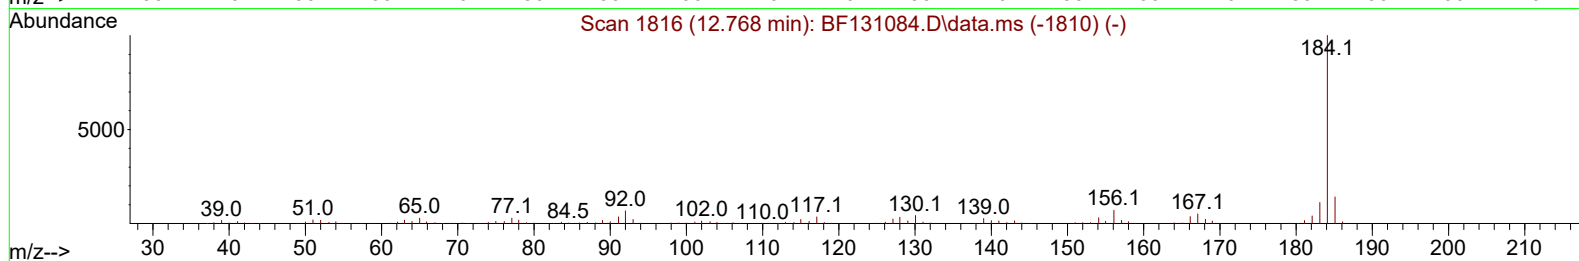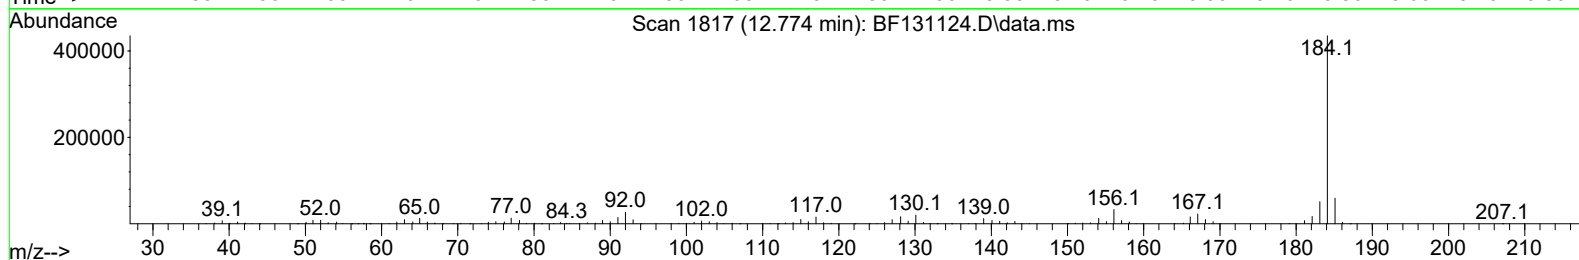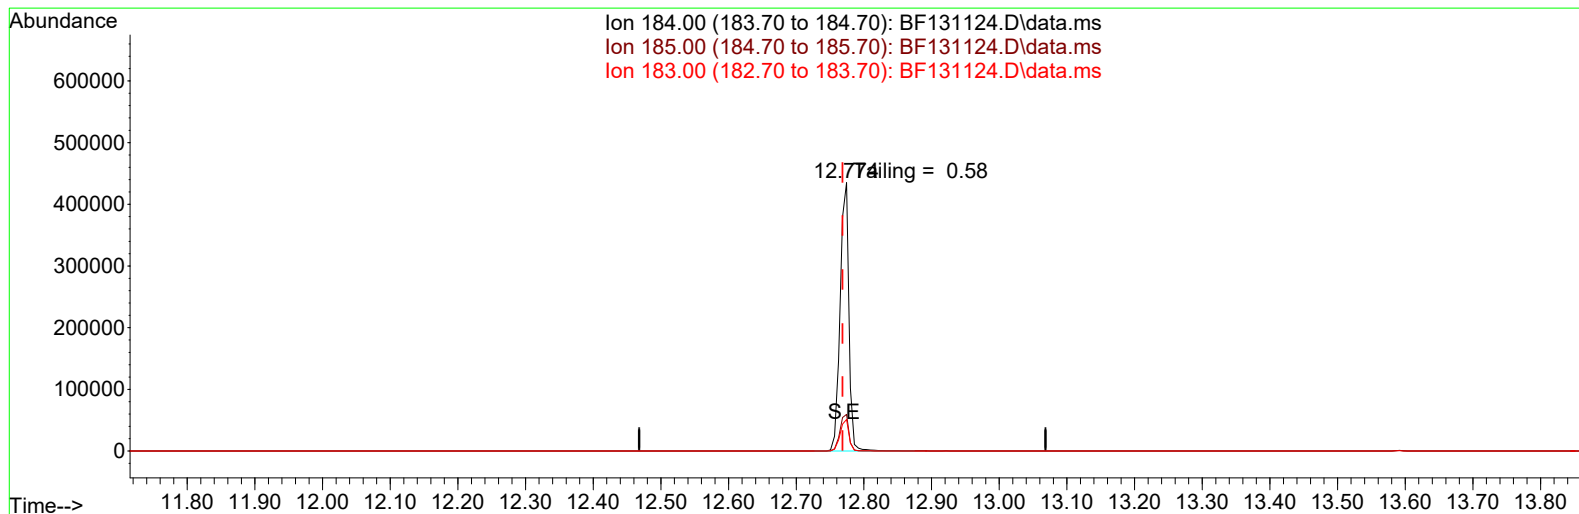

TIC: BF131124.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 394489

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.69
183.00	11.20	11.74
0.00	0.00	0.00