


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111022\
 Data File : BF131114.D
 Acq On : 10 Nov 2022 10:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 10 04:15:17 2022

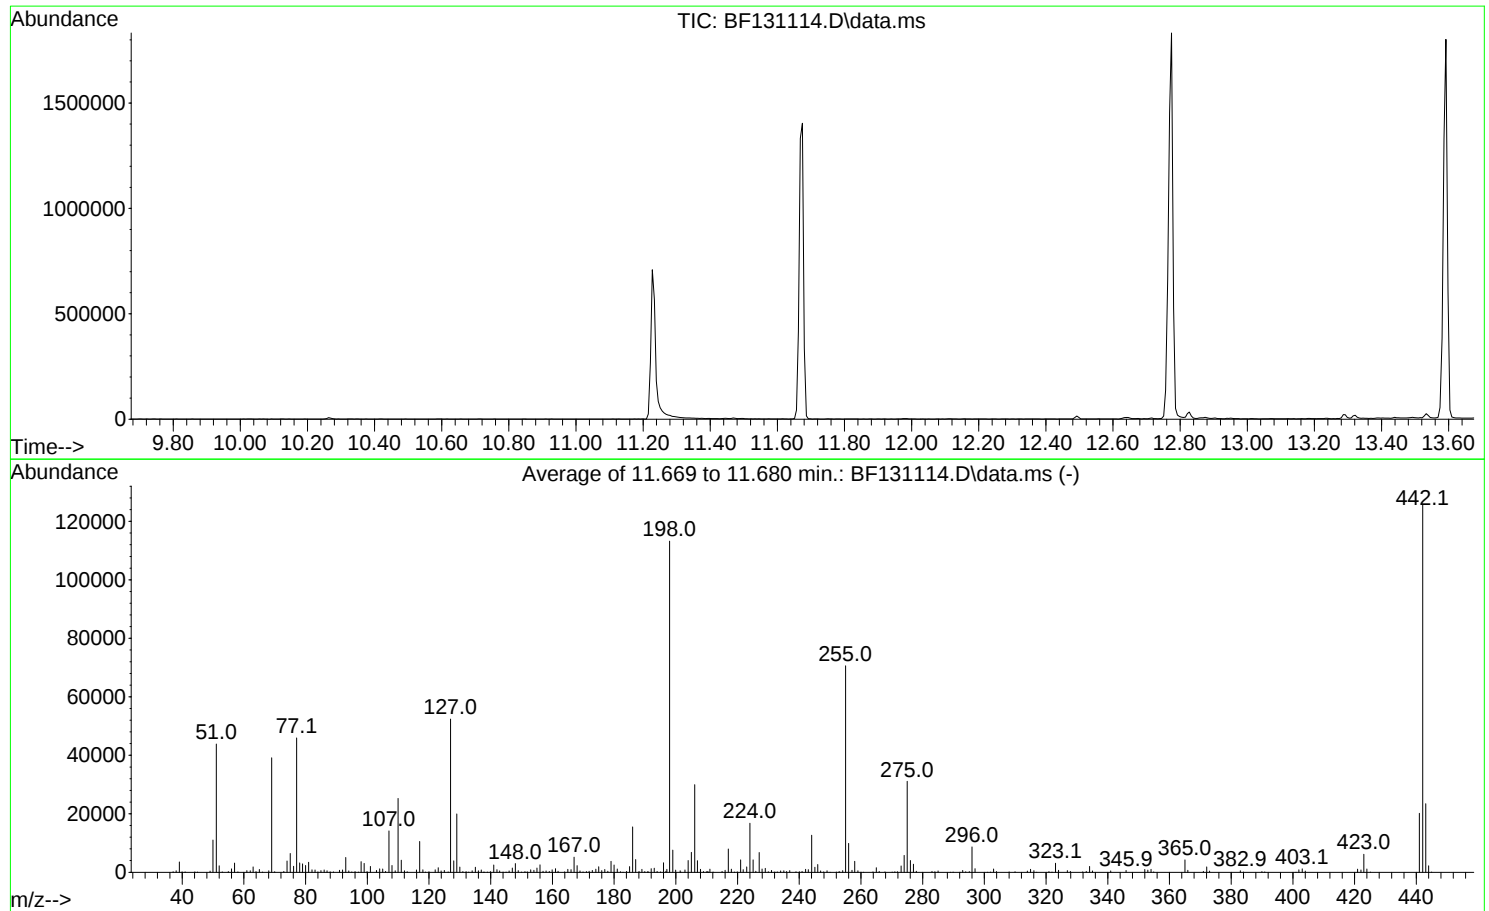




AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	43876	PASS
68	69	0.00	2	1.3	515	PASS
69	198	0.00	100	34.6	39145	PASS
70	69	0.00	2	0.5	198	PASS
127	198	10	80	46.3	52409	PASS
197	198	0.00	2	0.9	1011	PASS
198	198	100	100	100.0	113240	PASS
199	198	5	9	6.7	7591	PASS
275	198	10	60	27.5	31105	PASS
365	198	1	100	3.7	4216	PASS
441	198	0.01	100	17.8	20176	PASS
442	442	50	100	100.0	125787	PASS
443	442	15	24	18.6	23425	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111022\
Data File : BF131114.D
Acq On : 10 Nov 2022 10:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 11 04:47:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

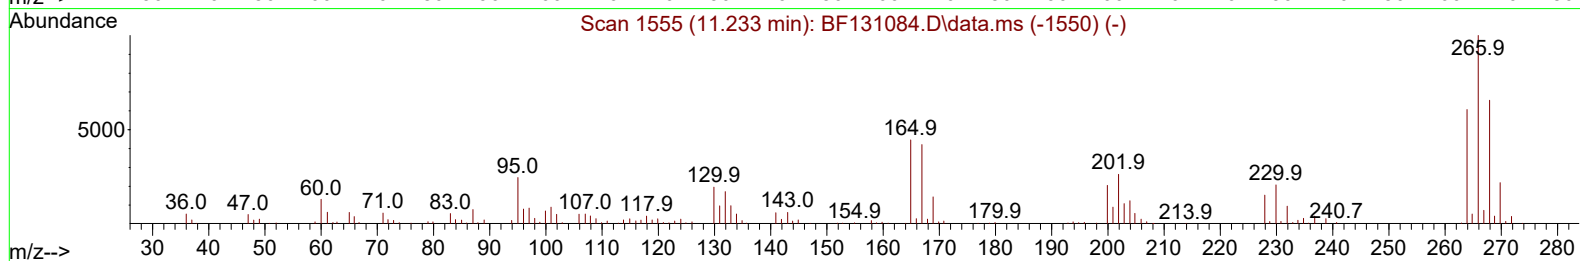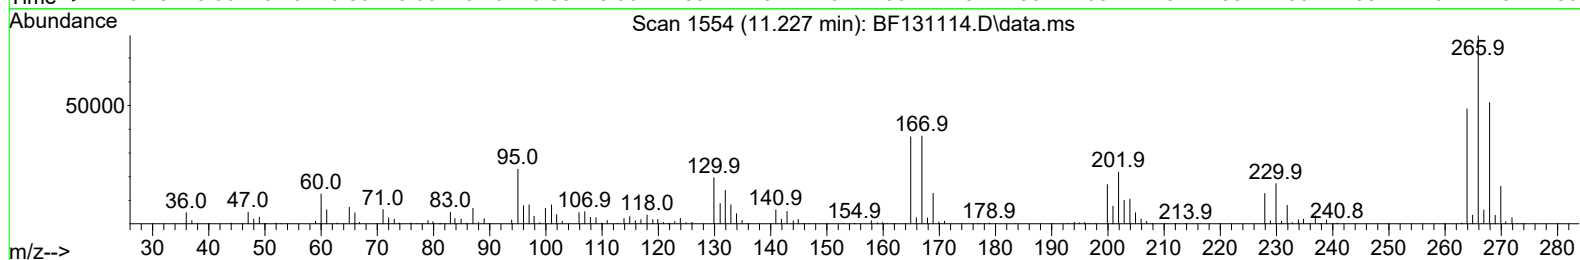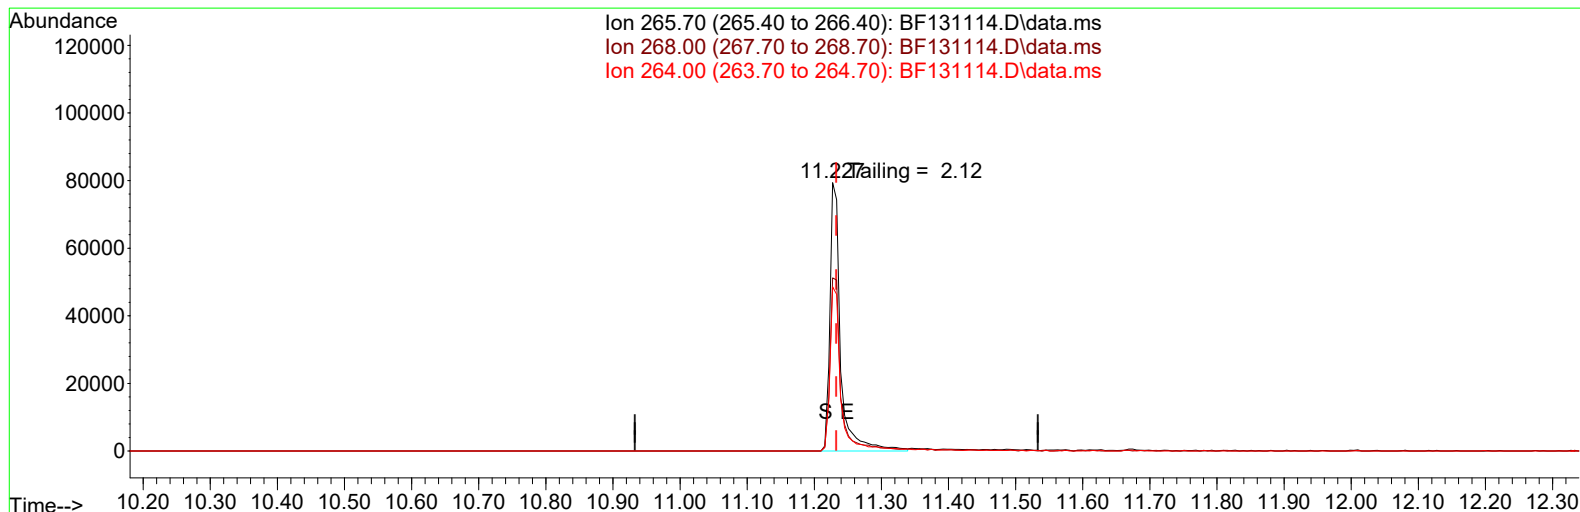

TIC: BF131114.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 31869.64 ng




response 87988

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	64.51
264.00	60.70	61.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111022\
Data File : BF131114.D
Acq On : 10 Nov 2022 10:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 11 04:47:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

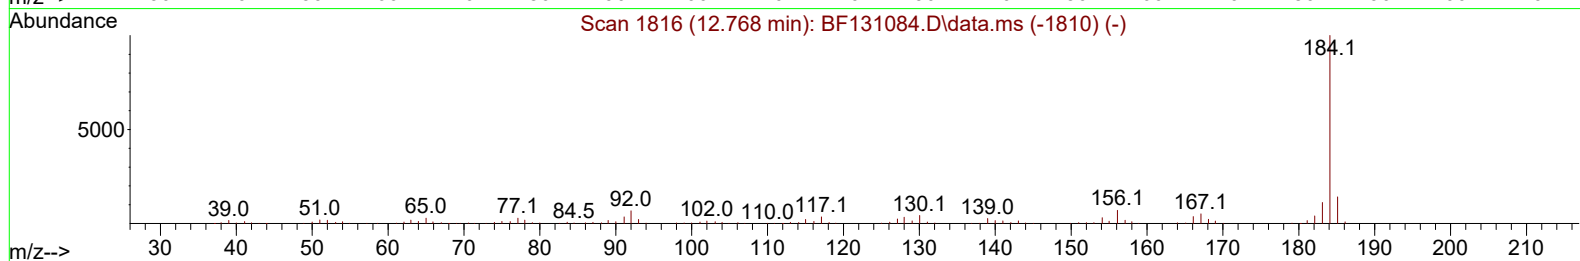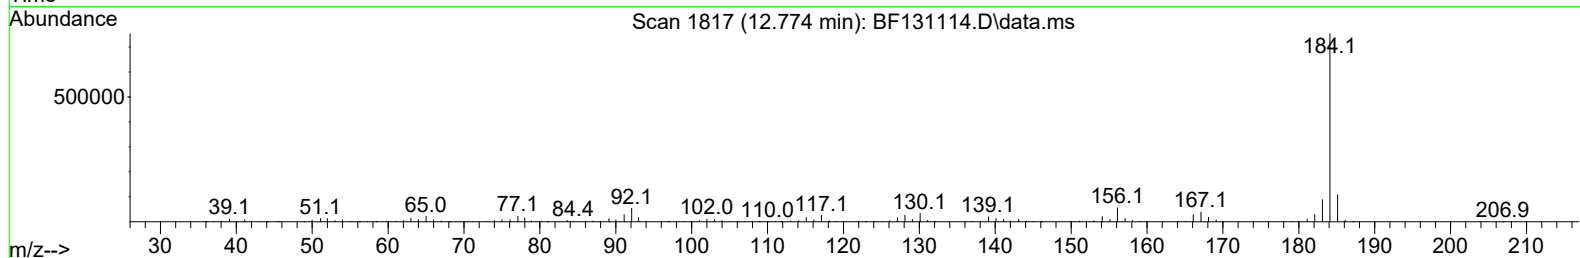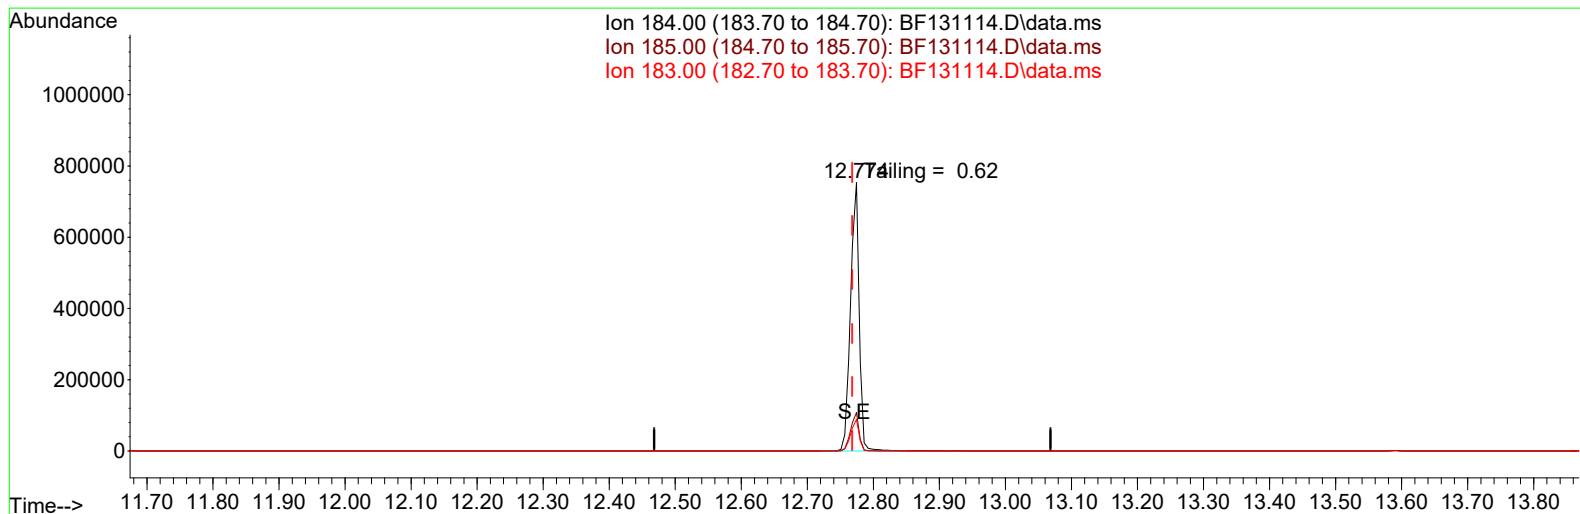

TIC: BF131114.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 687585

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.35
183.00	11.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/10/2022	BNA_F	<u>BF131114.D</u>
Compound Name	Response	Retention Time
DDT	294175	13.592
DDD	7012	13.292
DDE	550	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7562	301737	2.51

Instrument :
BNA_F
ClientSampleId :
DFTPP