


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111022\  
 Data File : BF131124.D  
 Acq On : 10 Nov 2022 15:45  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110922.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Nov 10 04:15:17 2022

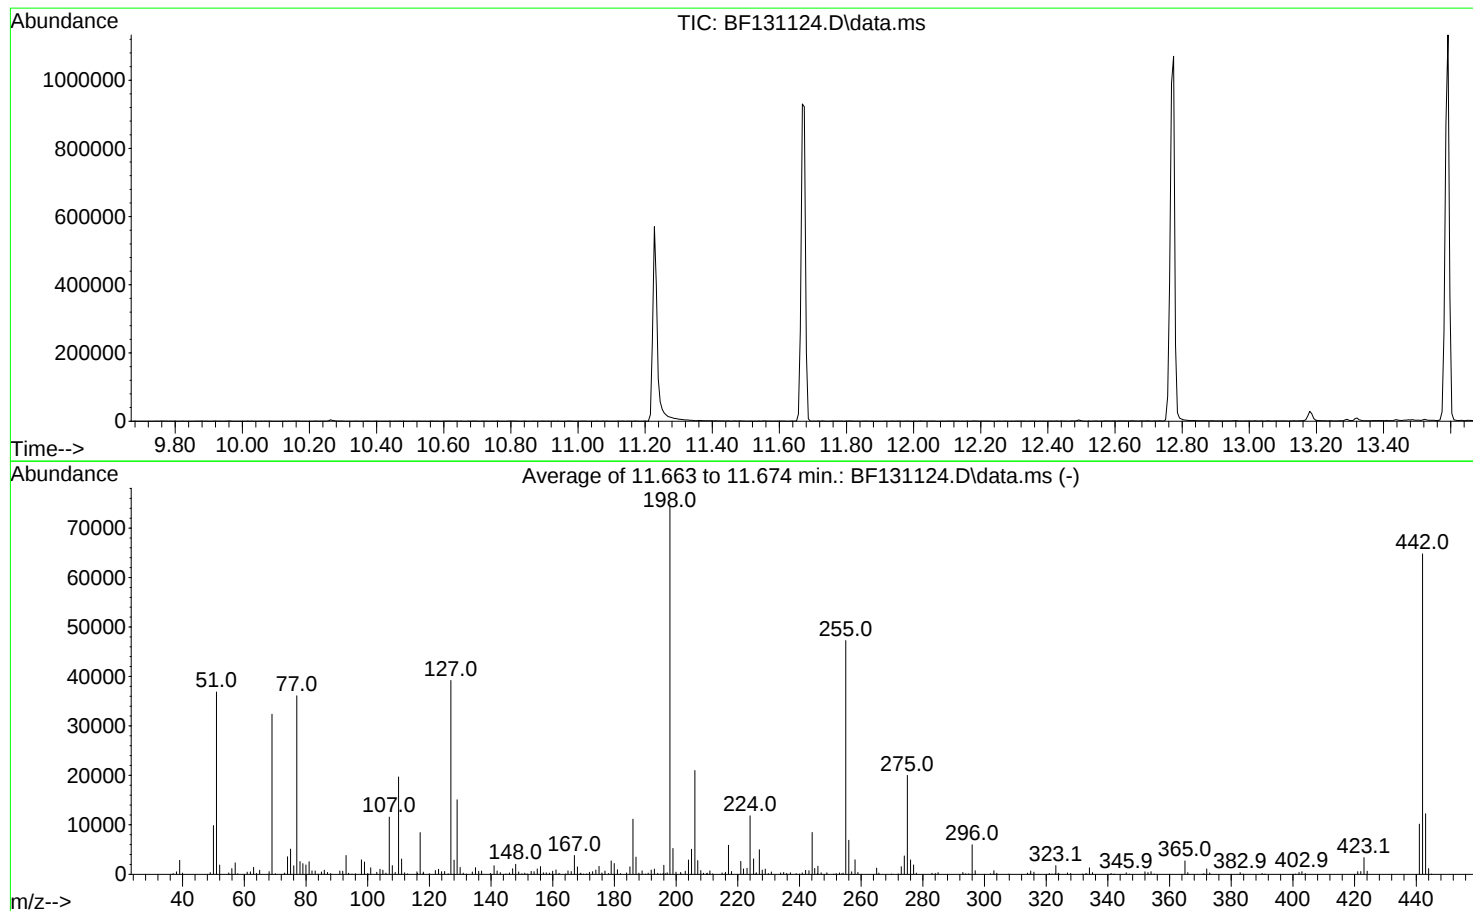




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1624

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 49.6         | 36861      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 540        | PASS                |
| 69             | 198             | 0.00            | 100             | 43.5         | 32368      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 123        | PASS                |
| 127            | 198             | 10              | 80              | 52.7         | 39200      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 327        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 74379      | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 5239       | PASS                |
| 275            | 198             | 10              | 60              | 26.9         | 20026      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 2694       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.7         | 10153      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 64781      | PASS                |
| 443            | 442             | 15              | 24              | 18.9         | 12260      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111022\  
Data File : BF131124.D  
Acq On : 10 Nov 2022 15:45  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 11 04:49:07 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 10 04:15:17 2022  
Response via : Initial Calibration

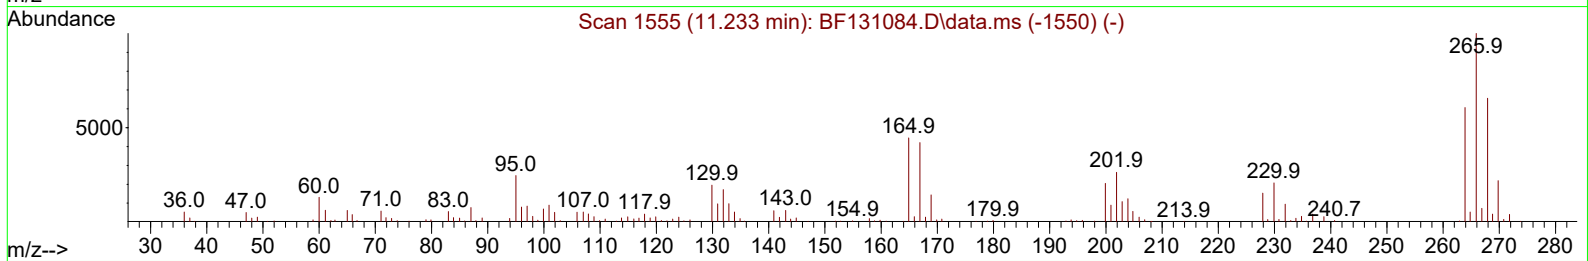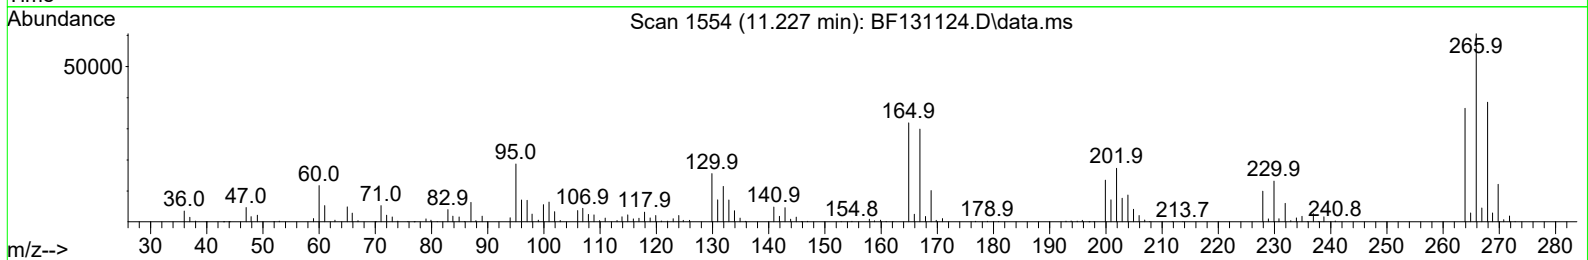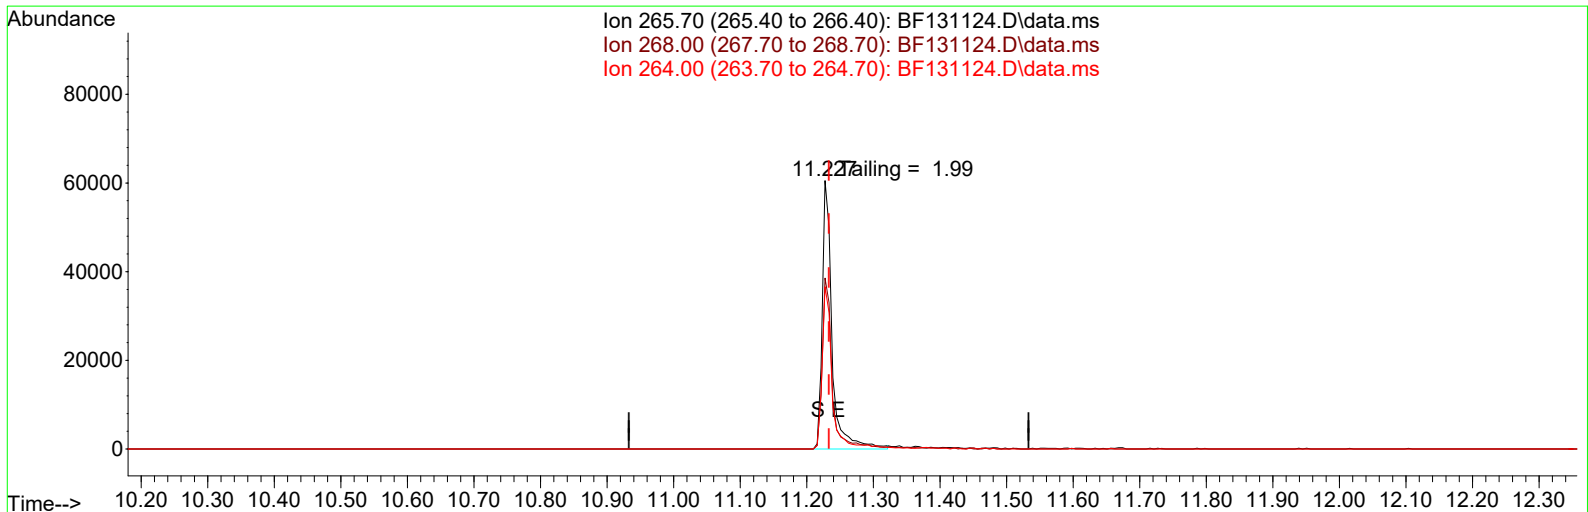

TIC: BF131124.D\data.ms

**(70) Pentachlorophenol (C)**

**11.227min (-0.006) 33428.14 ng**




**response 62989**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.60  | 63.71  |
| 264.00 | 60.70  | 60.43  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111022\  
Data File : BF131124.D  
Acq On : 10 Nov 2022 15:45  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 11 04:49:07 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF110922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 10 04:15:17 2022  
Response via : Initial Calibration

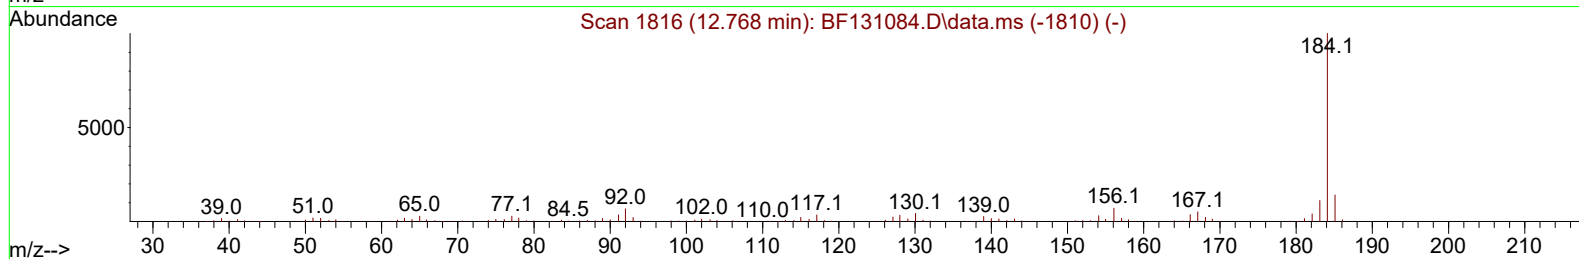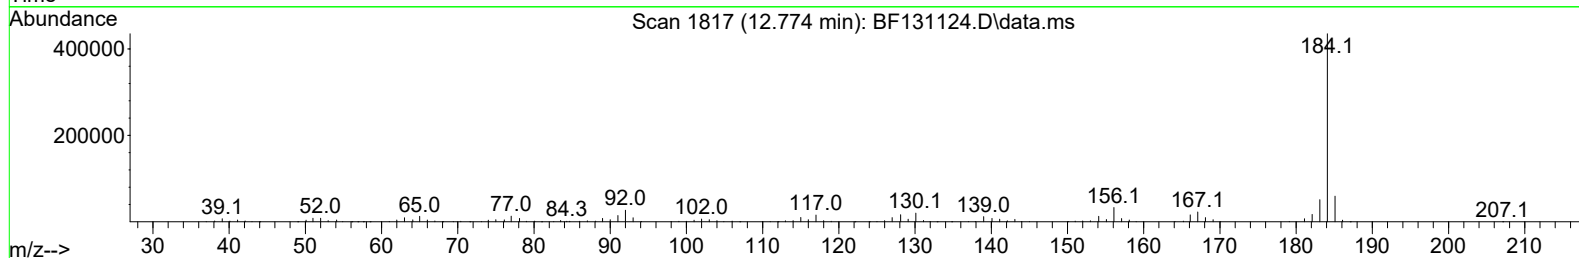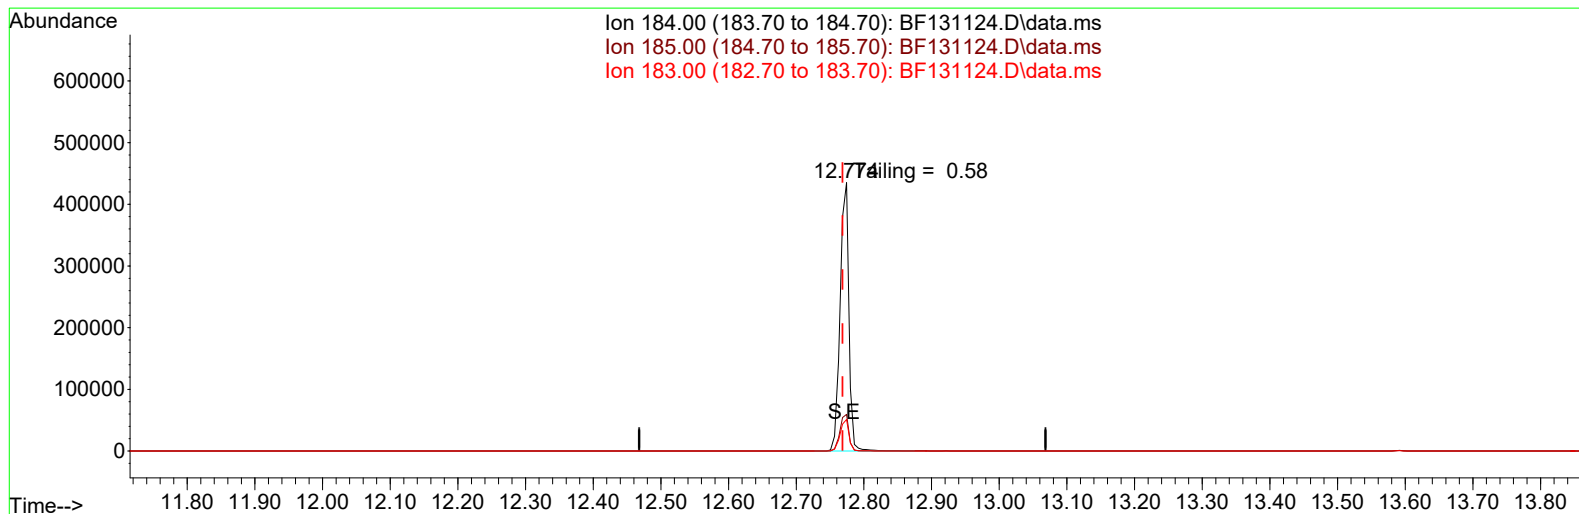

TIC: BF131124.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 394489

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 13.69  |
| 183.00 | 11.20  | 11.74  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/10/2022    | BNA_F            | <u>BF131124.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 182080           | 13.592             |
| DDD           | 2850             | 13.321             |
| DDE           | 103              | 12.957             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 2953          | 185033           | 1.60               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP