

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111116\
 Data File : BF091139.D
 Acq On : 11 Nov 2016 14:49
 Operator : UM/SJ
 Sample : PB94644BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB94644BL

Quant Time: Nov 11 15:55:11 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 12:59:29 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.65	152	147610	20.00	ng	-0.01
21) Naphthalene-d8	7.93	136	643331	20.00	ng	-0.02
38) Acenaphthene-d10	9.68	164	320913	20.00	ng	-0.02
63) Phenanthrene-d10	11.15	188	555430	20.00	ng	-0.02
75) Chrysene-d12	13.78	240	533003	20.00	ng	-0.03
86) Perylene-d12	15.15	264	481021	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	718061	80.34	ng	0.00
7) Phenol-d6	6.29	99	988570	81.49	ng	-0.02
23) Nitrobenzene-d5	7.21	82	1007474	85.43	ng	-0.03
41) 2,4,6-Tribromophenol	10.46	330	218081	75.17	ng	-0.02
44) 2-Fluorobiphenyl	9.01	172	1749180	93.84	ng	-0.02
78) Terphenyl-d14	12.74	244	1763941	82.59	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111116\
Data File : BF091139.D
Acq On : 11 Nov 2016 14:49
Operator : UM/SJ
Sample : PB94644BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94644BL

Quant Time: Nov 11 15:55:11 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

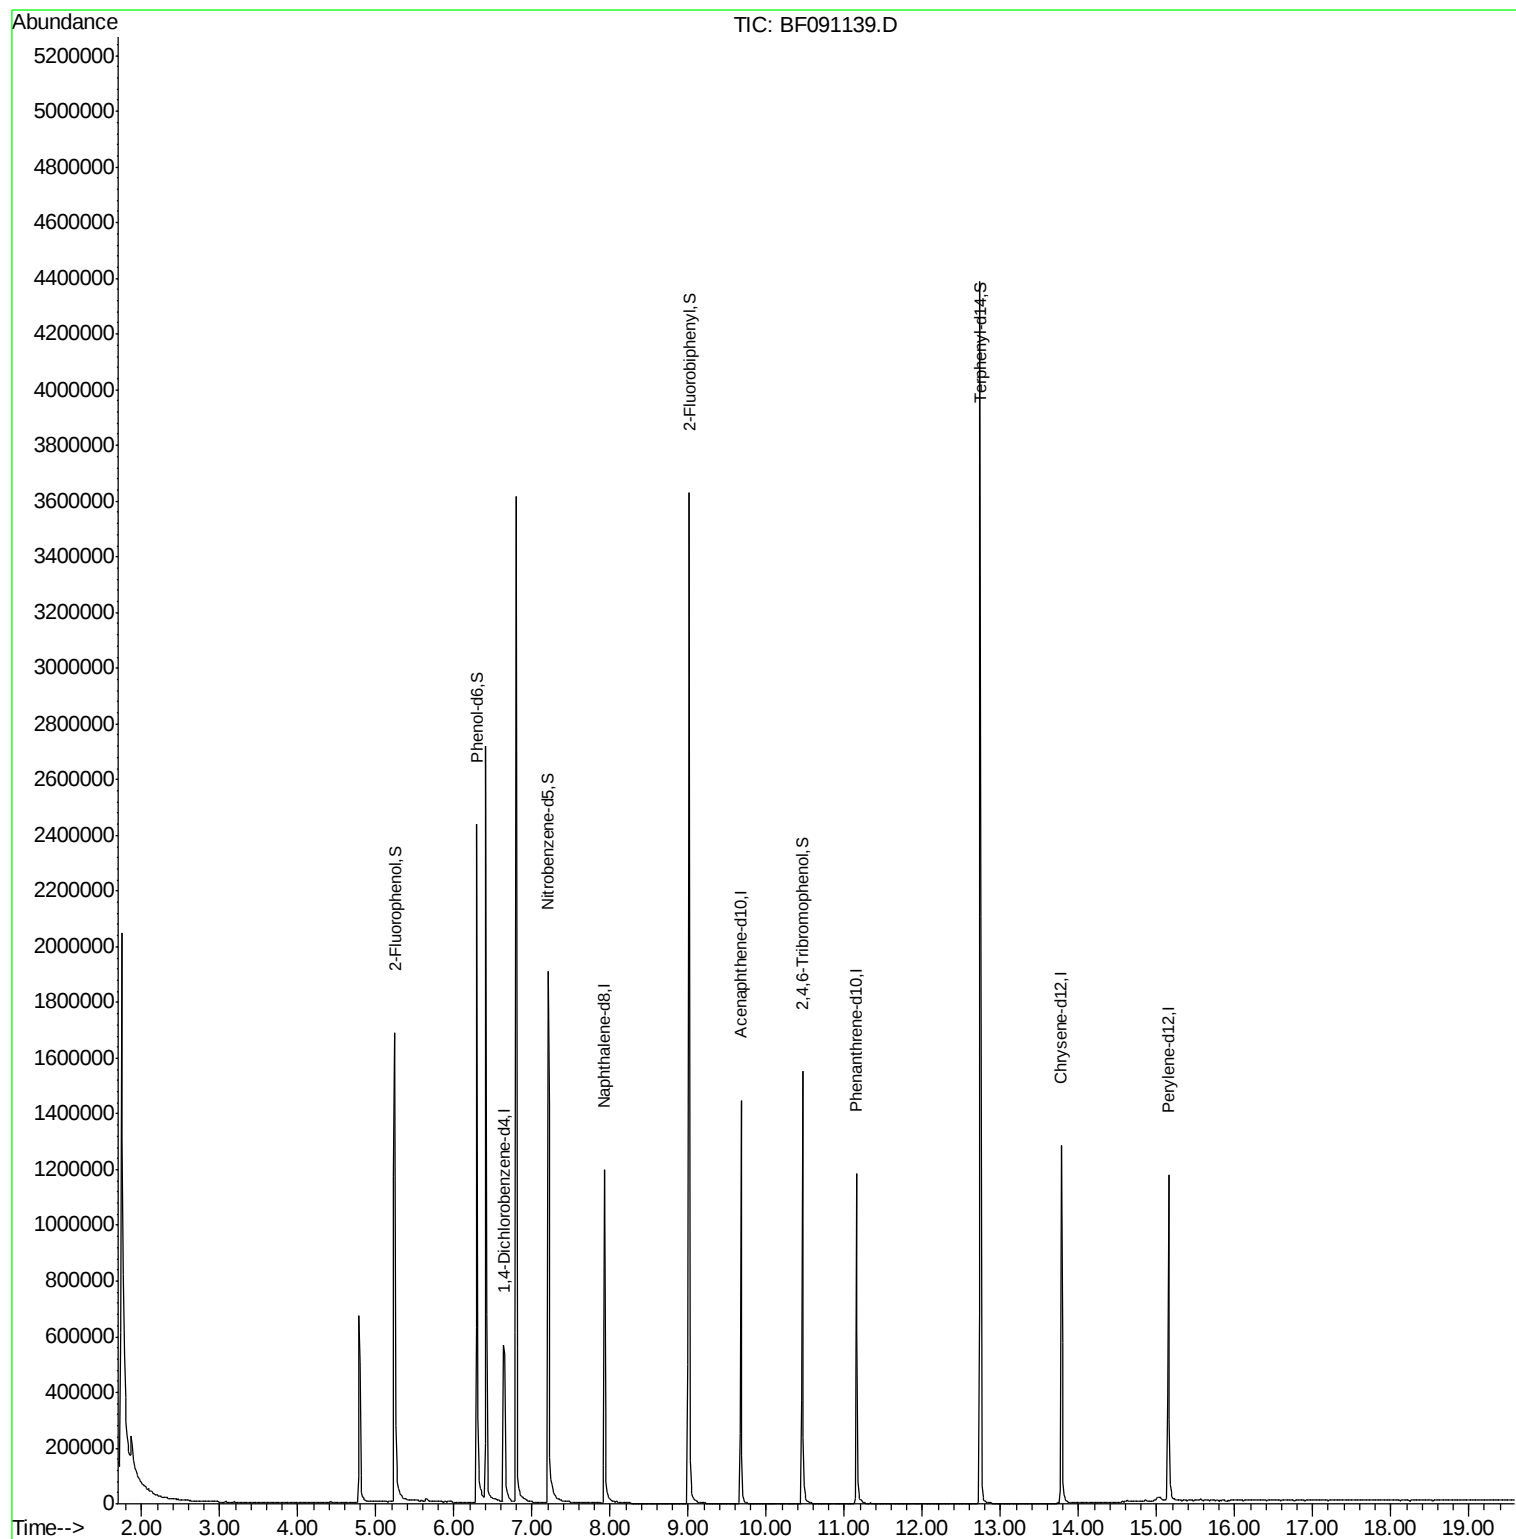

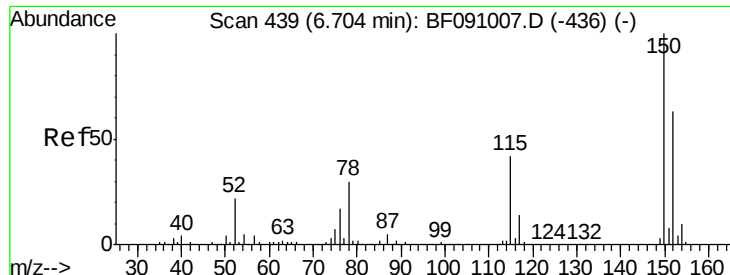


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.65 min Scan# 434
Delta R.T. -0.01 min
Lab File: BF091139.D
Acq: 11 Nov 2016 14:49

Instrument :
BNA_F
ClientSampleId :
PB94644BL

Tot Ion:152 Resp: 147610
Ion Ratio Lower Upper
152 100
150 153.6 126.8 190.2
115 58.0 53.3 79.9

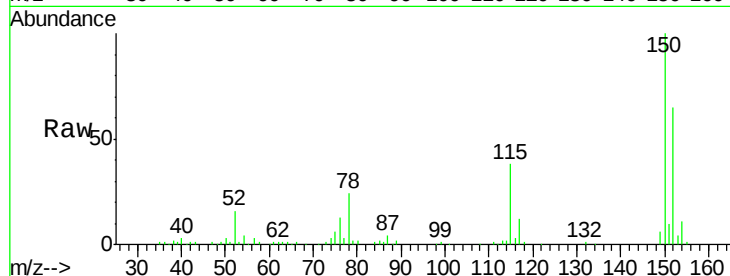


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

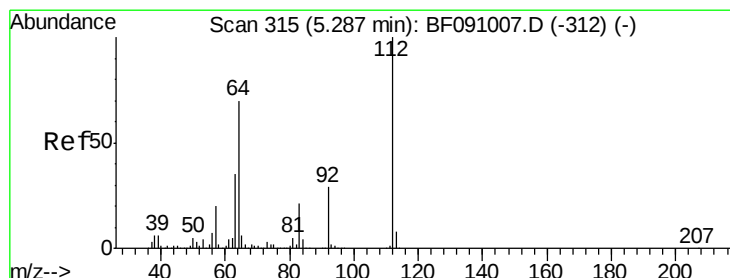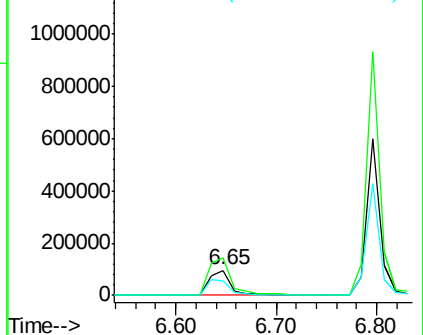



#5


2-Fluorophenol
Concen: 80.34 ng
RT: 5.24 min Scan# 311
Delta R.T. -0.00 min
Lab File: BF091139.D
Acq: 11 Nov 2016 14:49

Tgt Ion:112 Resp: 718061
Ion Ratio Lower Upper
112 100
64 54.5 55.8 83.6#
63 27.2 28.0 42.0#

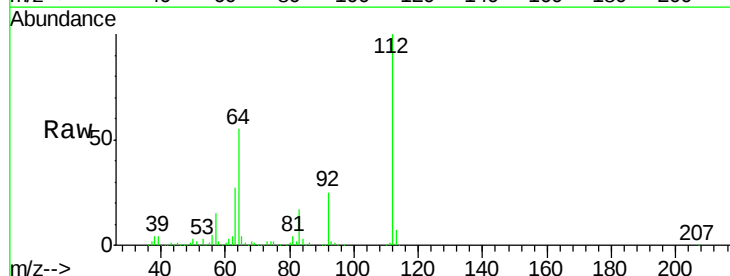

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

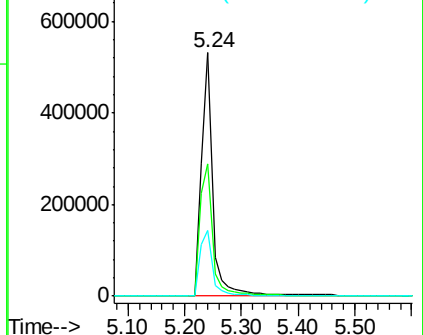



#7

Phenol-d6

Concen: 81.49 ng

RT: 6.29 min Scan# 403

Delta R.T. -0.02 min

Lab File: BF091139.D

Acq: 11 Nov 2016 14:49

Instrument :

BNA_F

ClientSampleId :

PB94644BL


Tot Ion: 99 Resp: 988570

Ion Ratio Lower Upper

99 100

42 15.0 13.9 20.9




71 32.4 27.8 41.8

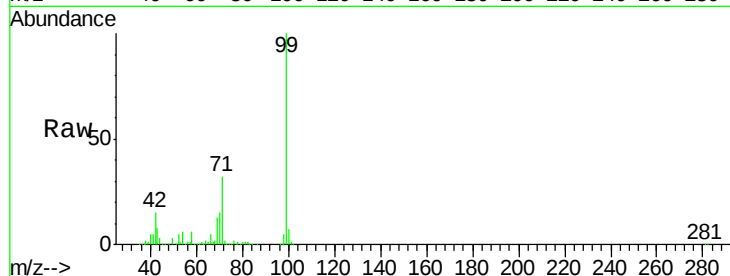

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

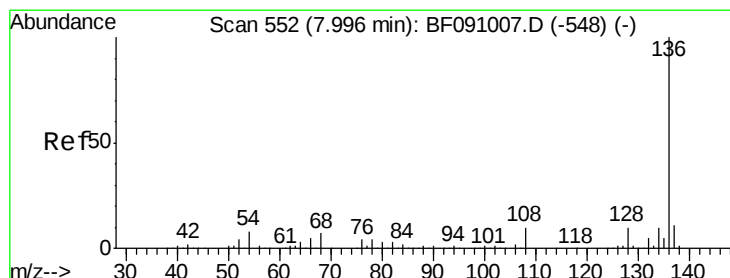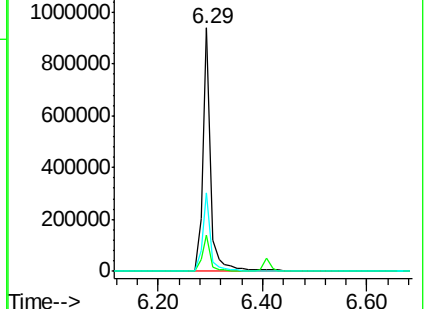

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.93 min Scan# 546

Delta R.T. -0.02 min

Lab File: BF091139.D

Acq: 11 Nov 2016 14:49

Tgt Ion: 136 Resp: 643331


Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 8.9 6.2 9.2

68 7.6 5.5 8.3


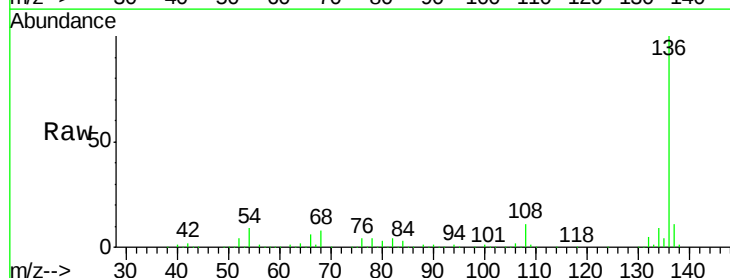



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0




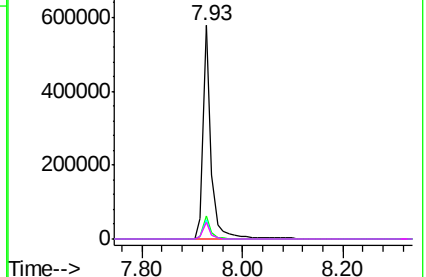




#23
 Nitrobenzene-d5
 Concen: 85.43 ng
 RT: 7.21 min Scan# 483
 Delta R.T. -0.03 min
 Lab File: BF091139.D
 Acq: 11 Nov 2016 14:49




Instrument :
 BNA_F
 ClientSampled :
 PB94644BL


Tot Ion: 82 Resp: 1007474
 Ion Ratio Lower Upper
 82 100
 128 37.7 32.4 48.6
 54 49.0 39.2 58.8

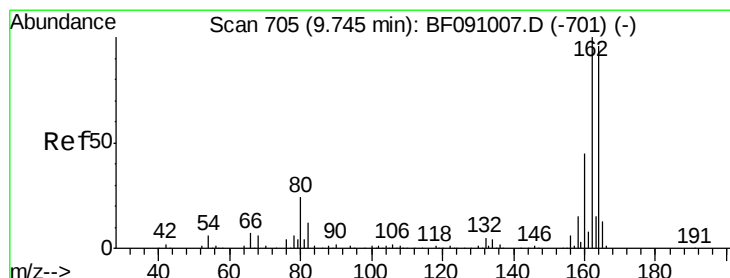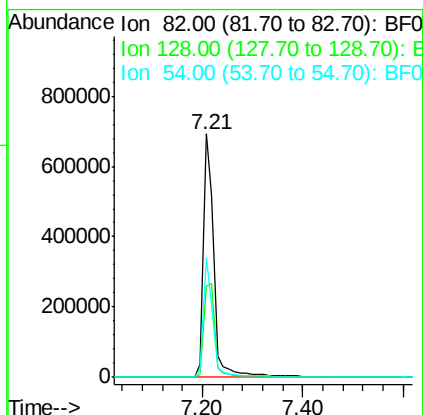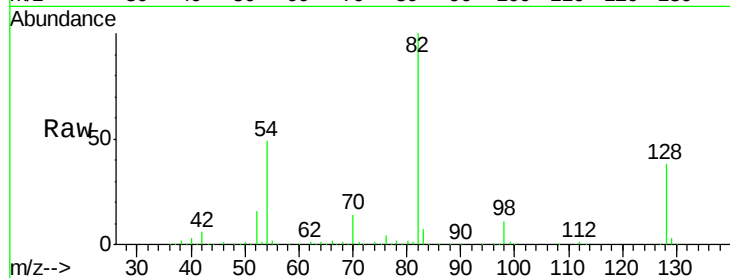

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.68 min Scan# 699
 Delta R.T. -0.02 min
 Lab File: BF091139.D
 Acq: 11 Nov 2016 14:49

Tgt Ion: 164 Resp: 320913
 Ion Ratio Lower Upper
 164 100
 162 104.2 83.6 125.4
 160 47.2 37.9 56.9

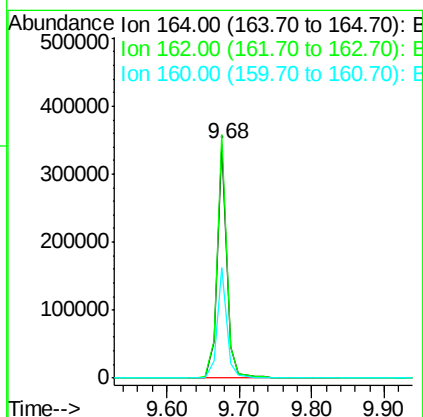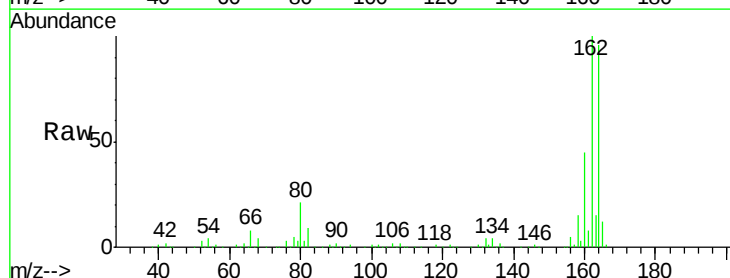


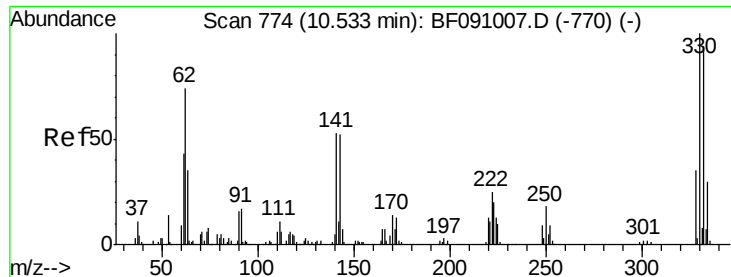




#41
 2,4,6-Tribromophenol
 Concen: 75.17 ng
 RT: 10.46 min Scan# 768
 Delta R.T. -0.02 min
 Lab File: BF091139.D
 Acq: 11 Nov 2016 14:49

Instrument :
 BNA_F
 ClientSampled :
 PB94644BL

Tot Ion:330 Resp: 218081
 Ion Ratio Lower Upper
 330 100
 332 97.5 75.9 113.9
 141 33.7 36.1 54.1#

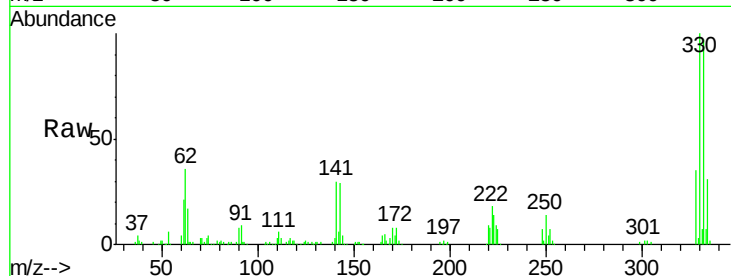


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

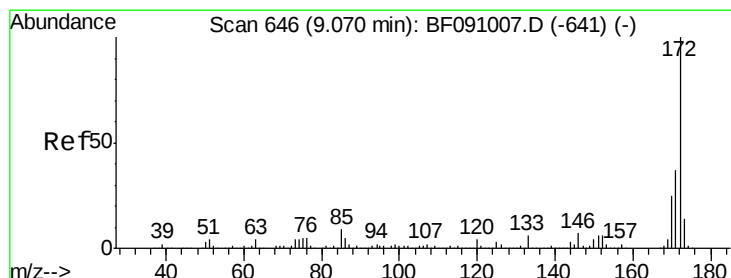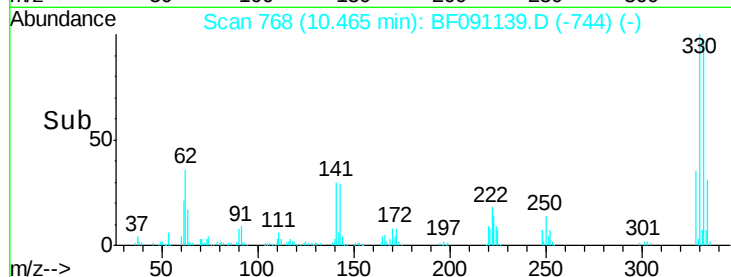
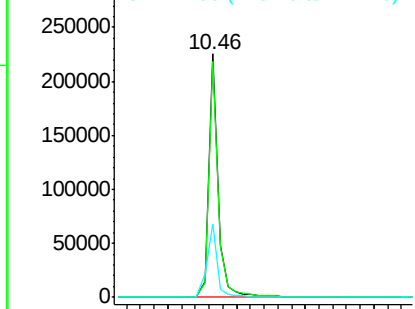



#44
 2-Fluorobiphenyl
 Concen: 93.84 ng
 RT: 9.01 min Scan# 641
 Delta R.T. -0.02 min
 Lab File: BF091139.D
 Acq: 11 Nov 2016 14:49

Tgt Ion:172 Resp: 1749180
 Ion Ratio Lower Upper
 172 100
 171 36.3 29.8 44.6
 170 25.0 20.3 30.5

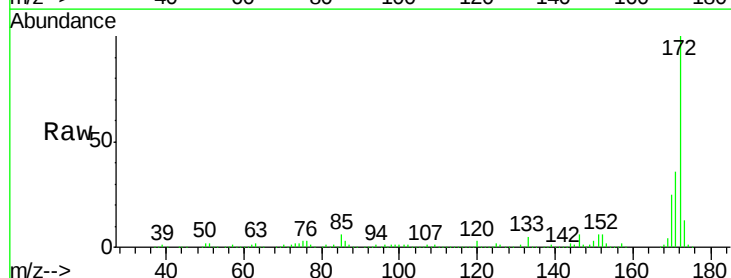

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

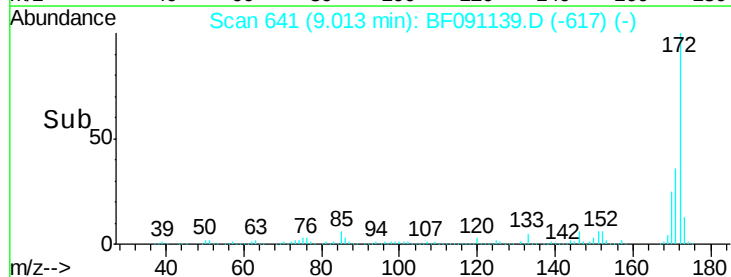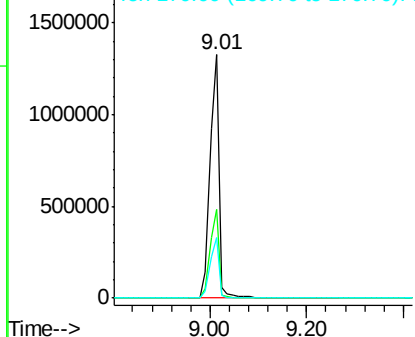







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.15 min Scan# 828
Delta R.T. -0.02 min
Lab File: BF091139.D
Acq: 11 Nov 2016 14:49

Instrument :
BNA_F
ClientSampleId :
PB94644BL

Tot Ion:188 Resp: 555430
Ion Ratio Lower Upper
188 100
94 14.6 7.0 10.4#
80 16.1 7.5 11.3#

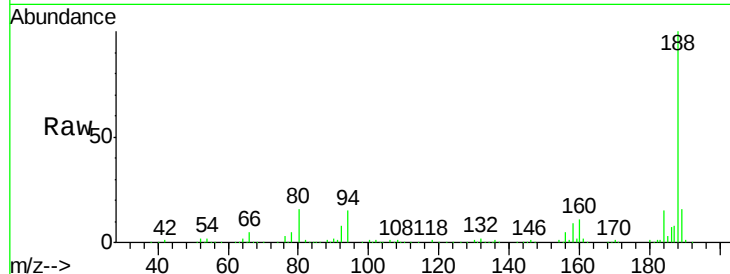


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

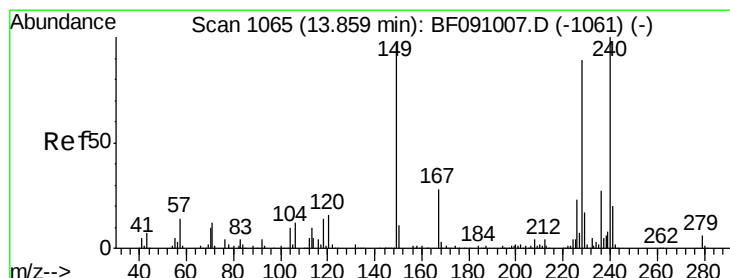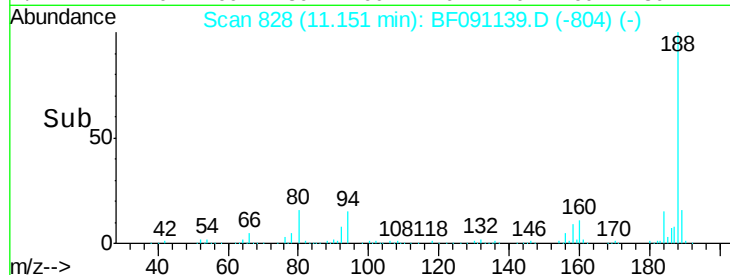
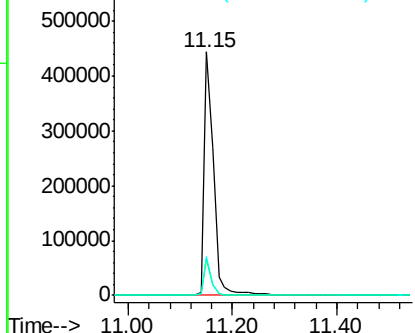



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.78 min Scan# 1058
Delta R.T. -0.03 min
Lab File: BF091139.D
Acq: 11 Nov 2016 14:49

Tgt Ion:240 Resp: 533003
Ion Ratio Lower Upper
240 100
120 16.6 12.9 19.3
236 27.8 21.9 32.9

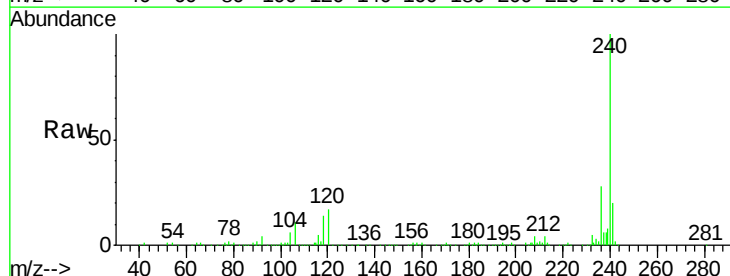

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

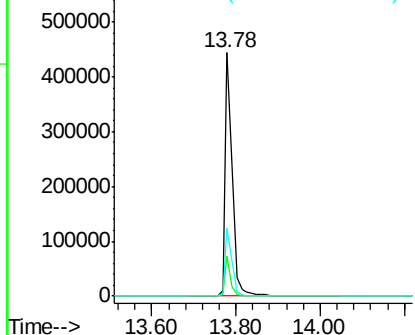


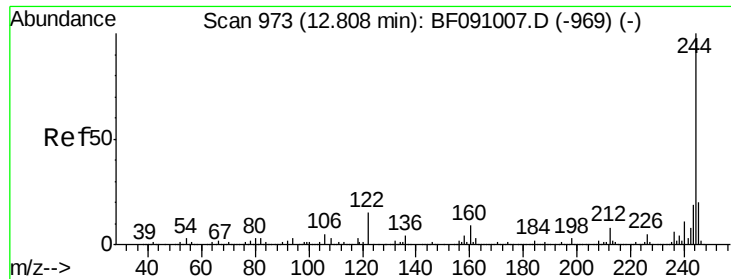




#78
 Terphenyl-d14
 Concen: 82.59 ng
 RT: 12.74 min Scan# 967
 Delta R.T. -0.02 min
 Lab File: BF091139.D
 Acq: 11 Nov 2016 14:49

Instrument :
 BNA_F
 ClientSampleId :
 PB94644BL

Tot Ion:244 Resp: 1763941
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.4 9.6
 122 13.8 12.3 18.5

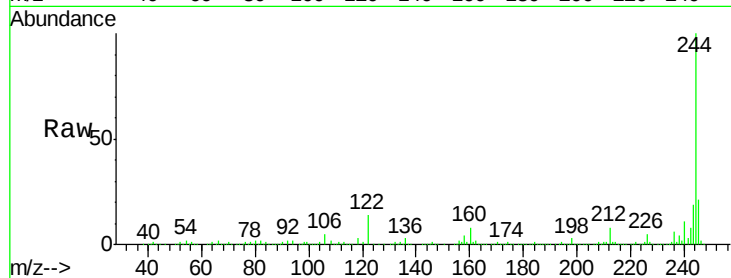


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

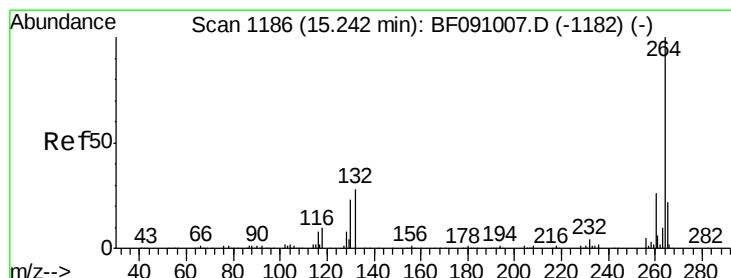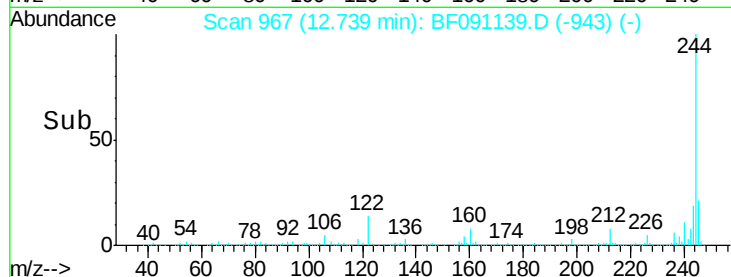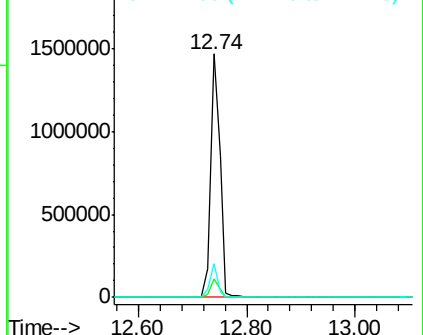

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.15 min Scan# 1178
 Delta R.T. -0.03 min
 Lab File: BF091139.D
 Acq: 11 Nov 2016 14:49

Tgt Ion:264 Resp: 481021
 Ion Ratio Lower Upper
 264 100
 260 25.6 20.6 30.8
 265 21.8 17.8 26.8

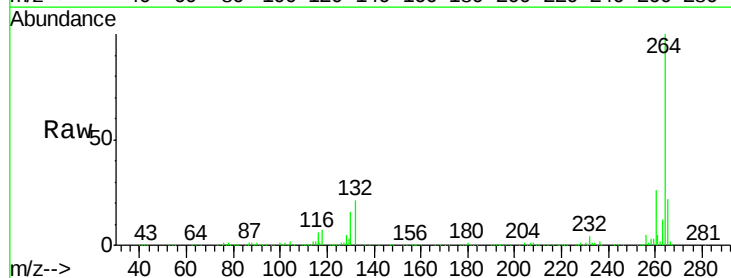

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

