

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111117\
 Data File : BF100446.D
 Acq On : 11 Nov 2017 17:44
 Operator : SJ/JU
 Sample : I6409-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH=110917-02-FREEZE-PIT

Quant Time: Nov 13 03:54:54 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 10 15:44:40 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	150512	20.00	ng	0.00
21) Naphthalene-d8	8.19	136	534746	20.00	ng	0.00
38) Acenaphthene-d10	9.94	164	204864	20.00	ng	0.00
63) Phenanthrene-d10	11.43	188	330157	20.00	ng	0.00
75) Chrysene-d12	14.07	240	320795	20.00	ng	0.00
86) Perylene-d12	15.55	264	226648	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	474203	50.50	ng	0.00
7) Phenol-d6	6.52	99	344595	29.76	ng	0.00
23) Nitrobenzene-d5	7.47	82	849433	105.02	ng	0.00
41) 2,4,6-Tribromophenol	10.73	330	217376	104.13	ng	0.00
44) 2-Fluorobiphenyl	9.26	172	1360196	101.10	ng	0.00
78) Terphenyl-d14	13.02	244	1083254	77.59	ng	0.00
Target Compounds						
10) Phenol	6.53	94	28591	2.352	ng	96
49) Dimethylphthalate	9.65	163	32826	2.099	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF111117\
Data File : BF100446.D
Acq On : 11 Nov 2017 17:44
Operator : SJ/JU
Sample : I6409-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH=110917-02-FREEZE-PIT

Quant Time: Nov 13 03:54:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:44:40 2017
Response via : Initial Calibration

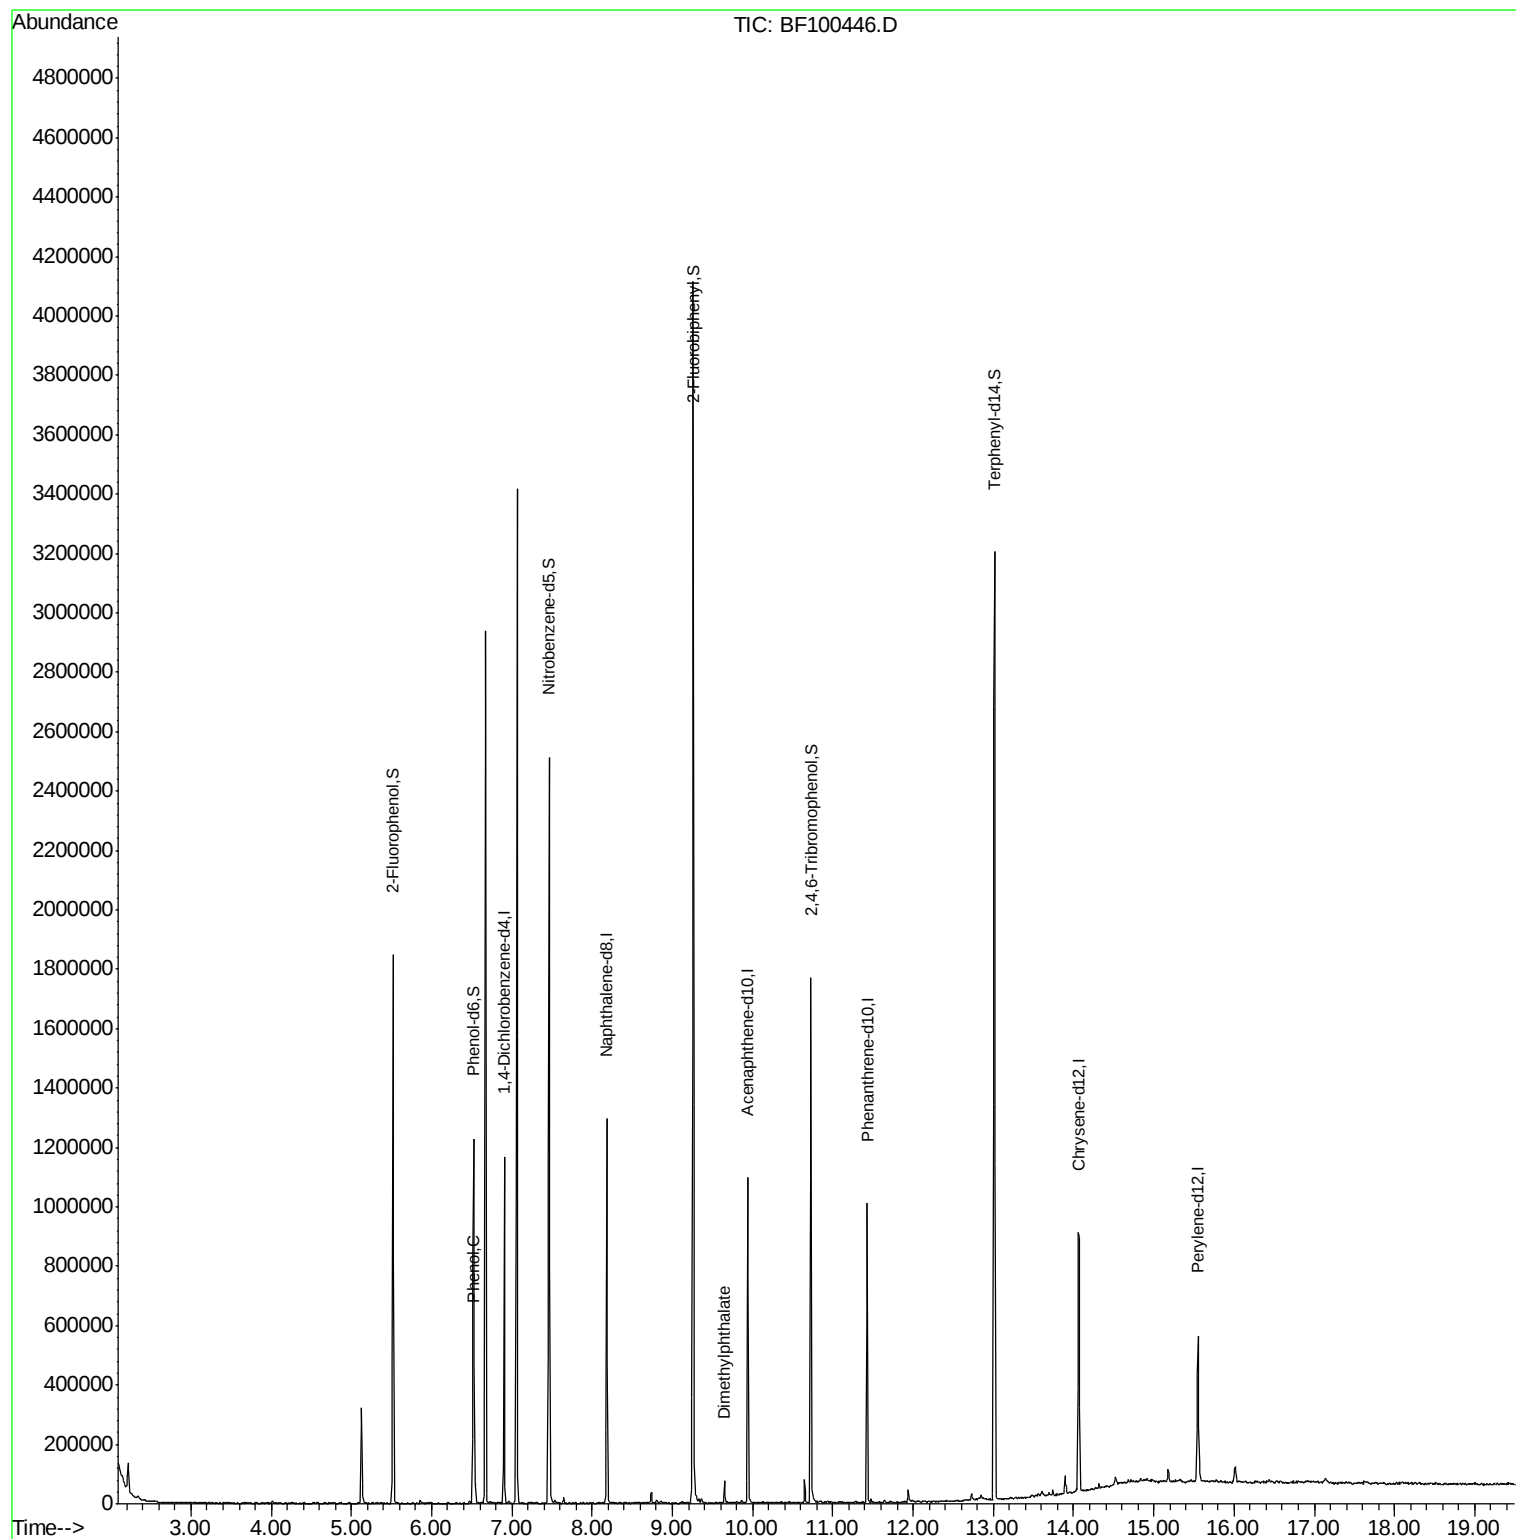

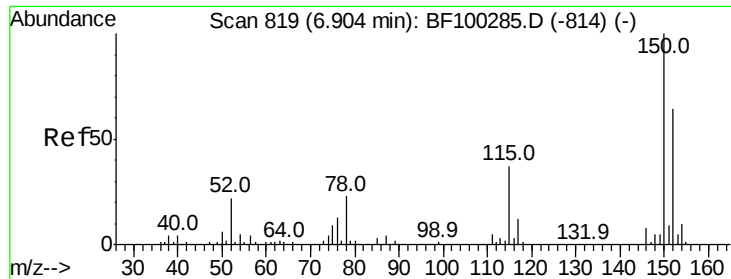


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.90 min Scan# 819
Delta R.T. -0.00 min
Lab File: BF100446.D
Acq: 11 Nov 2017 17:44

Instrument :
BNA_F
ClientSampleId :
MH=110917-02-FREEZE-PIT

Tot Ion:152 Resp: 150512
Ion Ratio Lower Upper
152 100
150 156.5 124.6 186.8
115 59.7 50.1 75.1

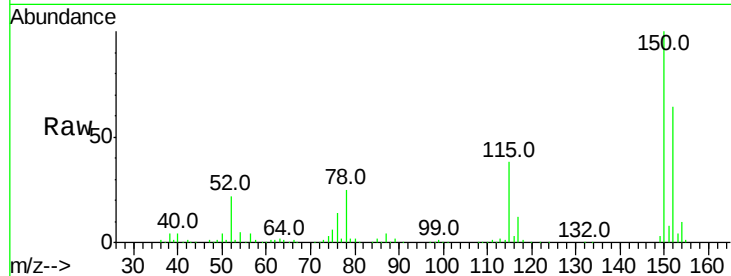


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

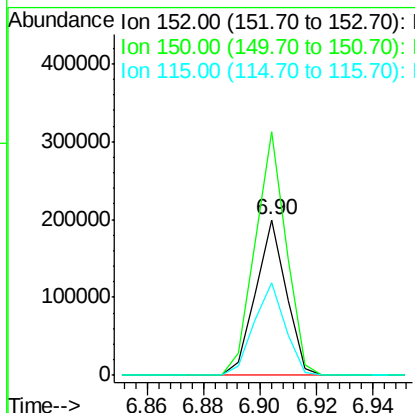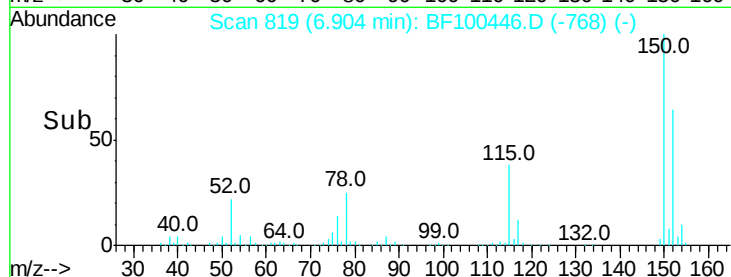



#5

2-Fluorophenol
Concen: 50.504 ng
RT: 5.52 min Scan# 584
Delta R.T. 0.01 min
Lab File: BF100446.D
Acq: 11 Nov 2017 17:44

Tgt Ion:112 Resp: 474203
Ion Ratio Lower Upper
112 100
64 59.9 47.9 71.9
63 31.0 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

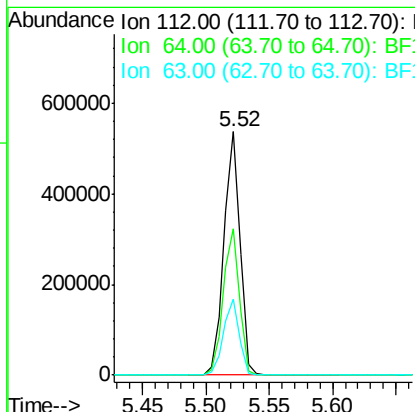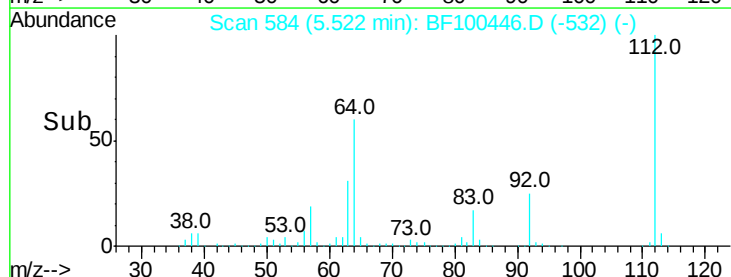



#7

Phenol-d6

Concen: 29.762 ng

RT: 6.52 min Scan# 754

Delta R.T. -0.01 min

Lab File: BF100446.D

Acq: 11 Nov 2017 17:44

Instrument :

BNA_F

ClientSampleId :

MH=110917-02-FREEZE-PIT





Tot Ion: 99 Resp: 344595

Ion Ratio Lower Upper

99 100

42 19.6 14.5 21.7

71 31.9 25.4 38.0

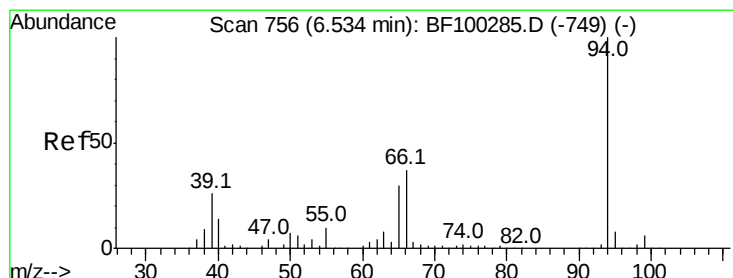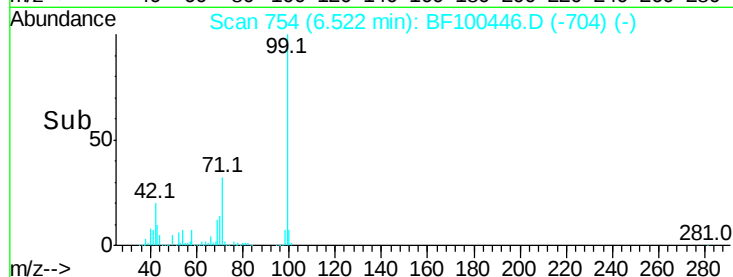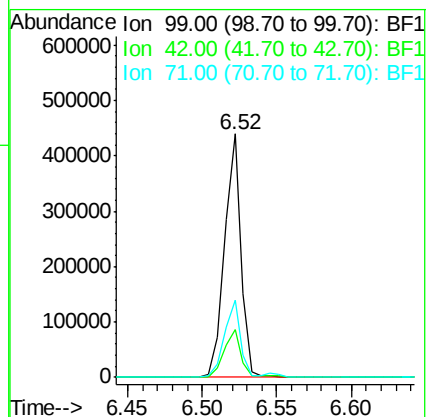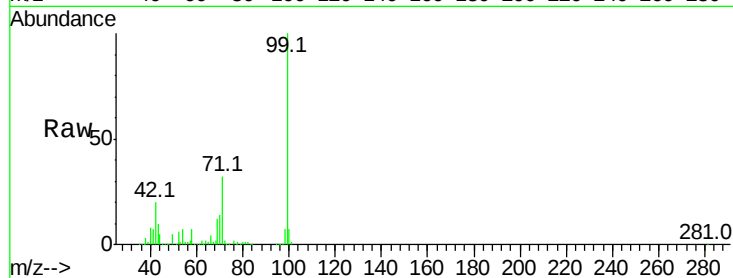

#10

Phenol

Concen: 2.352 ng

RT: 6.53 min Scan# 756

Delta R.T. -0.01 min

Lab File: BF100446.D

Acq: 11 Nov 2017 17:44




Tgt Ion: 94 Resp: 28591


Ion Ratio Lower Upper

94 100

65 26.3 7.9 47.9

66 33.7 16.2 56.2

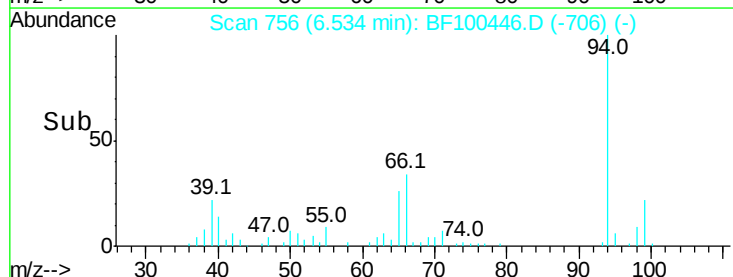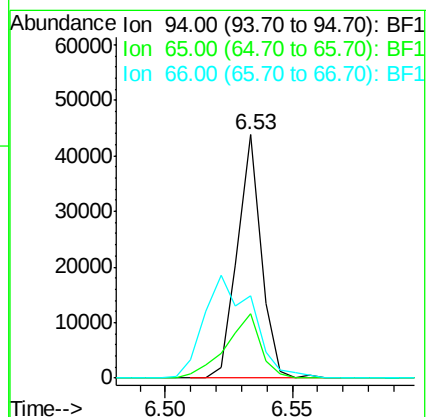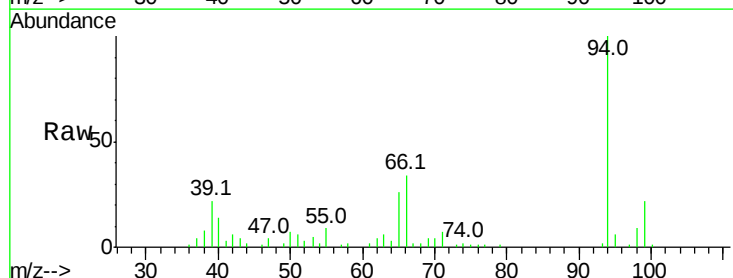


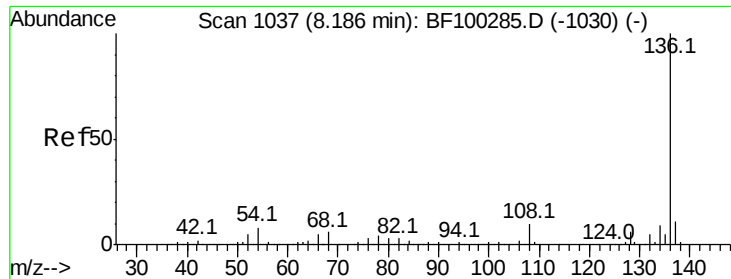




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.19 min Scan# 1037
Delta R.T. -0.00 min
Lab File: BF100446.D
Acq: 11 Nov 2017 17:44

Instrument :
BNA_F
ClientSampleId :
MH=110917-02-FREEZE-PIT

Tot Ion:136	Resp:	534746
Ion Ratio	Lower	Upper
136	100	
137	10.6	8.9 13.3
54	8.1	6.6 9.8
68	6.2	5.0 7.4

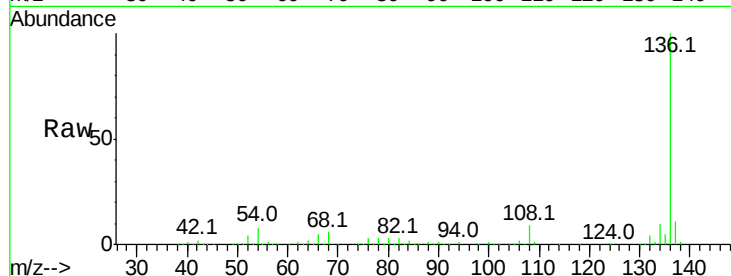


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

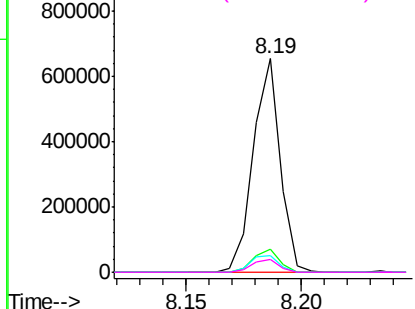
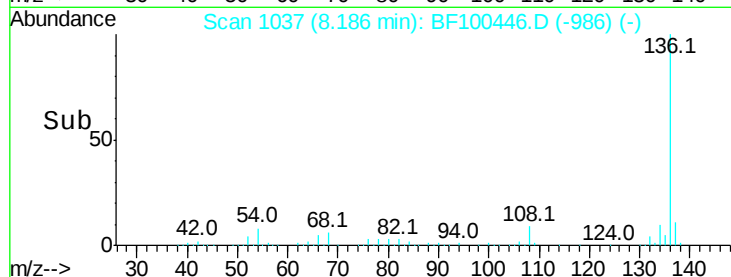



#23
Nitrobenzene-d5
Concen: 105.020 ng
RT: 7.47 min Scan# 915
Delta R.T. -0.00 min
Lab File: BF100446.D
Acq: 11 Nov 2017 17:44

Tgt Ion: 82	Resp:	849433
Ion Ratio	Lower	Upper
82	100	
128	45.7	36.1 54.1
54	53.6	41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1



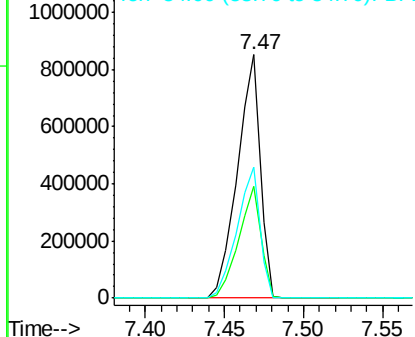
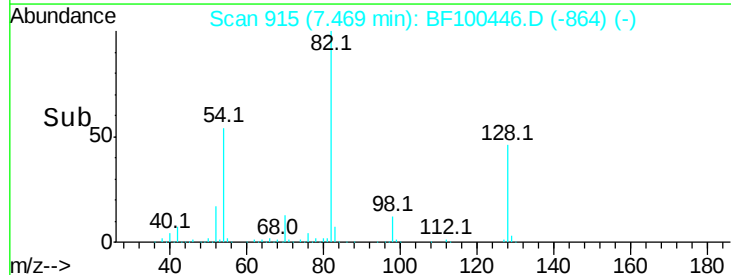


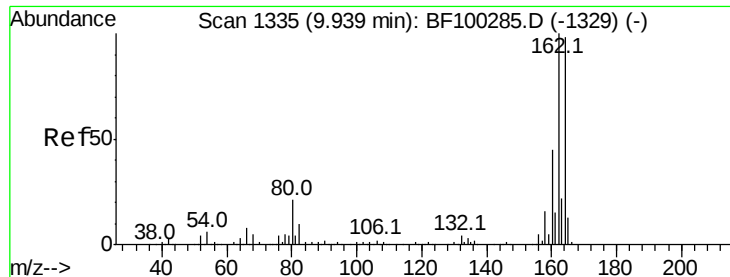

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.94 min Scan# 1335
 Delta R.T. -0.01 min
 Lab File: BF100446.D
 Acq: 11 Nov 2017 17:44




Instrument :
 BNA_F
 ClientSampleId :
 MH=110917-02-FREEZE-PIT


Tot Ion	Ratio	Lower	Upper
164	100		
162	103.4	86.1	129.1
160	46.6	38.3	57.5

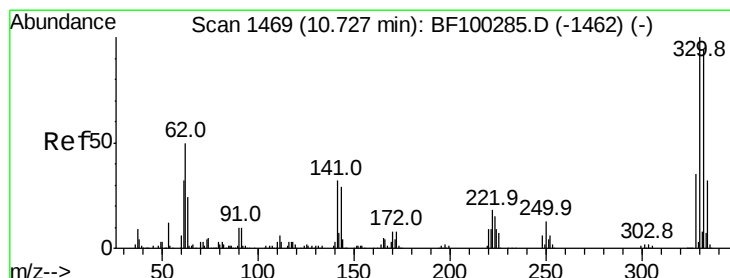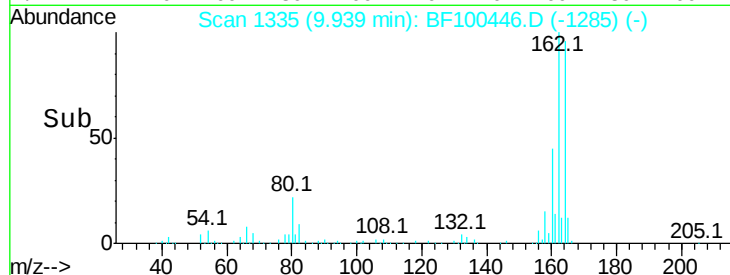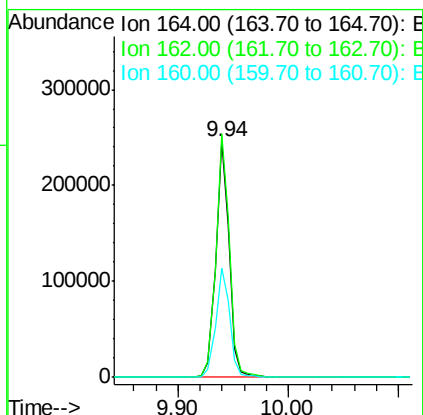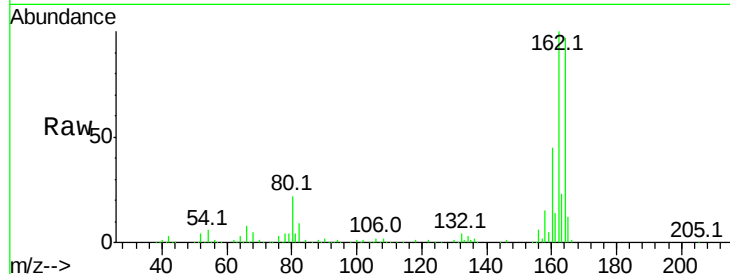

#41
 2,4,6-Tribromophenol
 Concen: 104.129 ng
 RT: 10.73 min Scan# 1469
 Delta R.T. -0.01 min
 Lab File: BF100446.D
 Acq: 11 Nov 2017 17:44

Tgt Ion	Ratio	Lower	Upper
330	100		
332	94.8	77.0	115.6
141	31.2	29.9	44.9

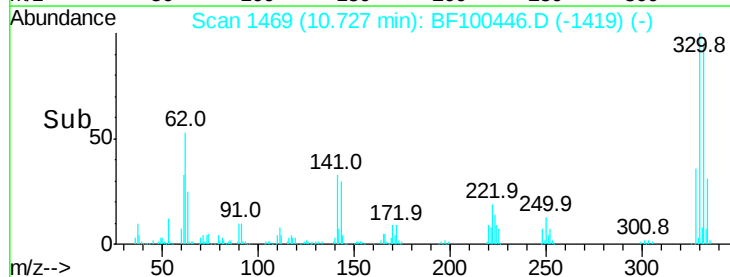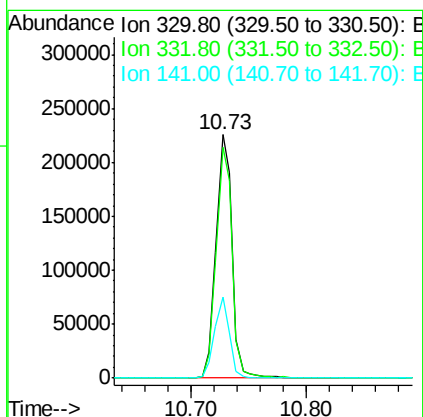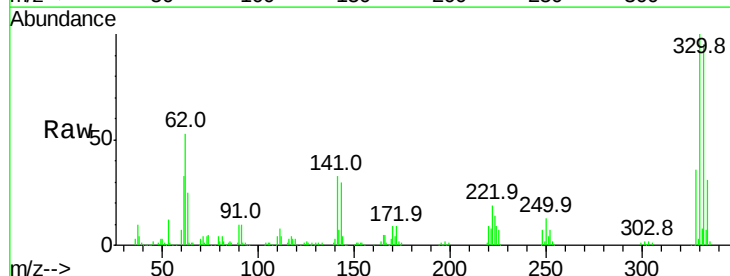


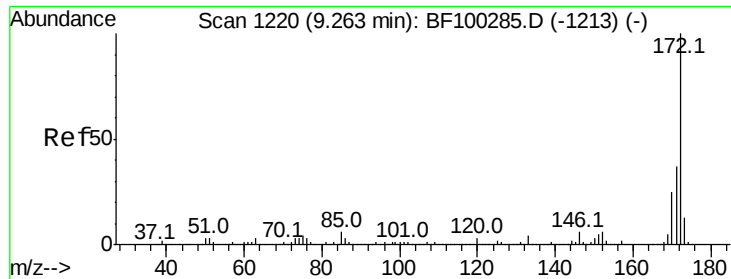




#44
2-Fluorobiphenyl
Concen: 101.101 ng
RT: 9.26 min Scan# 1220
Delta R.T. -0.00 min
Lab File: BF100446.D
Acq: 11 Nov 2017 17:44

Instrument :
BNA_F
ClientSampleId :
MH=110917-02-FREEZE-PIT

Tot Ion:172 Resp: 1360196
Ion Ratio Lower Upper
172 100
171 36.1 29.7 44.5
170 24.5 19.6 29.4




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

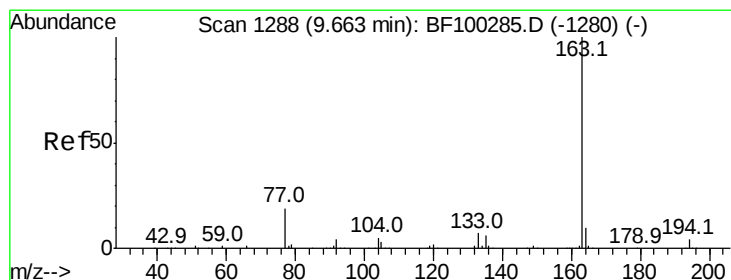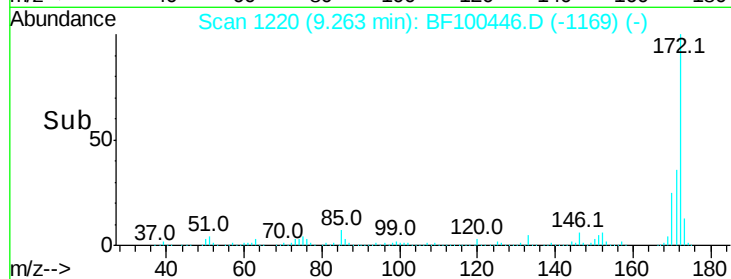
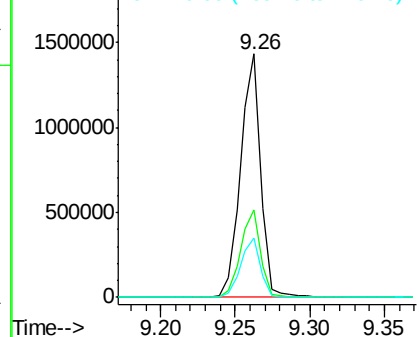



#49
Dimethylphthalate
Concen: 2.099 ng
RT: 9.65 min Scan# 1286
Delta R.T. -0.01 min
Lab File: BF100446.D
Acq: 11 Nov 2017 17:44

Tgt Ion:163 Resp: 32826
Ion Ratio Lower Upper
163 100
194 3.3 2.7 4.1
164 10.3 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



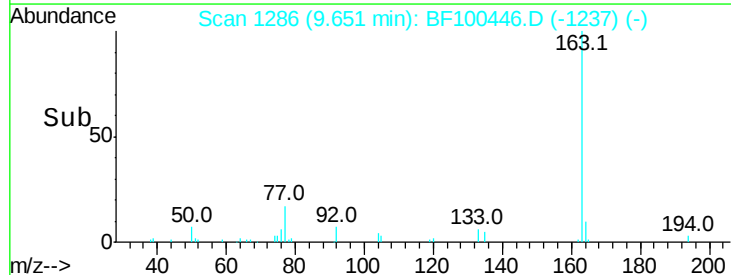
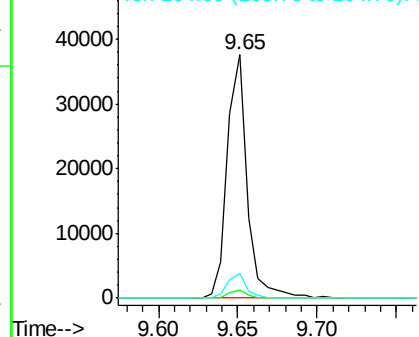


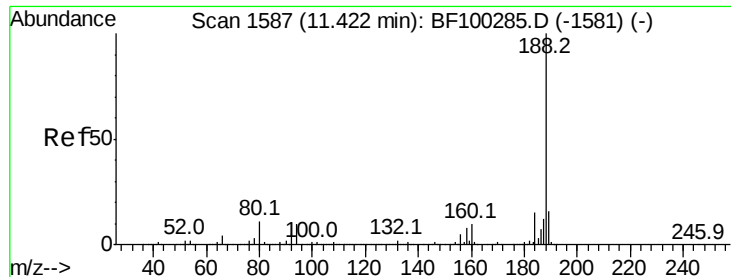

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.43 min Scan# 1588
Delta R.T. -0.00 min
Lab File: BF100446.D
Acq: 11 Nov 2017 17:44




Instrument :
BNA_F
ClientSampleId :
MH=110917-02-FREEZE-PIT


Tot Ion:188 Resp: 330157
Ion Ratio Lower Upper
188 100
94 10.1 8.5 12.7
80 10.7 9.2 13.8

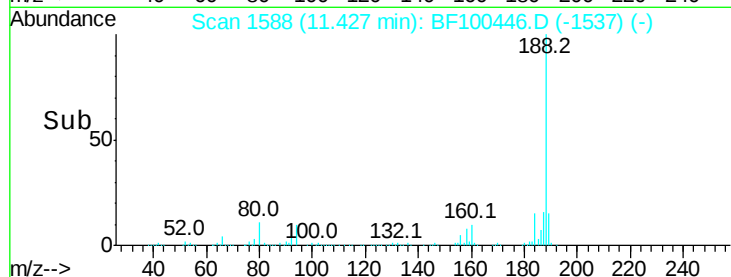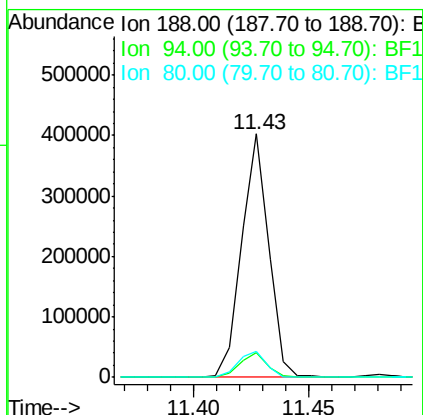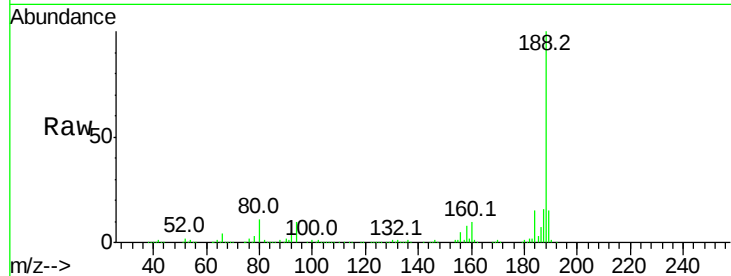

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.07 min Scan# 2037
Delta R.T. -0.00 min
Lab File: BF100446.D
Acq: 11 Nov 2017 17:44

Tgt Ion:240 Resp: 320795
Ion Ratio Lower Upper
240 100
120 10.3 9.5 14.3
236 25.4 20.7 31.1

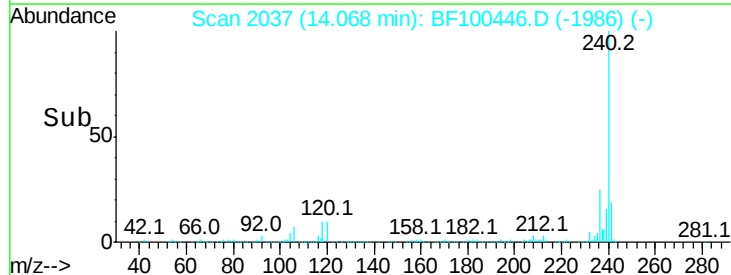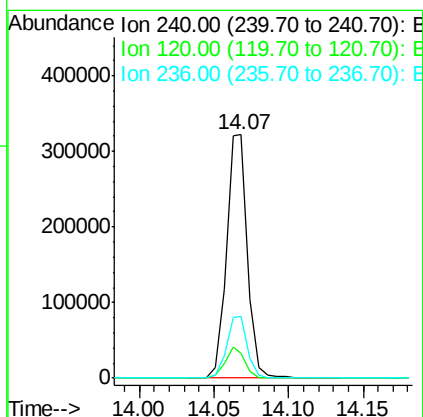

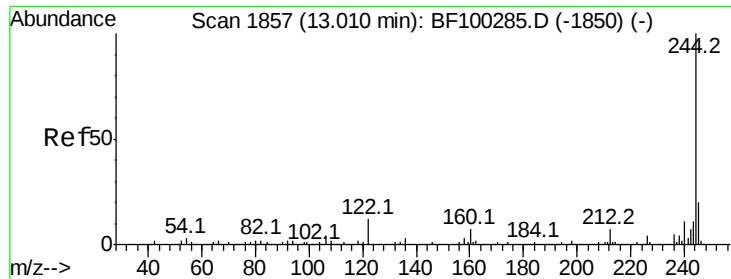

#78

Terphenyl-d14

Concen: 77.589 ng

RT: 13.02 min Scan# 1858

Delta R.T. 0.01 min

Lab File: BF100446.D

Acq: 11 Nov 2017 17:44

Instrument :

BNA_F

ClientSampleId :

MH=110917-02-FREEZE-PIT


Tot Ion:244 Resp: 1083254

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0




122 11.1 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

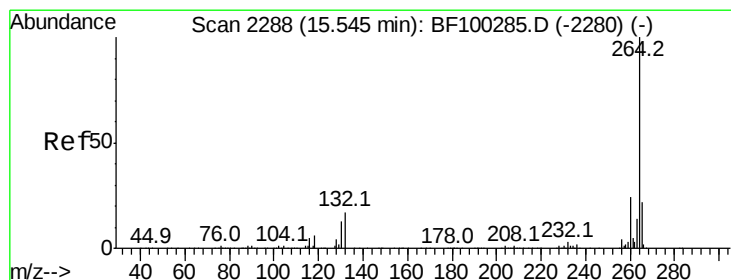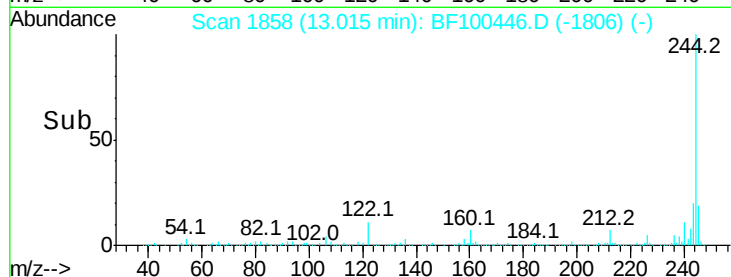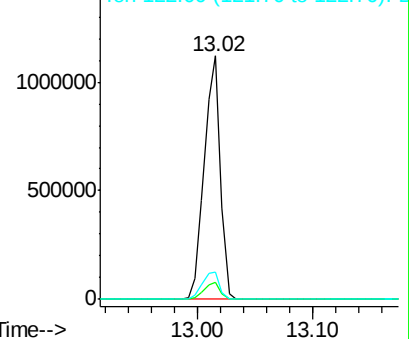

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.55 min Scan# 2289

Delta R.T. 0.01 min

Lab File: BF100446.D

Acq: 11 Nov 2017 17:44


Tgt Ion:264 Resp: 226648

Ion Ratio Lower Upper

264 100

260 24.8 19.2 28.8

265 21.3 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

