

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111117\
 Data File : BF100469.D
 Acq On : 12 Nov 2017 5:16
 Operator : SJ/JU
 Sample : I6407-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 4632

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.145	516	520	533	rVB	688872	891460	23.19%	2.898%
2	5.534	581	586	589	rBV	3143100	3231472	84.05%	10.504%
3	6.528	750	755	758	rBV	2706547	2840335	73.87%	9.233%
4	6.675	775	780	783	rBV	3494712	3493239	90.86%	11.355%
5	6.904	815	819	822	rBV	1032465	814238	21.18%	2.647%
6	7.063	841	846	849	rBV	3025326	2860269	74.39%	9.298%
7	7.463	909	914	917	rBV	2125995	2337680	60.80%	7.599%
8	8.181	1032	1036	1038	rBV	1100315	1071601	27.87%	3.483%
9	8.204	1038	1040	1044	rVV	1454862	1152610	29.98%	3.747%
10	8.257	1045	1049	1052	rVB	104360	92931	2.42%	0.302%
11	8.892	1154	1157	1161	rBV	207698	165851	4.31%	0.539%
12	8.992	1169	1174	1178	rBV	107740	87268	2.27%	0.284%
13	9.257	1214	1219	1223	rBV	3761982	3844841	100.00%	12.498%
14	9.939	1331	1335	1338	rBV	1056975	938706	24.41%	3.051%
15	9.969	1338	1340	1343	rVB	85745	67336	1.75%	0.219%
16	10.727	1464	1469	1472	rBV	1897777	1747638	45.45%	5.681%
17	11.427	1584	1588	1590	rBV	858906	797477	20.74%	2.592%
18	11.445	1590	1591	1594	rVB	85274	56767	1.48%	0.185%
19	12.757	1811	1814	1819	rBV	105585	94126	2.45%	0.306%
20	13.010	1852	1857	1860	rBV	2883813	2825581	73.49%	9.185%
21	13.174	1881	1885	1890	rBV	56540	58444	1.52%	0.190%
22	14.063	2032	2036	2046	rVB	875247	764968	19.90%	2.487%
23	15.545	2283	2288	2299	rBV	370221	528985	13.76%	1.720%


Sum of corrected areas: 30763823

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111117\
Data File : BF100469.D
Acq On : 12 Nov 2017 5:16
Operator : SJ/JU
Sample : I6407-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
4632

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

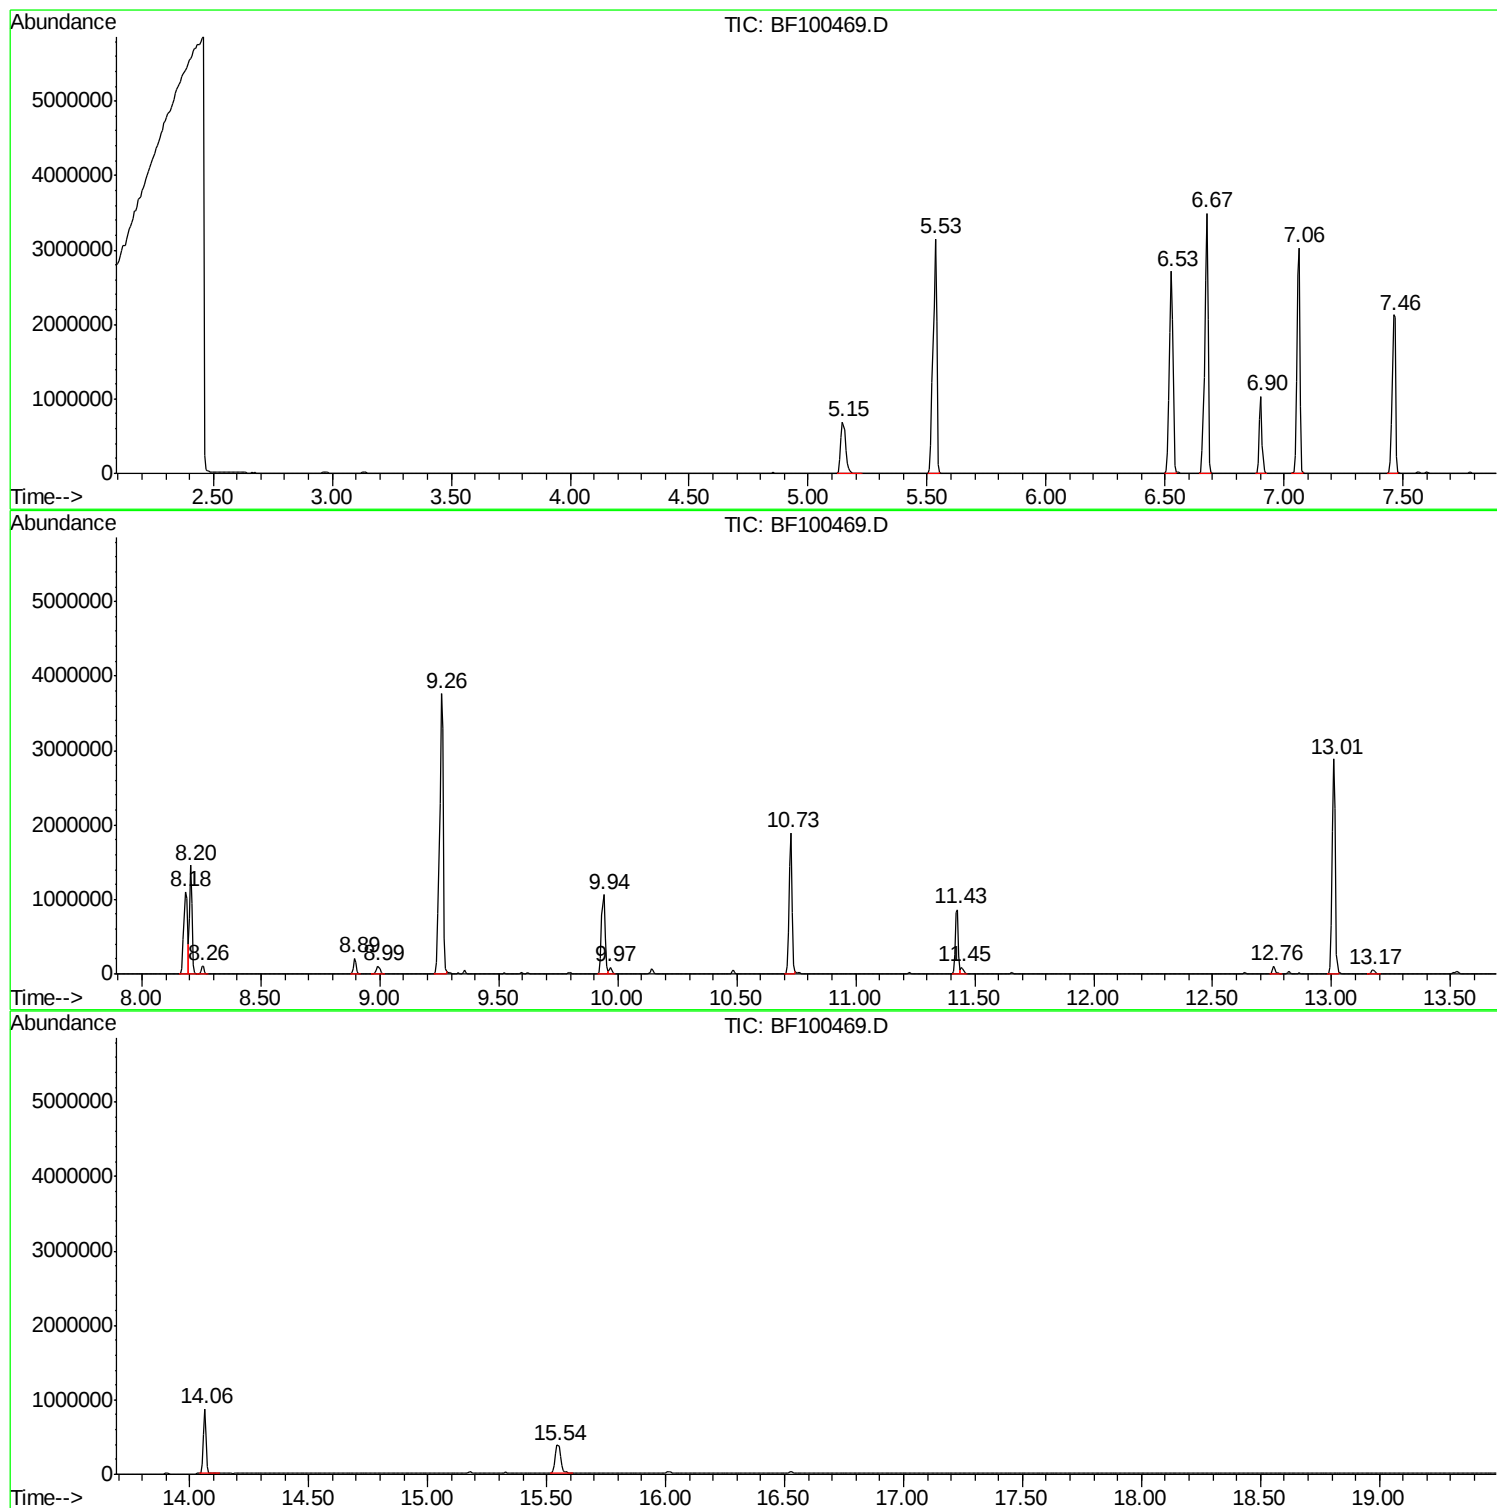

Data_Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF111117\
Data_File : BF100469.D
Acq_On : 12_Nov_2017. 5:166
Operator : SJ/JUU
Sample : I6407-055
Misc :
ALS_Vial : 40 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
4632

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
