

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF111117\
 Data File : BF100471.D
 Acq On : 12 Nov 2017 6:09
 Operator : SJ/JU
 Sample : PB104195BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB104195BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.134	514	518	526	rBV	524059	607755	17.30%	2.539%
2	5.522	580	584	588	rBV	2191794	2269318	64.61%	9.480%
3	6.522	749	754	757	rBV	2302486	2287627	65.13%	9.557%
4	6.545	757	758	766	rVB	56688	37686	1.07%	0.157%
5	6.669	774	779	782	rBV	2489160	2296231	65.37%	9.593%
6	6.898	815	818	822	rBV	923111	832846	23.71%	3.479%
7	7.057	841	845	849	rBV	2708816	2566260	73.06%	10.721%
8	7.463	909	914	917	rBV	2010275	2056872	58.56%	8.593%
9	8.181	1032	1036	1040	rBV	1178251	1034117	29.44%	4.320%
10	9.257	1214	1219	1229	rBV	3570463	3512447	100.00%	14.674%
11	9.939	1331	1335	1350	rVB	1092018	1002182	28.53%	4.187%
12	10.722	1464	1468	1482	rBV	964642	895776	25.50%	3.742%
13	11.422	1584	1587	1591	rBV	943206	821318	23.38%	3.431%
14	12.822	1822	1825	1830	rVB	67875	51450	1.46%	0.215%
15	13.010	1852	1857	1860	rBV	2625660	2435416	69.34%	10.174%
16	14.063	2032	2036	2046	rBV	797411	716848	20.41%	2.995%
17	15.545	2283	2288	2298	rBV	366535	513119	14.61%	2.144%


Sum of corrected areas: 23937268

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111117\
Data File : BF100471.D
Acq On : 12 Nov 2017 6:09
Operator : SJ/JU
Sample : PB104195BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104195BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

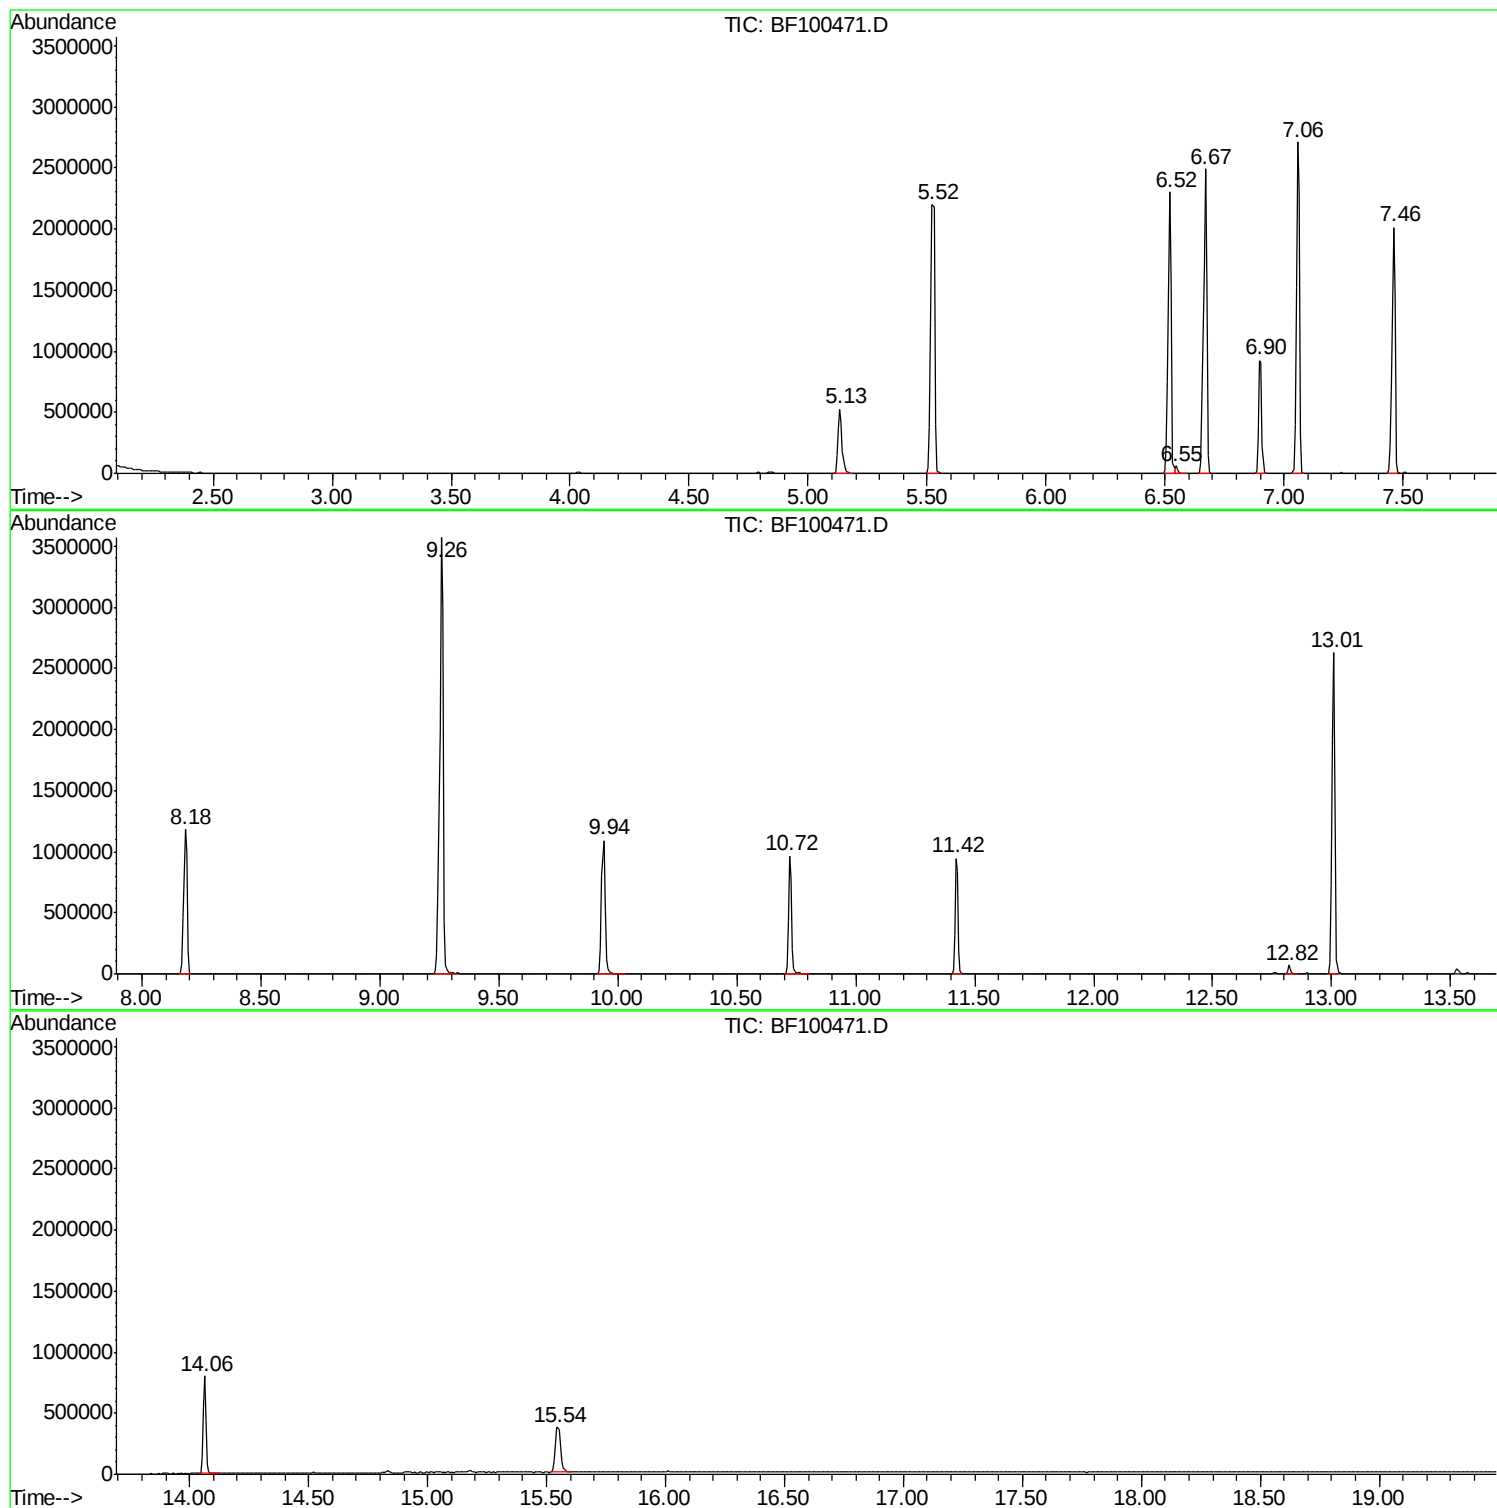

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF111117\
Data File : BF100471.D
Acq On : 12 Nov 2017 6:09
Operator : SJ/JU
Sample : PB104195BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104195BL









Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.13	14.59 ng	607755	1,4-Dichlorobenzene-d4	6.90

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
4			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
5			5-Oxohexanenitrile	111	C6H9NO	010412-98-3	9

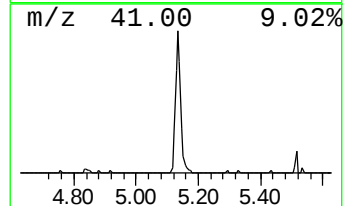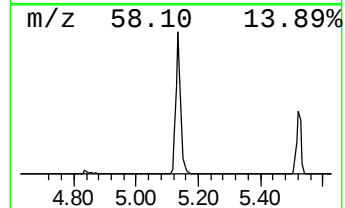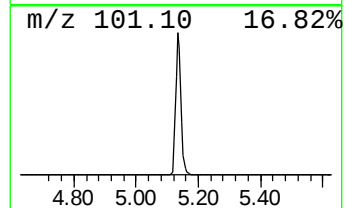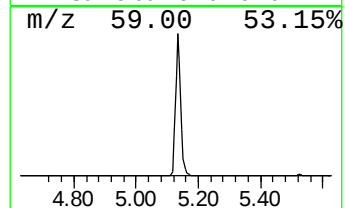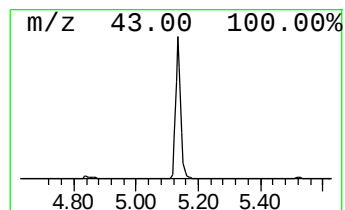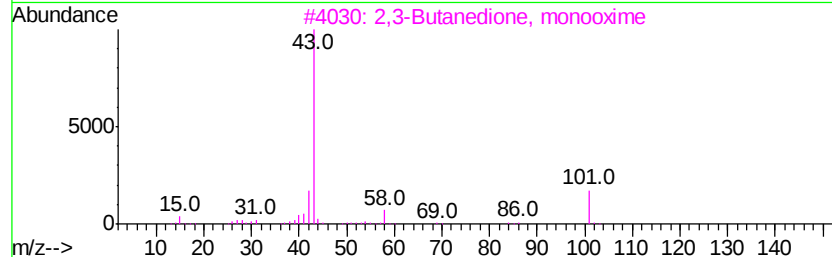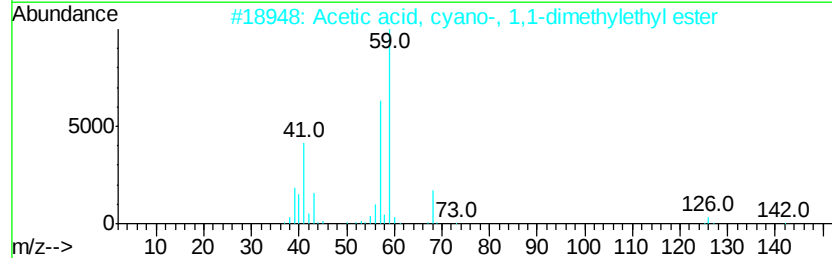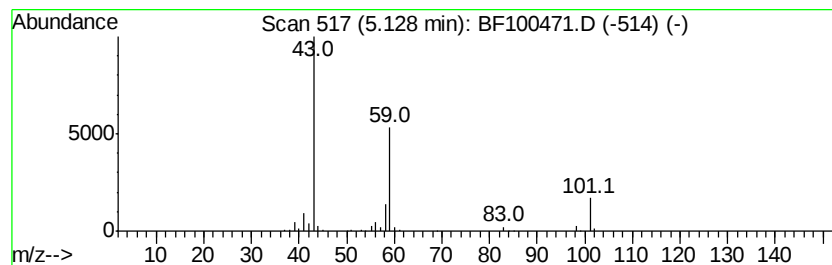

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF111117\
Data File : BF100471.D
Acq On : 12 Nov 2017 6:09
Operator : SJ/JU
Sample : PB104195BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104195BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.67 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.67	55.14 ng	2296230	1,4-Dichlorobenzene-d4	6.90

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3			Bicyclo[4.2.0]octa-1,3,5-triene...	132	C10H12	028749-81-7	9
4			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

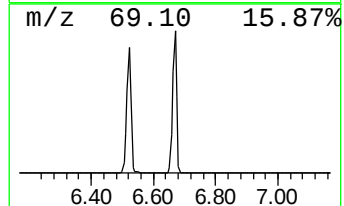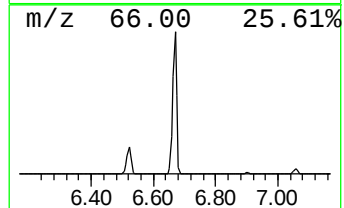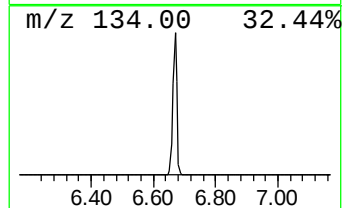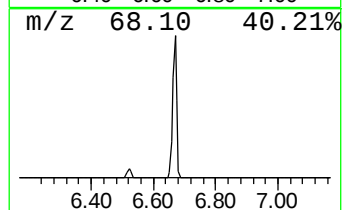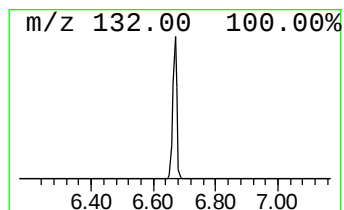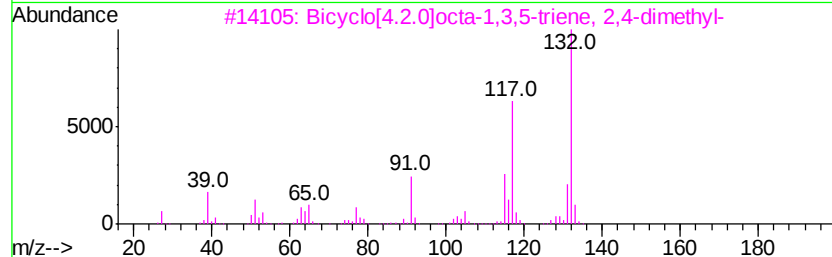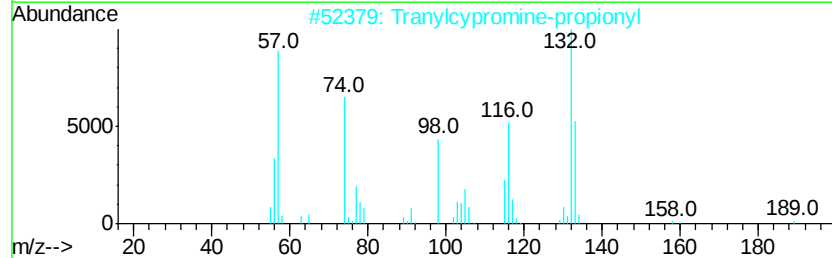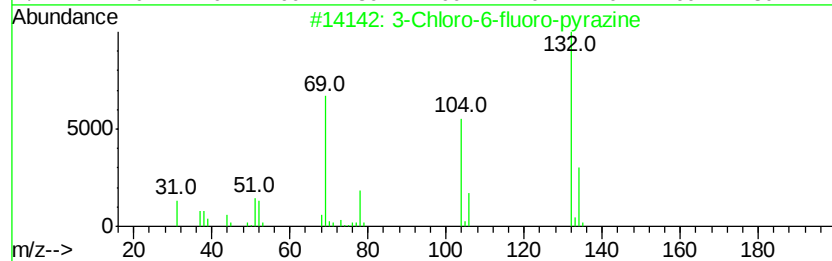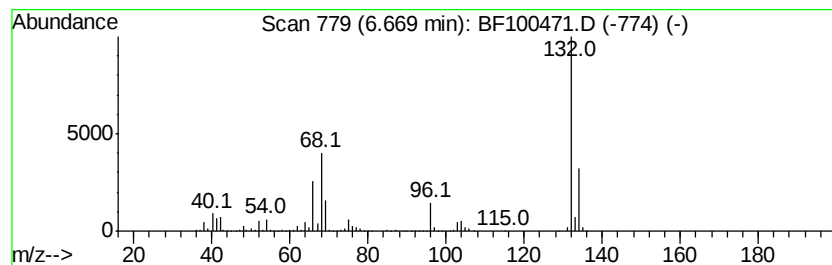

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF111117\
Data File : BF100471.D
Acq On : 12 Nov 2017 6:09
Operator : SJ/JU
Sample : PB104195BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB104195BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.13	14.6	ng	607755	1	6.90	832846	20.0
unknown6.67	6.67	55.1	ng	2296230	1	6.90	832846	20.0