


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF111117\
Data File : BF100454.D
Acq On : 11 Nov 2017 22:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 10 15:44:40 2017

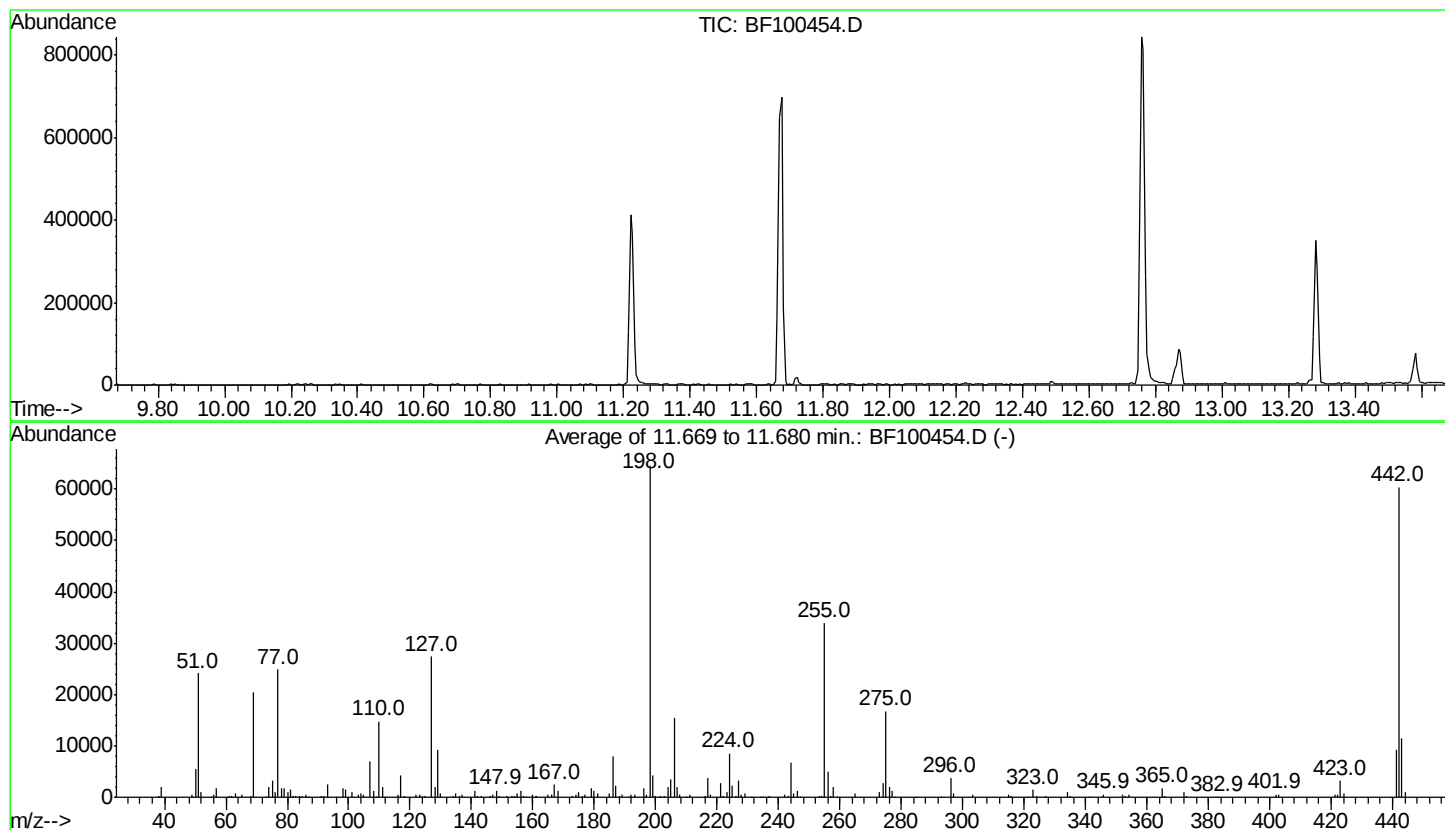

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	24115	PASS
68	69	0.00	2	1.5	314	PASS
69	198	0.00	100	31.5	20327	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	27377	PASS
197	198	0.00	2	1.0	614	PASS
198	198	100	100	100.0	64549	PASS
199	198	5	9	6.5	4203	PASS
275	198	10	60	26.1	16819	PASS
365	198	1	100	2.9	1841	PASS
441	443	0.01	100	79.5	9129	PASS
442	198	50	100	93.5	60341	PASS
443	442	15	24	19.0	11488	PASS