
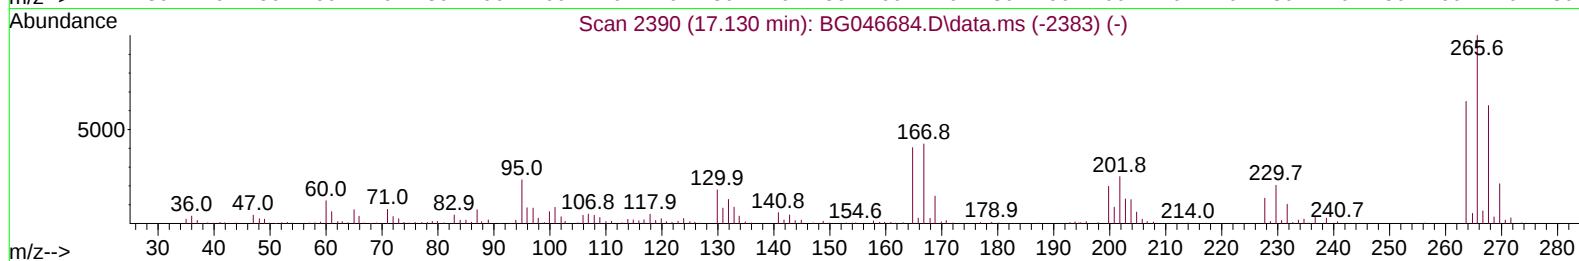
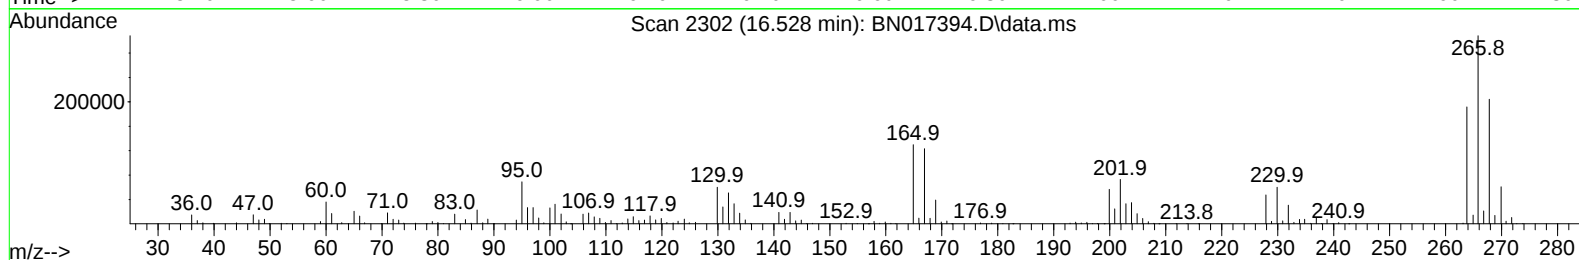


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111221\
Data File : BN017394.D
Acq On : 12 Nov 2021 07:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 13:16:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

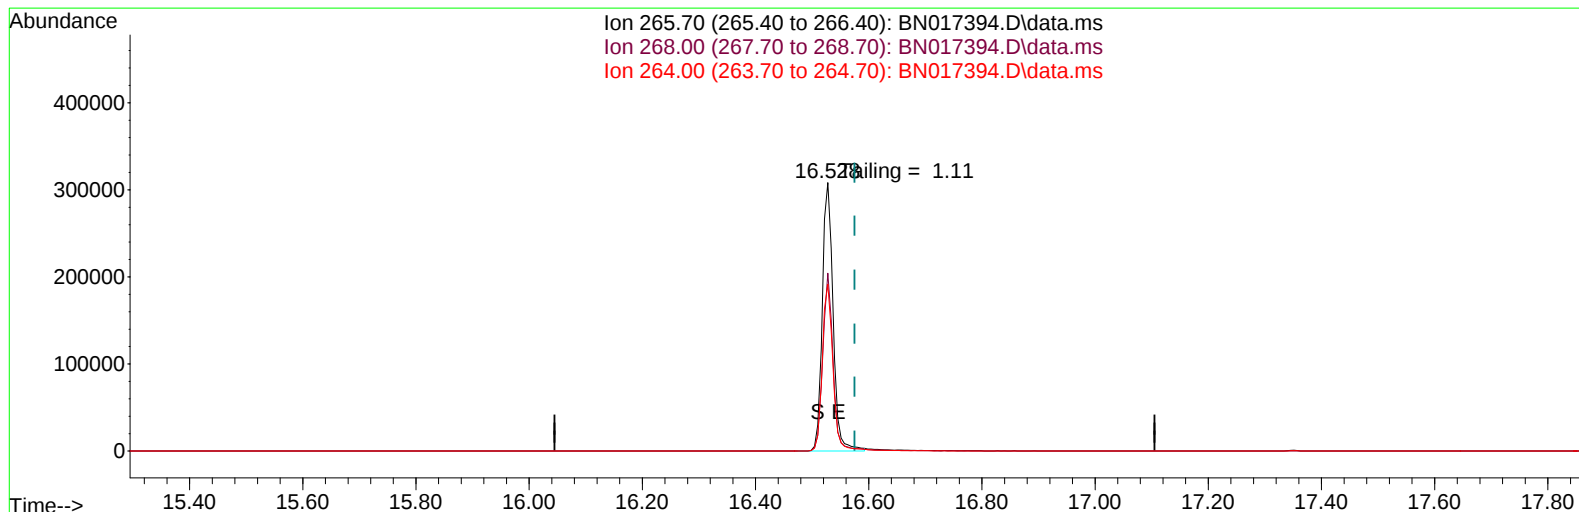

TIC: BN017394.D\data.ms

(70) Pentachlorophenol (C)

16.528min (-0.047) 22751.86 ng

response 416202

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.27
264.00	61.60	62.15
0.00	0.00	0.00