
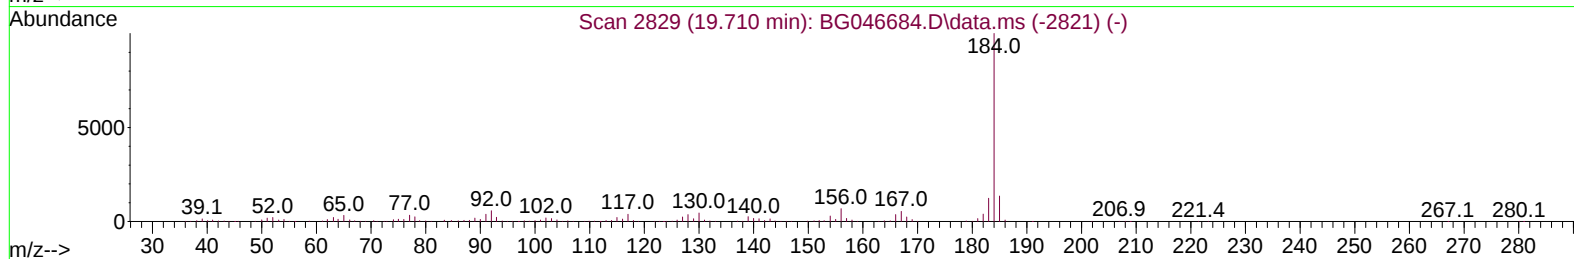
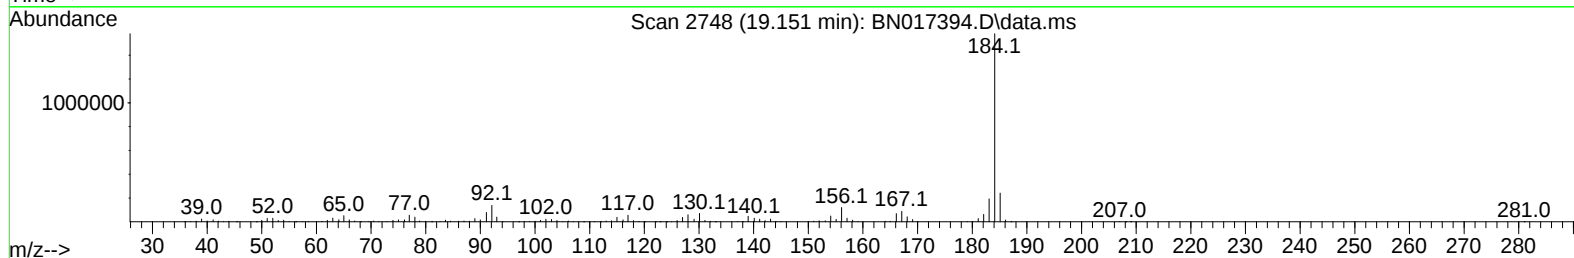


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111221\
Data File : BN017394.D
Acq On : 12 Nov 2021 07:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 13:16:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

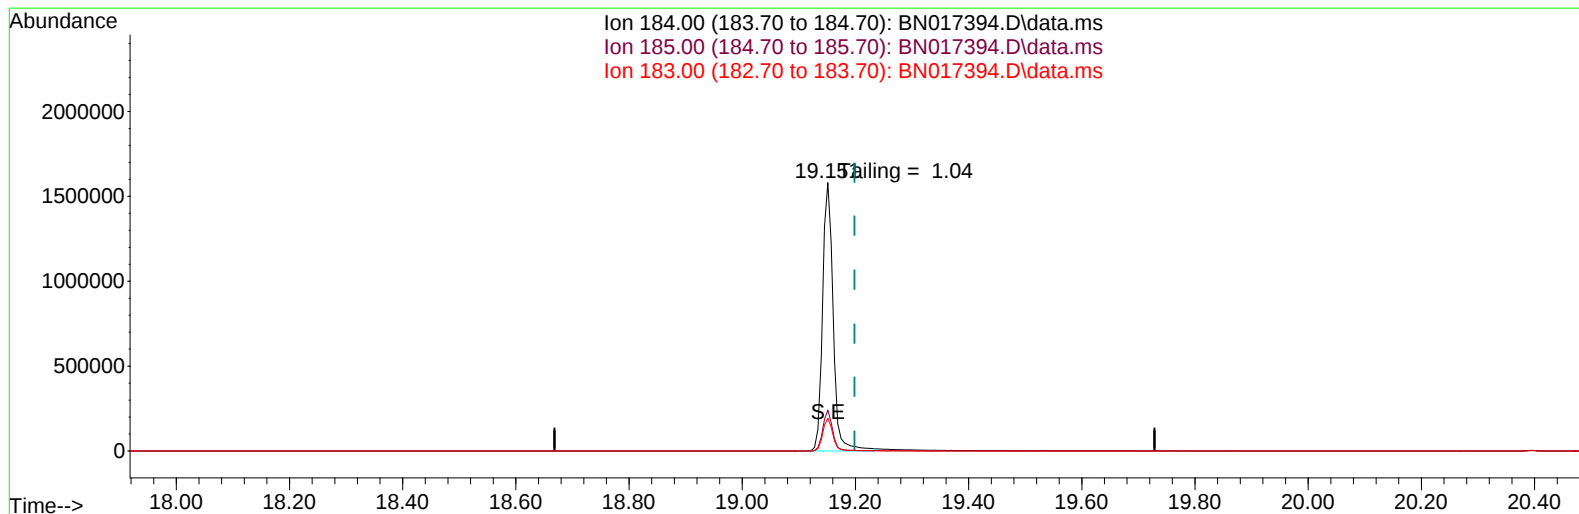

TIC: BN017394.D\data.ms

(77) Benzidine

19.151min (-0.047) 0.00 ng

response 2119002

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.28
183.00	13.20	12.15
0.00	0.00	0.00