
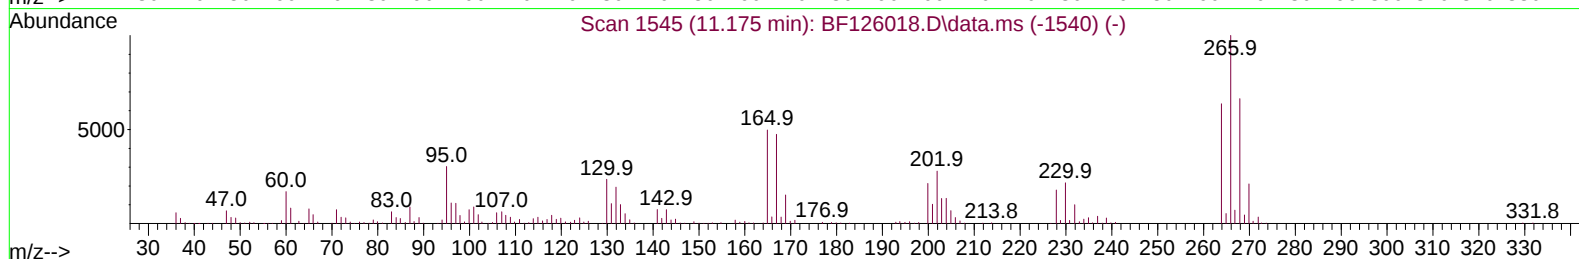
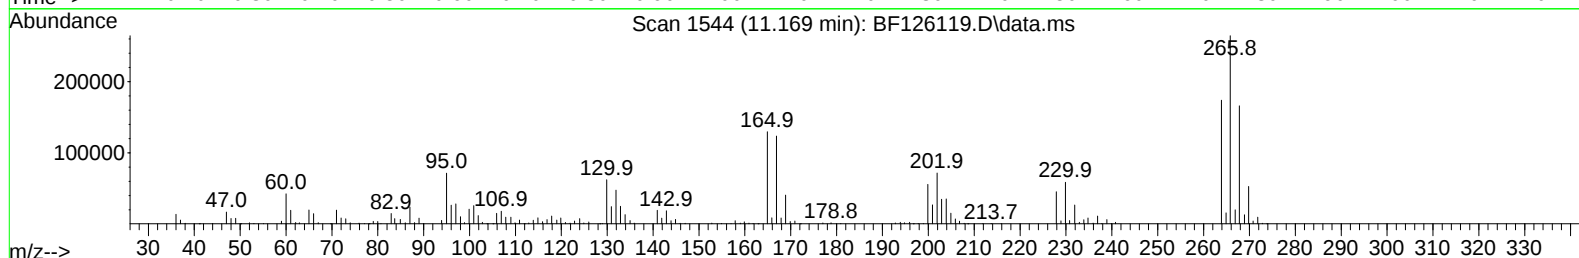


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\  
Data File : BF126119.D  
Acq On    : 11 Nov 2021  10:32  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 11 12:55:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

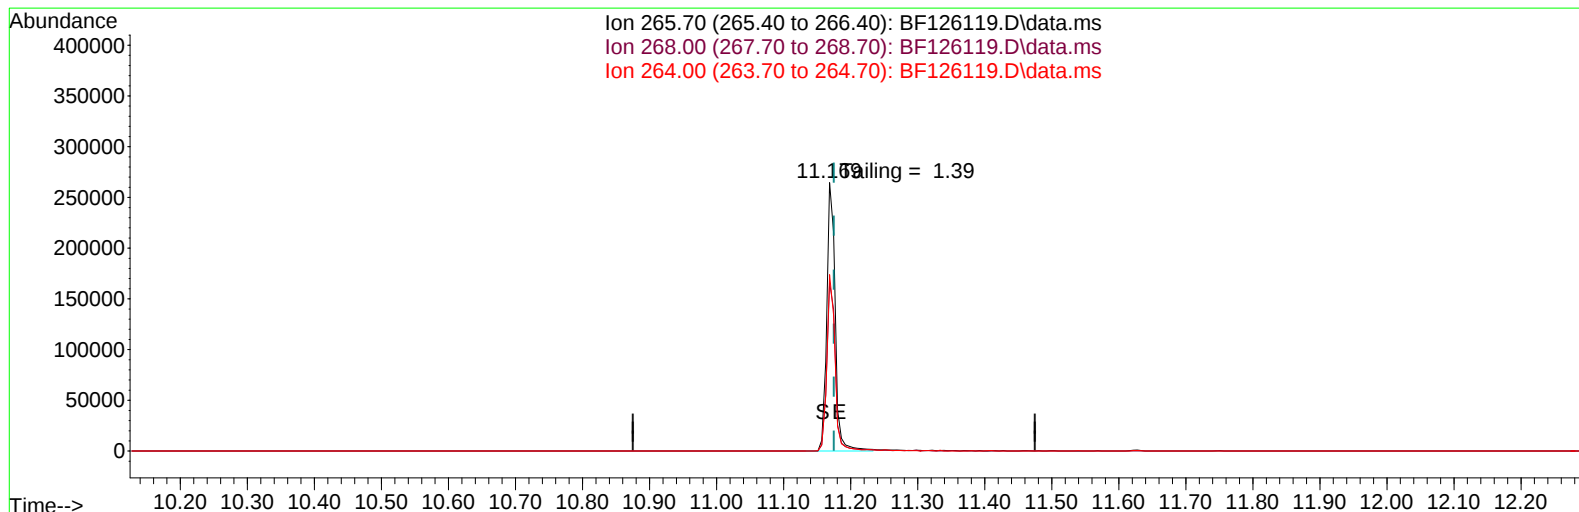

TIC: BF126119.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 28491.47 ng

response 234273

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.75
264.00	69.90	65.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
Data File : BF126119.D
Acq On : 11 Nov 2021 10:32
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 12:55:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

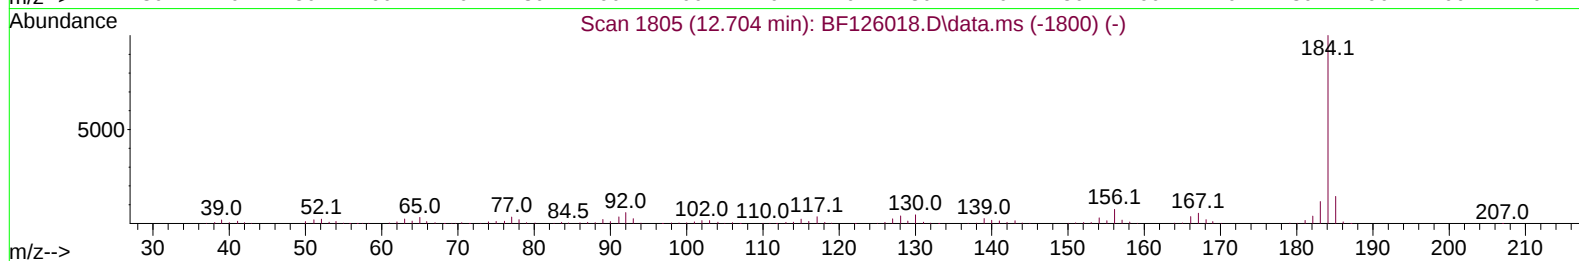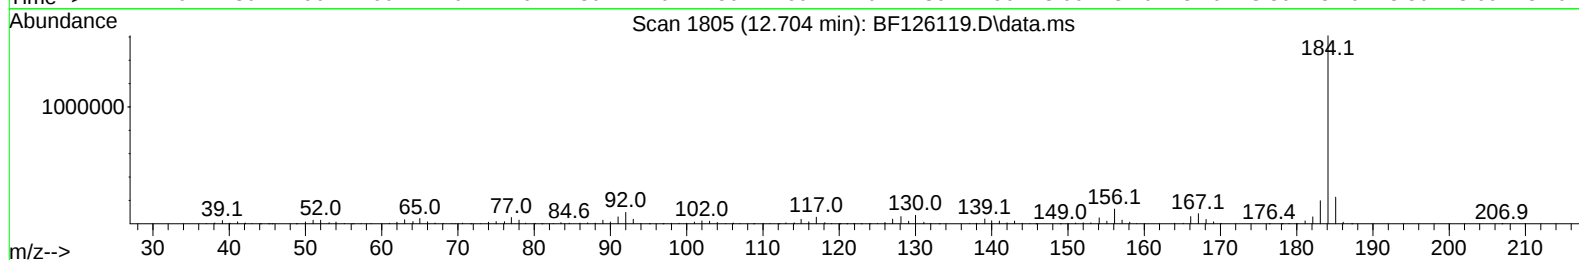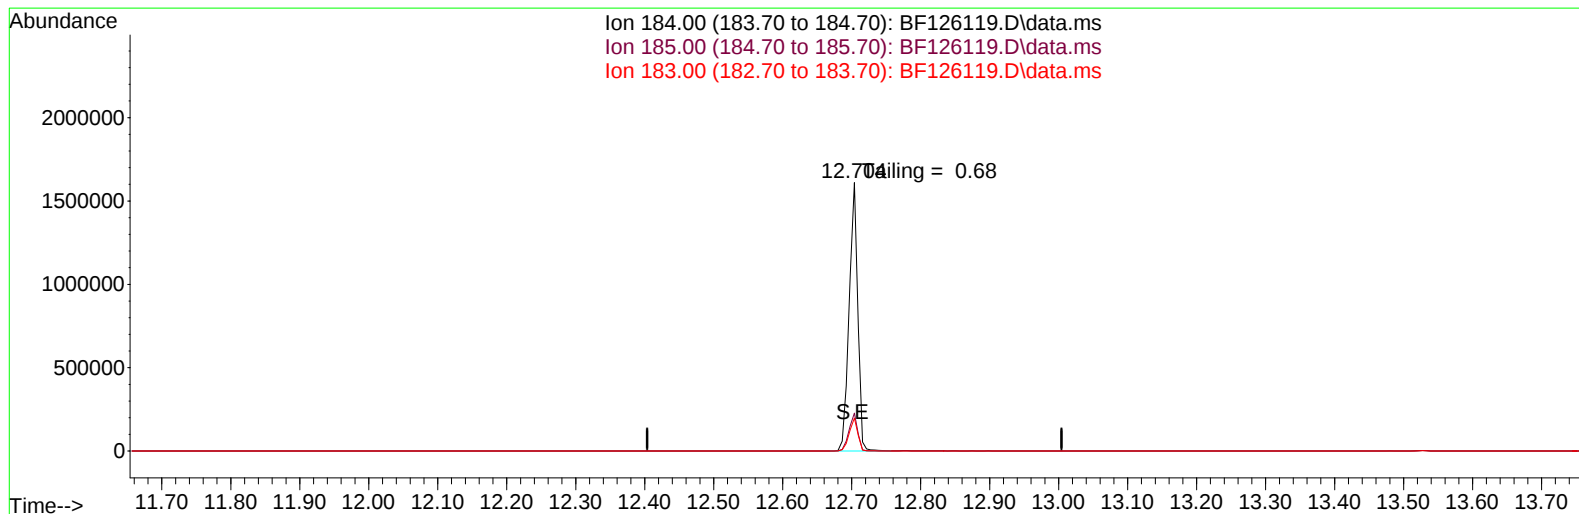

TIC: BF126119.D\data.ms

(77) Benzidine

12.704min (-0.000) 341137.85 ng m

response 1391274

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.18
183.00	10.10	12.27#
0.00	0.00	0.00