
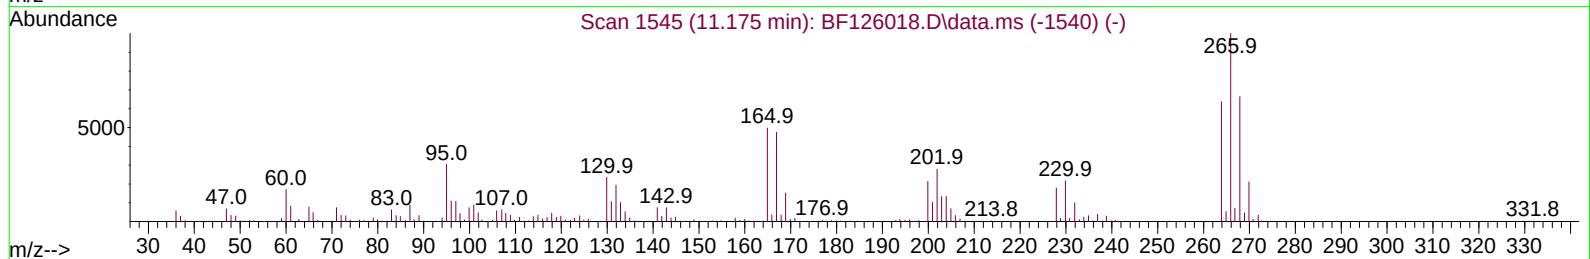
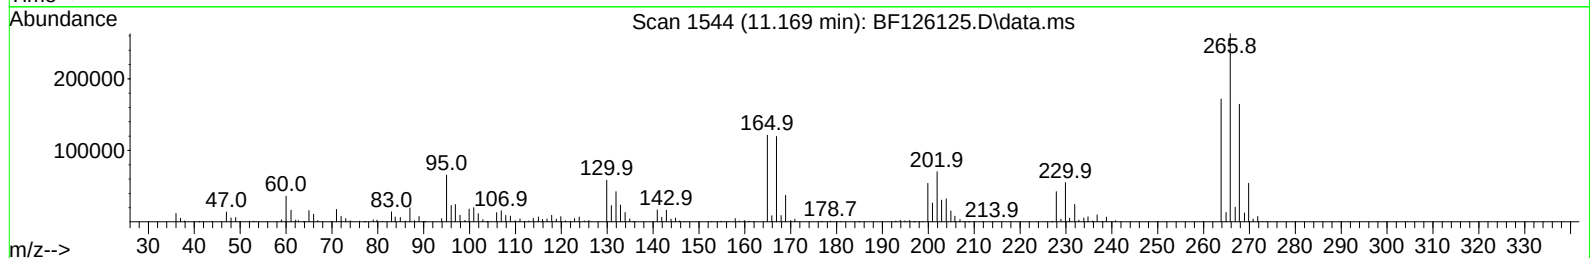


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
Data File : BF126125.D
Acq On : 11 Nov 2021 14:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 15:40:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

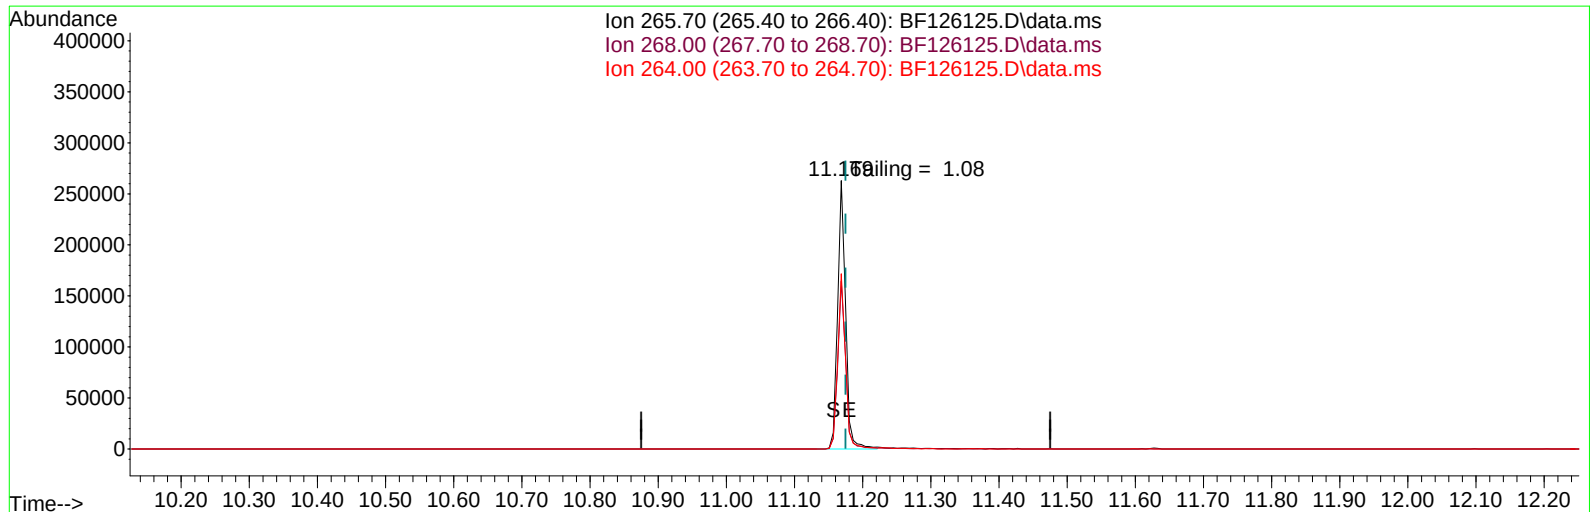

TIC: BF126125.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 23283.41 ng

response 216849

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.55
264.00	69.90	65.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
Data File : BF126125.D
Acq On : 11 Nov 2021 14:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 15:40:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

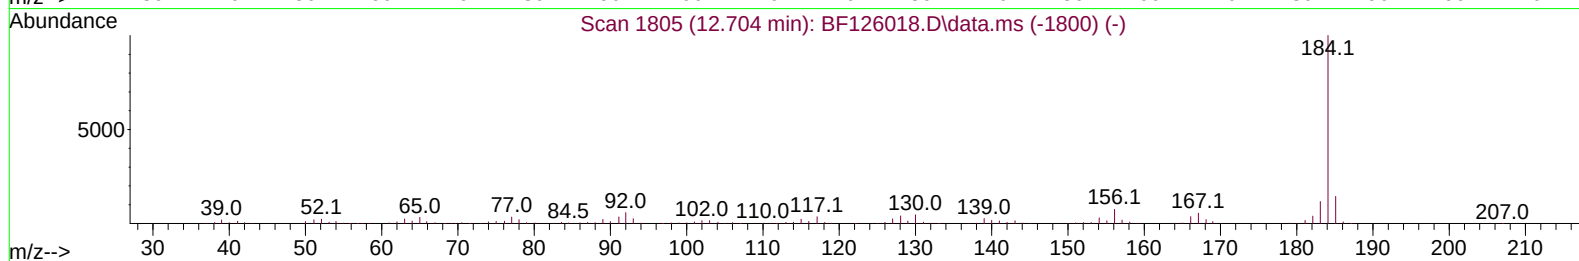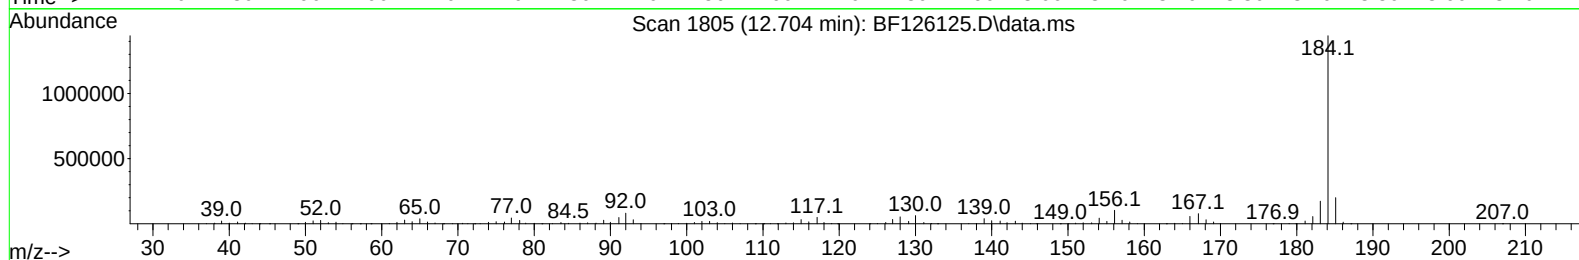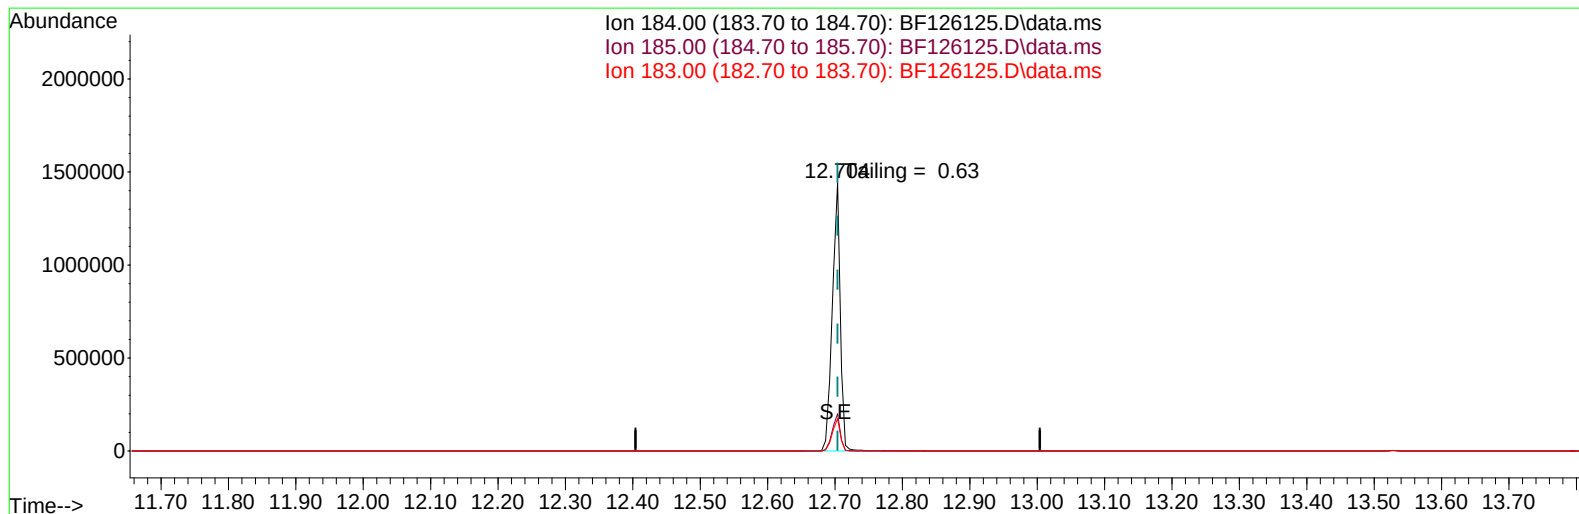

TIC: BF126125.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 1181138

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.89
183.00	10.10	12.06
0.00	0.00	0.00