

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
 Data File : BF126127.D
 Acq On : 11 Nov 2021 15:54
 Operator : JU/CG
 Sample : PB140700BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB140700BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.193	9	18	25	rVB	174047	229045	2.79%	0.503%
2	5.469	569	575	578	rBV	5686211	5755769	70.16%	12.647%
3	6.475	740	746	749	rBV	5379553	5903034	71.96%	12.970%
4	6.840	805	808	812	rBV	1450737	1183464	14.43%	2.600%
5	7.404	898	904	907	rBV	3752678	3852568	46.96%	8.465%
6	8.122	1021	1026	1030	rBV	1652585	1530351	18.65%	3.363%
7	9.204	1204	1210	1213	rBV	8314734	7305367	89.05%	16.052%
8	9.880	1319	1325	1328	rBV	2164417	1856246	22.63%	4.079%
9	10.669	1452	1459	1462	rBV	5749848	5004959	61.01%	10.997%
10	11.363	1572	1577	1581	rBV	2318592	1979073	24.12%	4.349%
11	12.957	1843	1848	1851	rVB	9012862	8203508	100.00%	18.025%
12	14.004	2022	2026	2029	rBV	1917253	1568133	19.12%	3.446%
13	15.468	2270	2275	2279	rBV	924379	1139893	13.90%	2.505%




Sum of corrected areas: 45511410

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
Data File : BF126127.D
Acq On : 11 Nov 2021 15:54
Operator : JU/CG
Sample : PB140700BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB140700BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

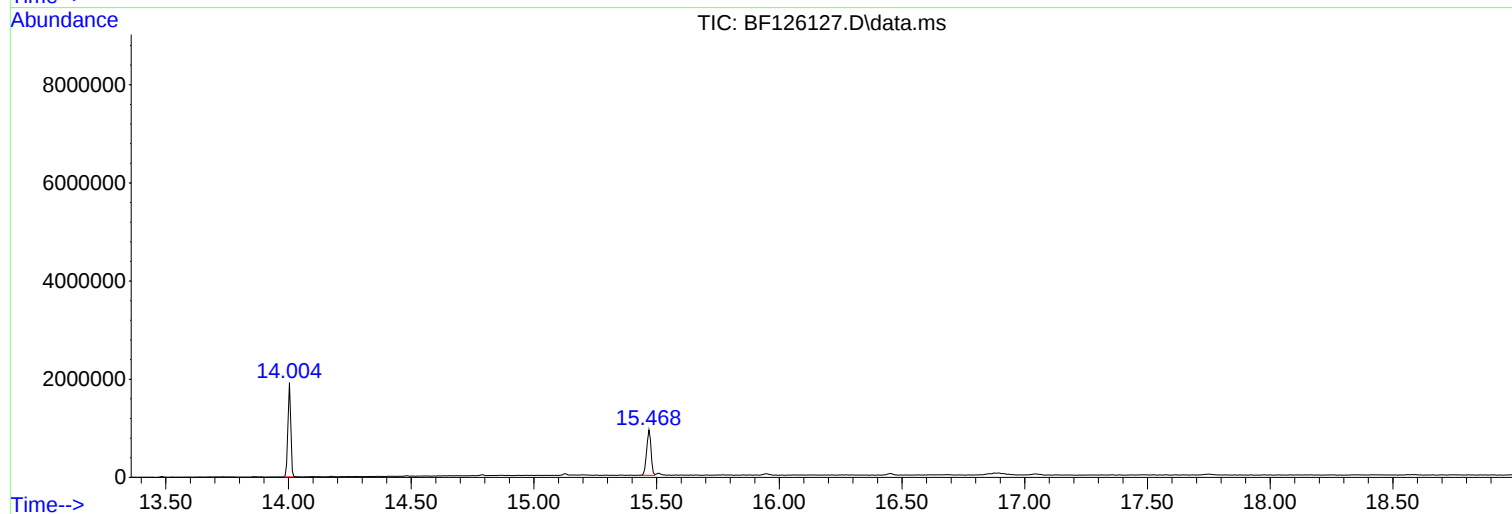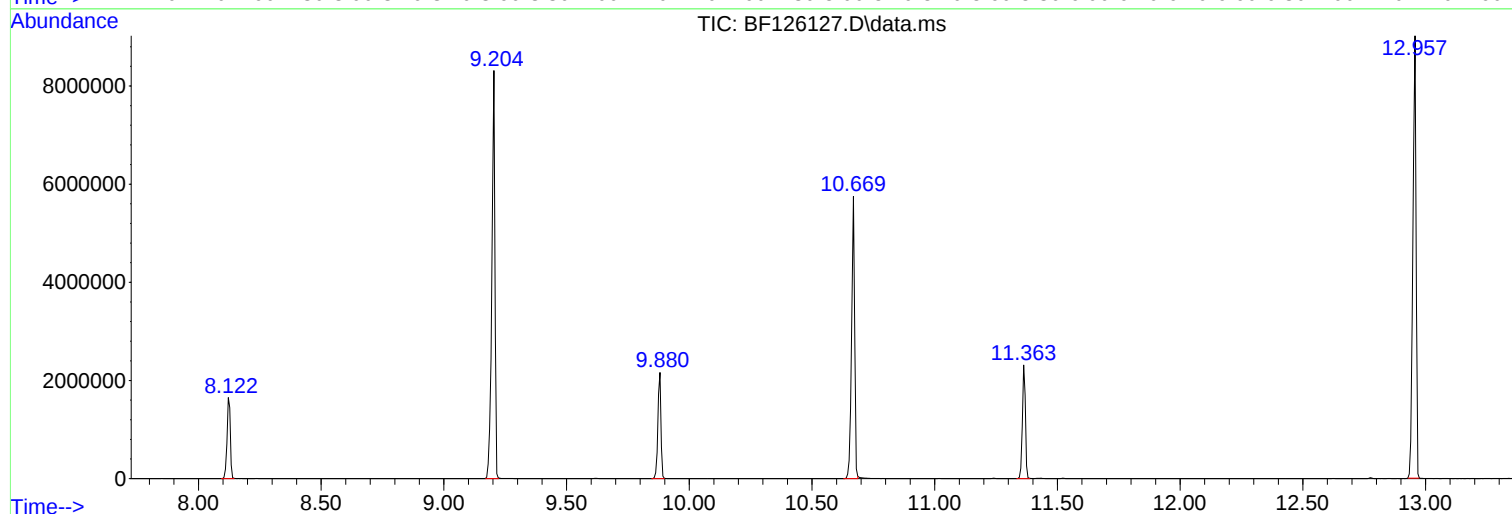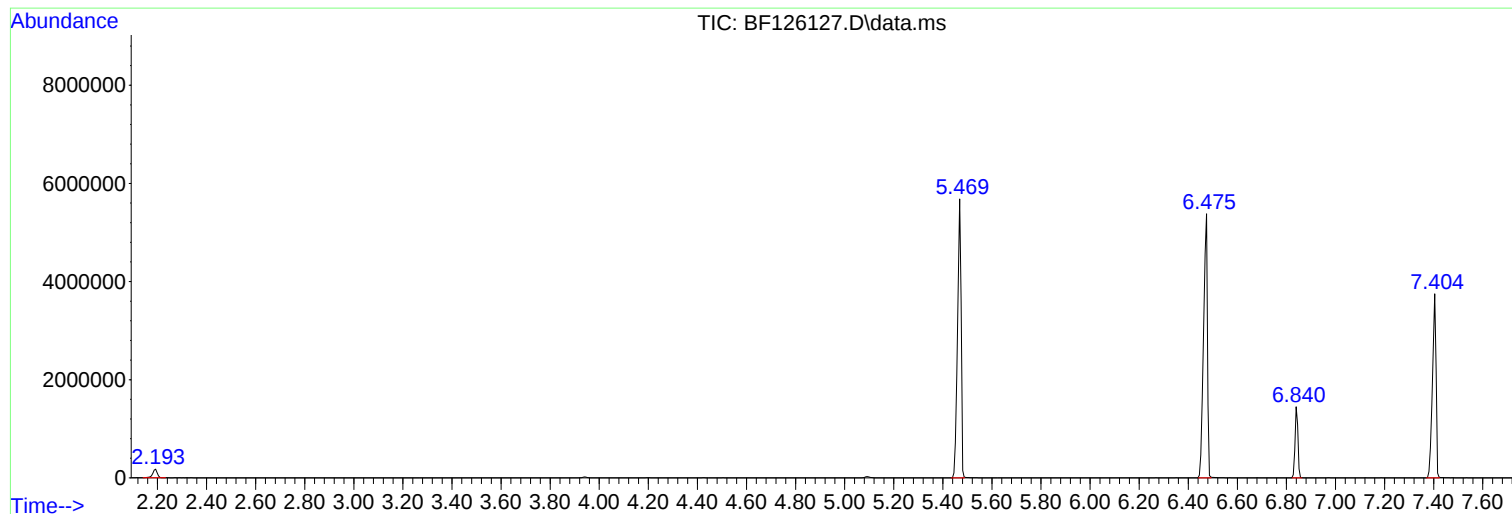

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
Data File : BF126127.D
Acq On : 11 Nov 2021 15:54
Operator : JU/CG
Sample : PB140700BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB140700BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.193	3.87 ng	229045	1,4-Dichlorobenzene-d4	6.840

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	25
4			Boronic acid, ethyl-, dimethyl e...	102	C4H11BO2	007318-82-3	16
5			Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

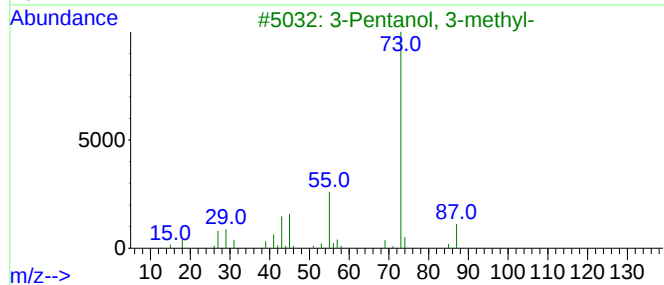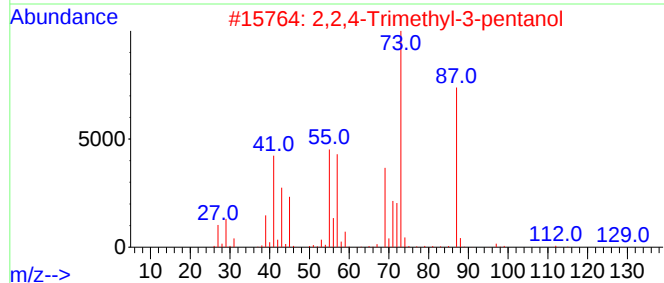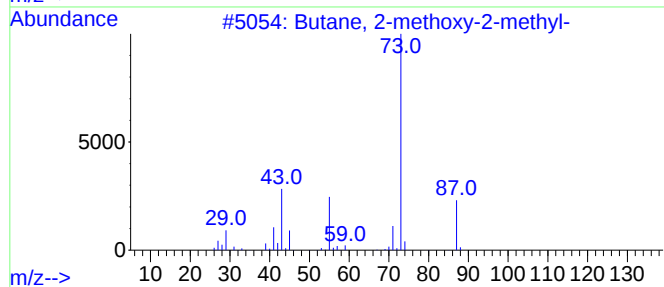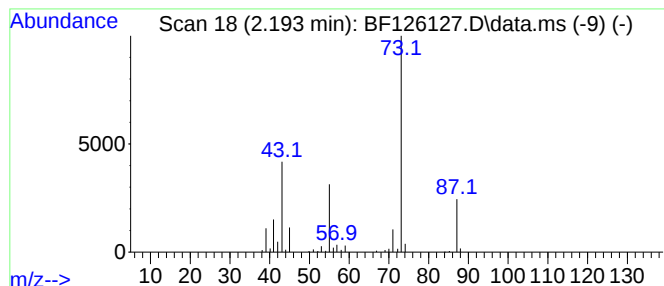

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
Data File : BF126127.D
Acq On : 11 Nov 2021 15:54
Operator : JU/CG
Sample : PB140700BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB140700BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.193	3.9	ng	229045	1	6.840	1183460	20.0