
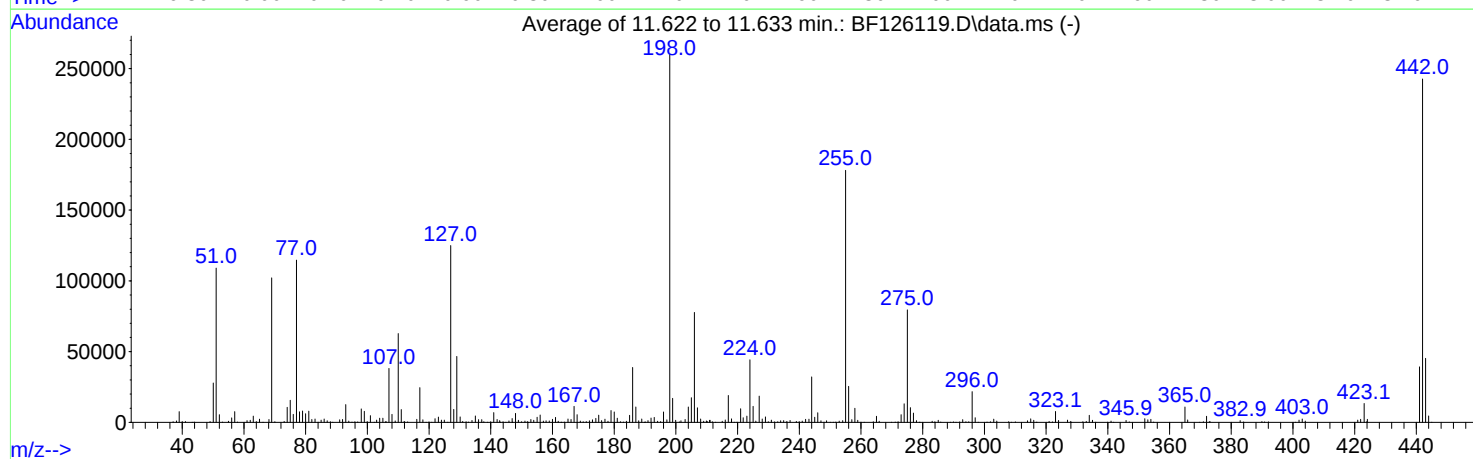


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
 Data File : BF126119.D
 Acq On : 11 Nov 2021 10:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 14:29:48 2021

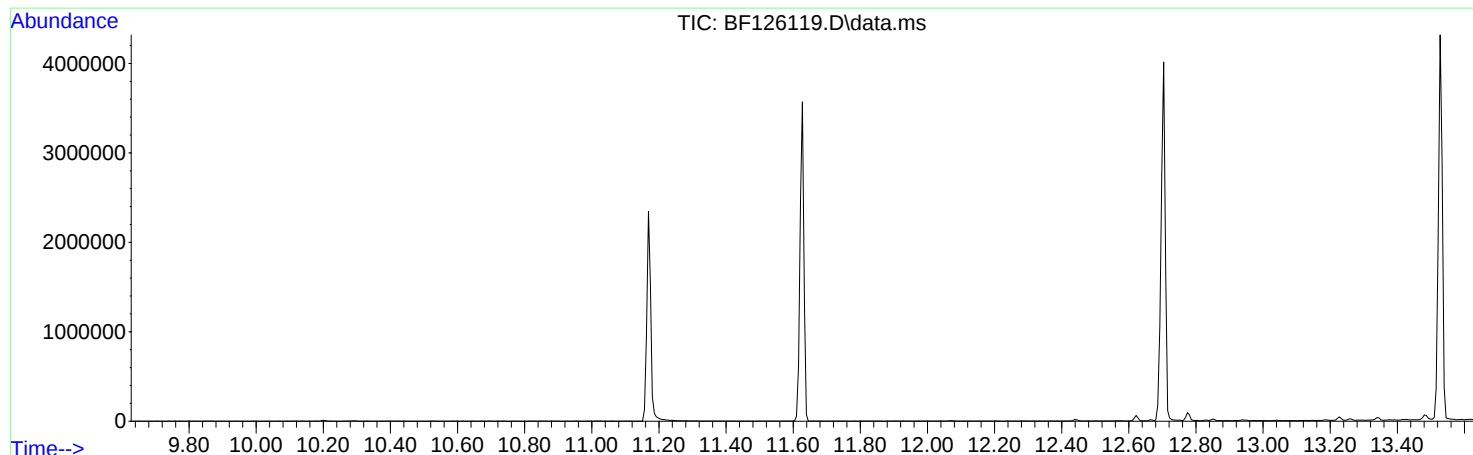




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	109016	PASS
68	69	0.00	2	2.0	2078	PASS
69	198	0.00	100	39.3	102101	PASS
70	69	0.00	2	0.4	402	PASS
127	198	10	80	48.1	124955	PASS
197	198	0.00	2	0.7	1800	PASS
198	198	100	100	100.0	259973	PASS
199	198	5	9	6.5	16999	PASS
275	198	10	60	30.6	79536	PASS
365	198	1	100	4.2	10839	PASS
441	198	0.01	100	15.1	39197	PASS
442	442	50	100	100.0	242667	PASS
443	442	15	24	18.6	45208	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
Data File : BF126119.D
Acq On : 11 Nov 2021 10:32
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 11 12:55:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

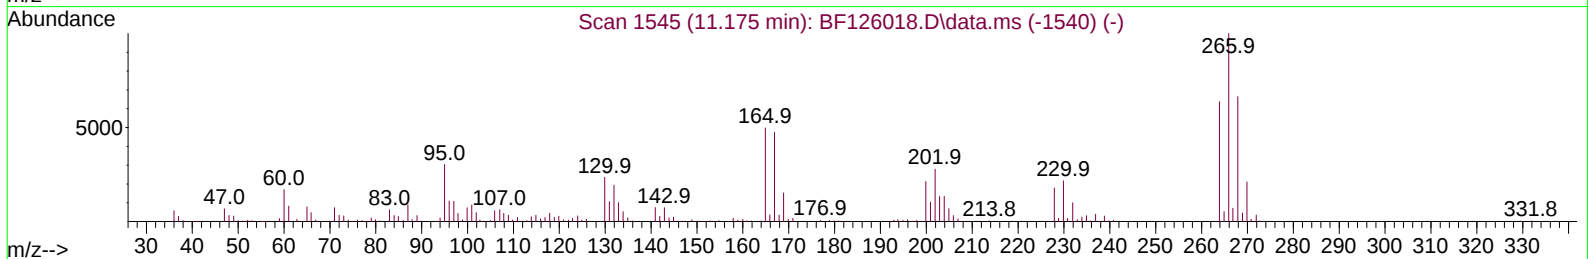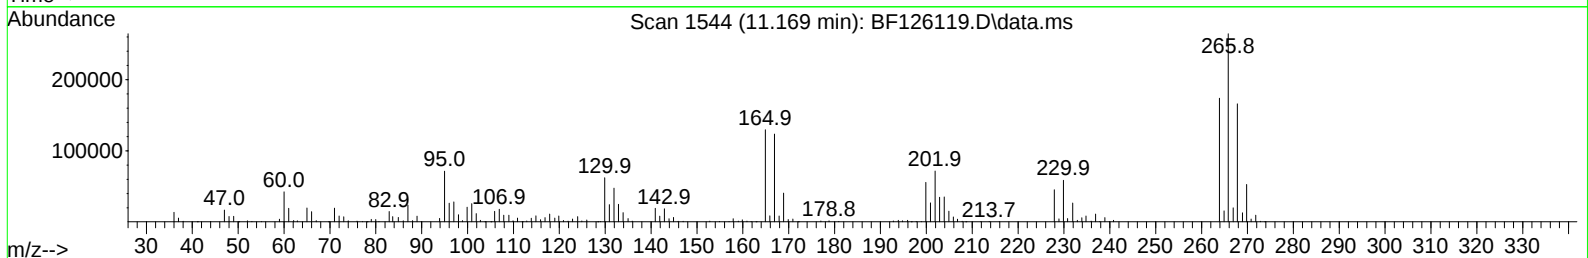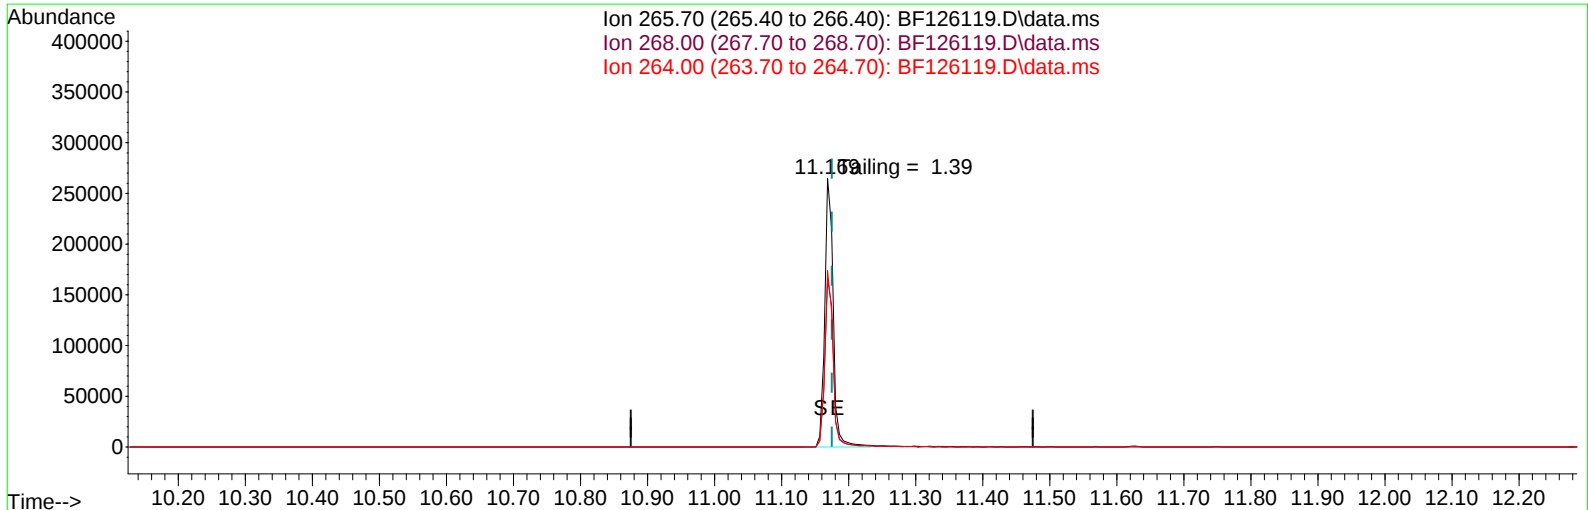

TIC: BF126119.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 28491.47 ng




response 234273

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.75
264.00	69.90	65.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111121\
Data File : BF126119.D
Acq On : 11 Nov 2021 10:32
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 11 12:55:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 17:21:25 2021
Response via : Initial Calibration

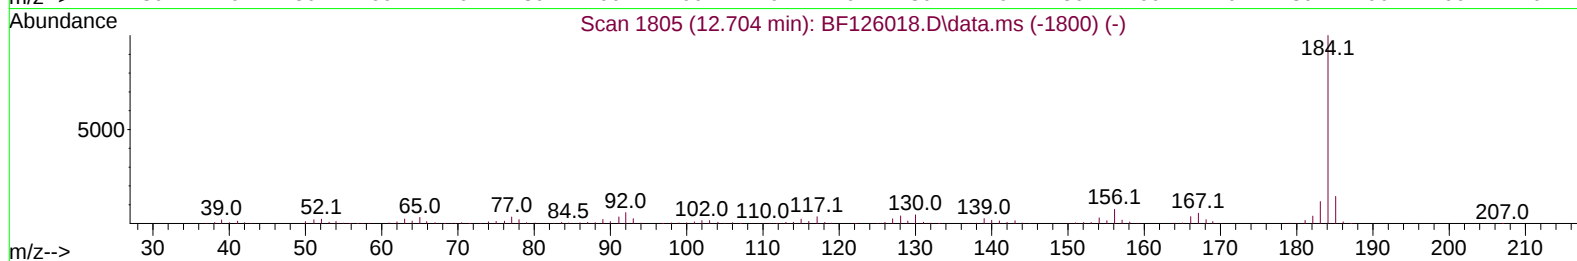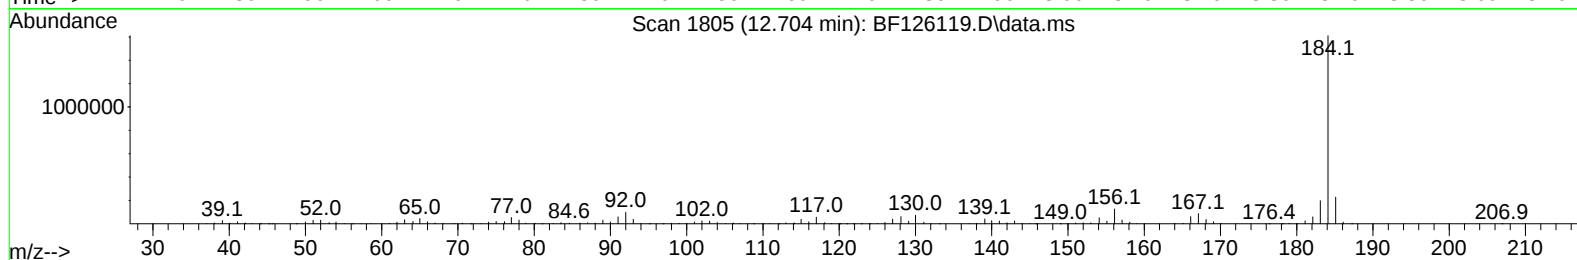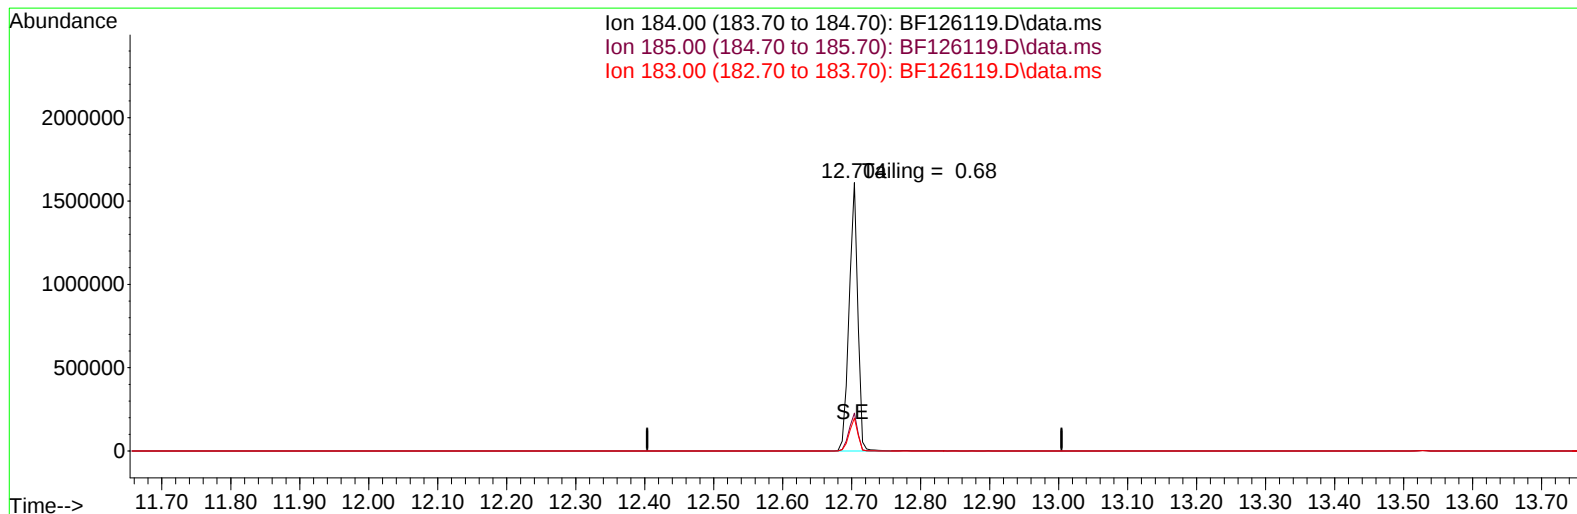

TIC: BF126119.D\data.ms

(77) Benzidine

12.704min (-0.000) 341137.85 ng m

response 1391274

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.18
183.00	10.10	12.27#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2021	BNA_F	<u>BF126119.D</u>
Compound Name	Response	Retention Time
DDT	680523	13.52
DDD	7098	13.22
DDE	494	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7592	688115	1.10

Instrument :
BNA_F
ClientSampleId :
DFTPP