


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111121\  
 Data File : BF126125.D  
 Acq On : 11 Nov 2021 14:46  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110321.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Nov 15 14:29:48 2021

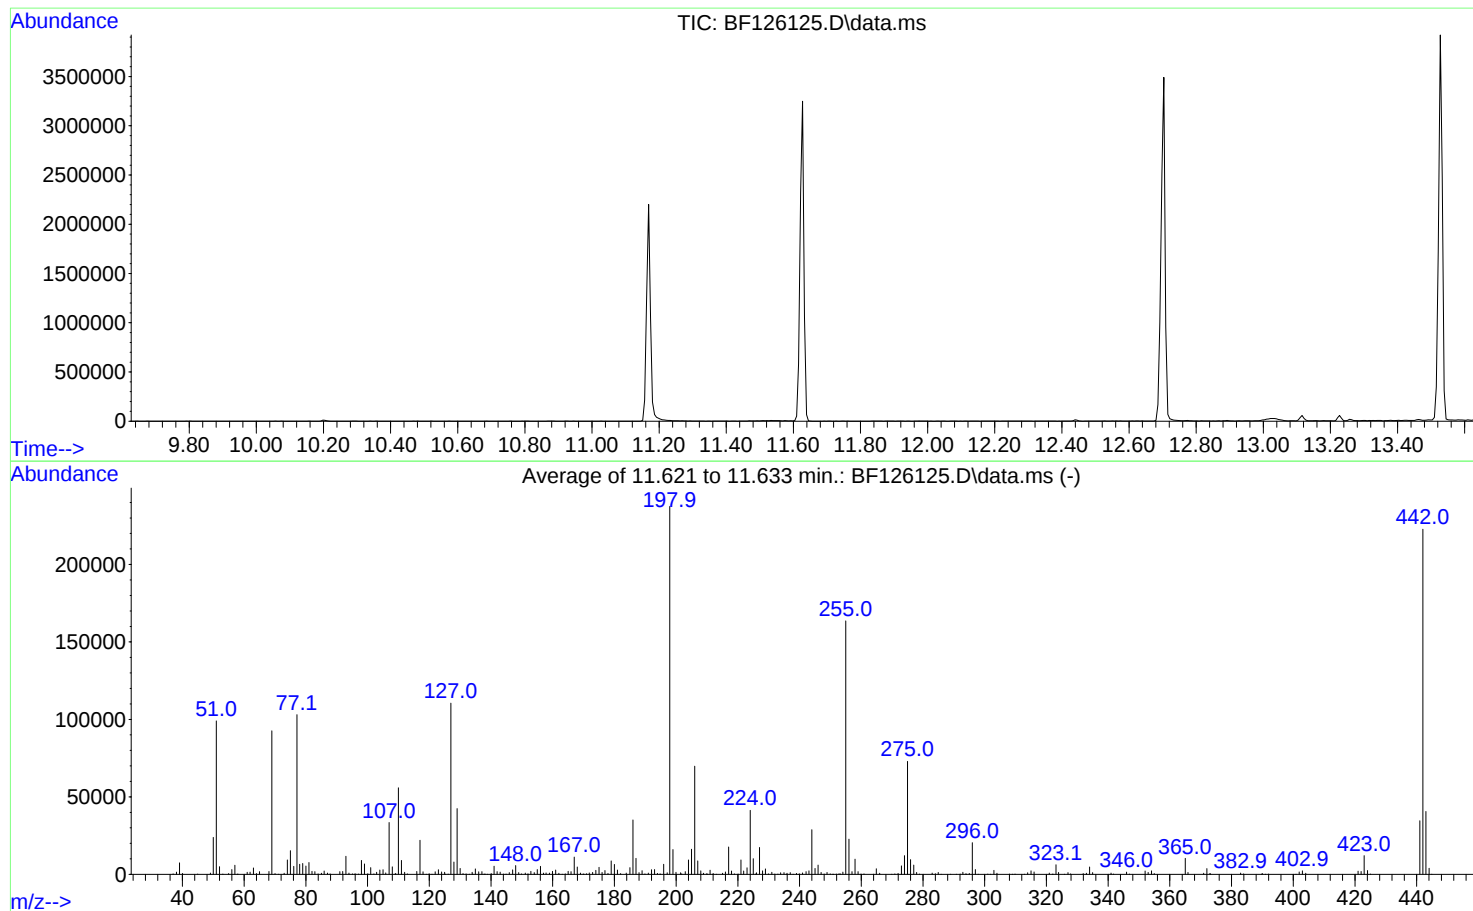




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.7         | 99005      | PASS                |
| 68             | 69              | 0.00            | 2               | 2.0          | 1821       | PASS                |
| 69             | 198             | 0.00            | 100             | 39.0         | 92672      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 525        | PASS                |
| 127            | 198             | 10              | 80              | 46.5         | 110440     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 1016       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 237397     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 15997      | PASS                |
| 275            | 198             | 10              | 60              | 30.7         | 72957      | PASS                |
| 365            | 198             | 1               | 100             | 4.3          | 10326      | PASS                |
| 441            | 198             | 0.01            | 100             | 14.6         | 34560      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 222771     | PASS                |
| 443            | 442             | 15              | 24              | 18.2         | 40587      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111121\  
 Data File : BF126125.D  
 Acq On : 11 Nov 2021 14:46  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Nov 11 15:40:48 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110321.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Nov 03 17:21:25 2021  
 Response via : Initial Calibration

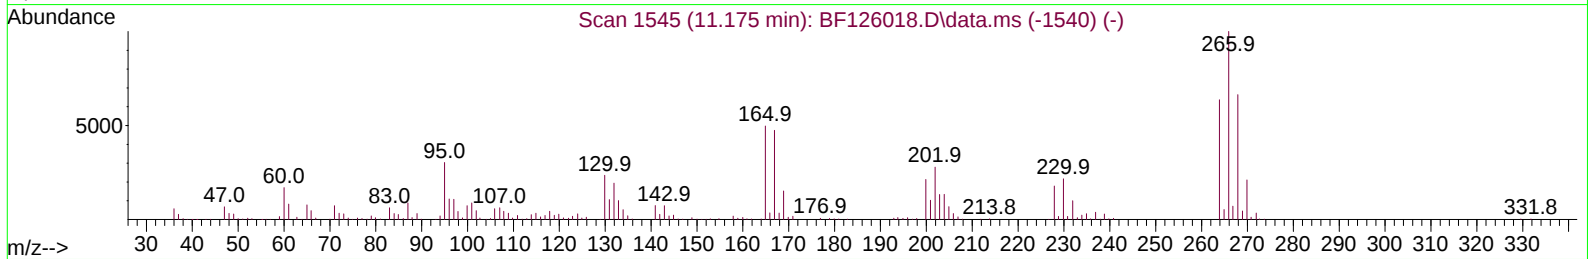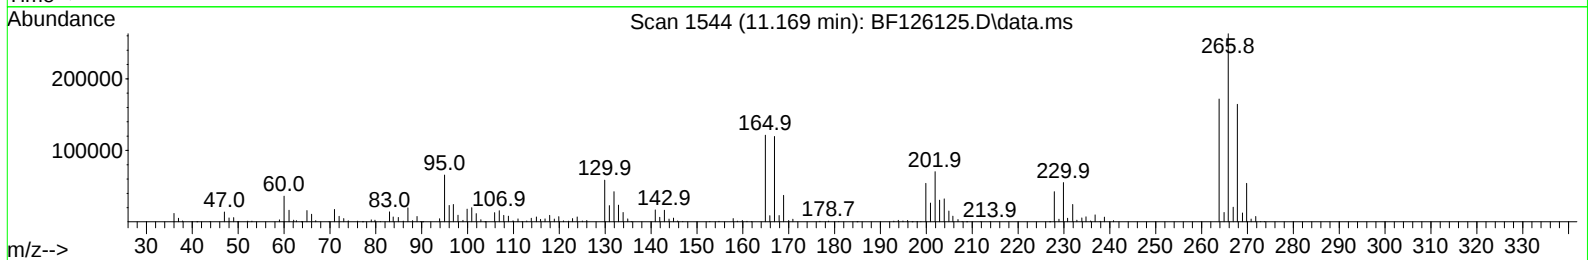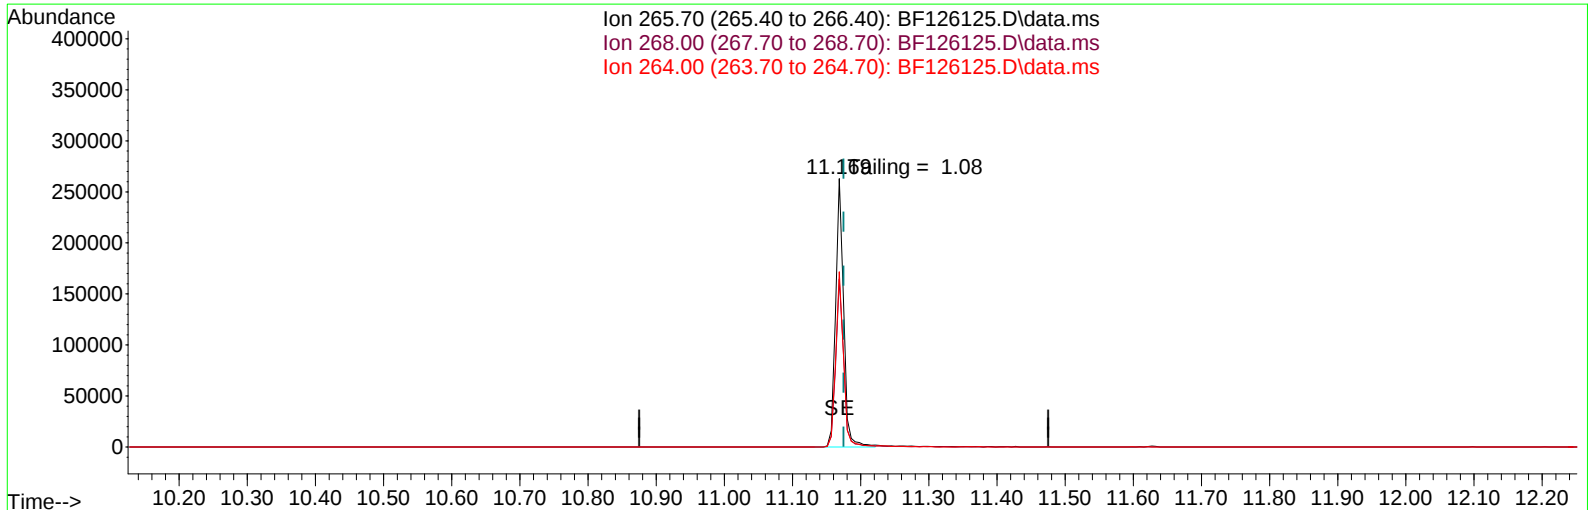

TIC: BF126125.D\data.ms

**(70) Pentachlorophenol (C)**

**11.169min (-0.006) 23283.41 ng**




**response 216849**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.10  | 62.55  |
| 264.00 | 69.90  | 65.30  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111121\  
Data File : BF126125.D  
Acq On : 11 Nov 2021 14:46  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 11 15:40:48 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 03 17:21:25 2021  
Response via : Initial Calibration

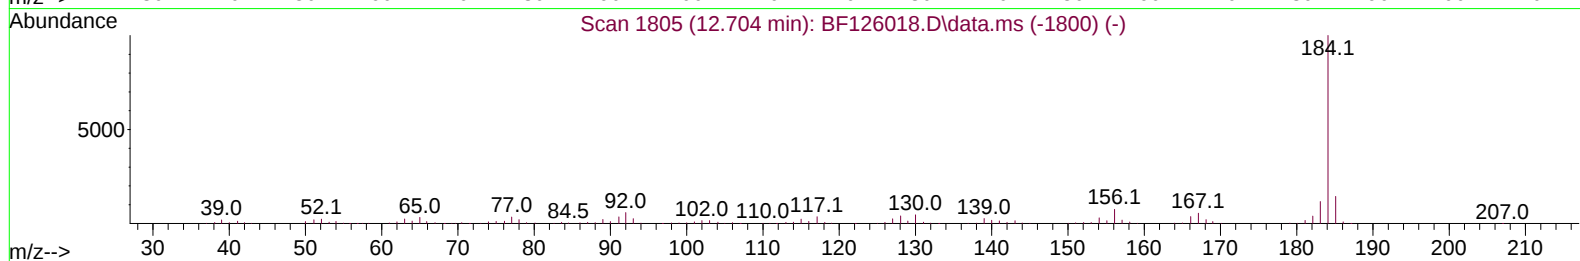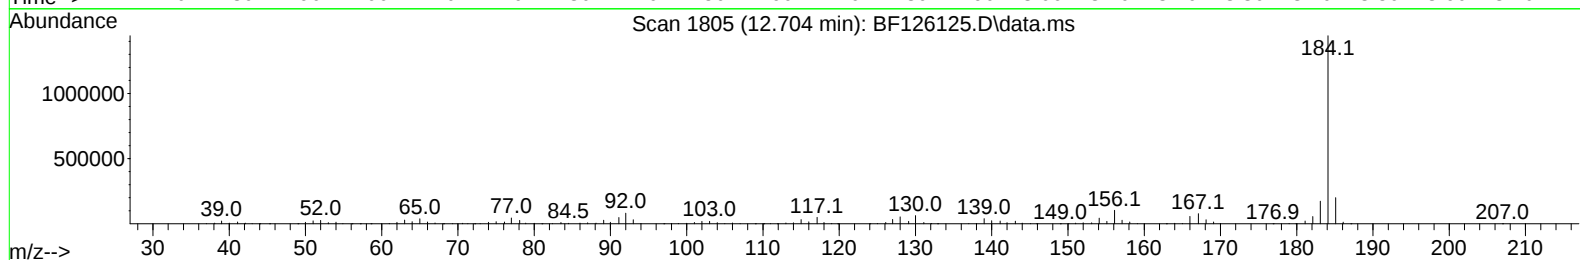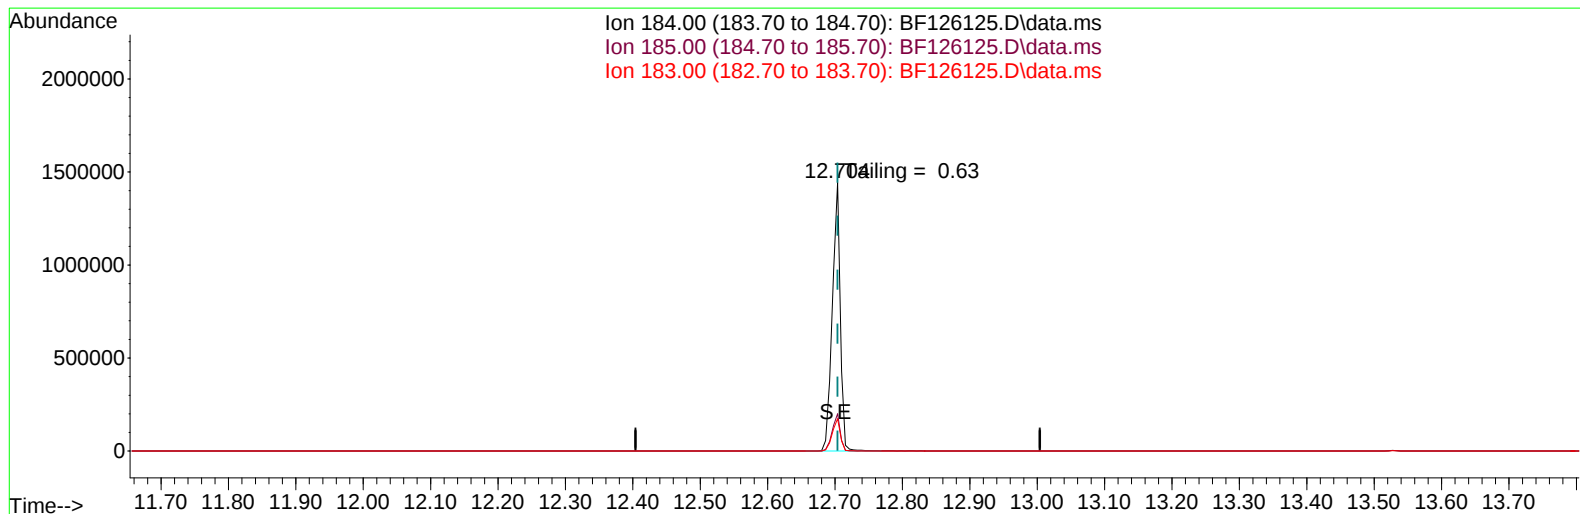

TIC: BF126125.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 1181138

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 13.89  |
| 183.00 | 10.10  | 12.06  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/11/2021    | BNA_F            | <u>BF126125.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 607255           | 13.52              |
| DDD           | 8453             | 13.22              |
| DDE           | 857              | 12.89              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 9310          | 616565           | 1.51               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP