
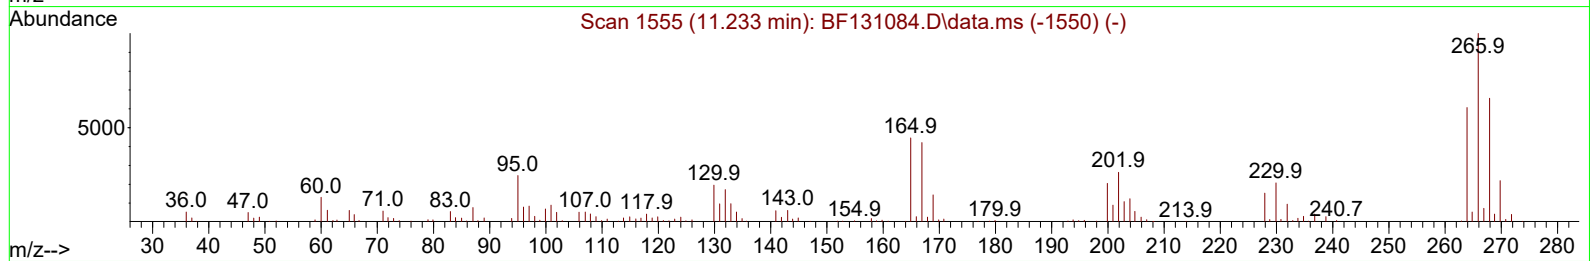
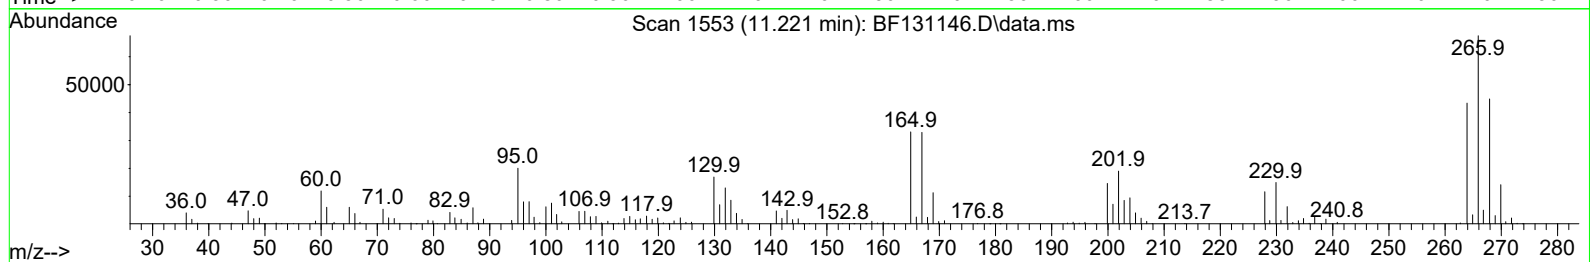


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
Data File : BF131146.D
Acq On : 11 Nov 2022 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 14:38:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

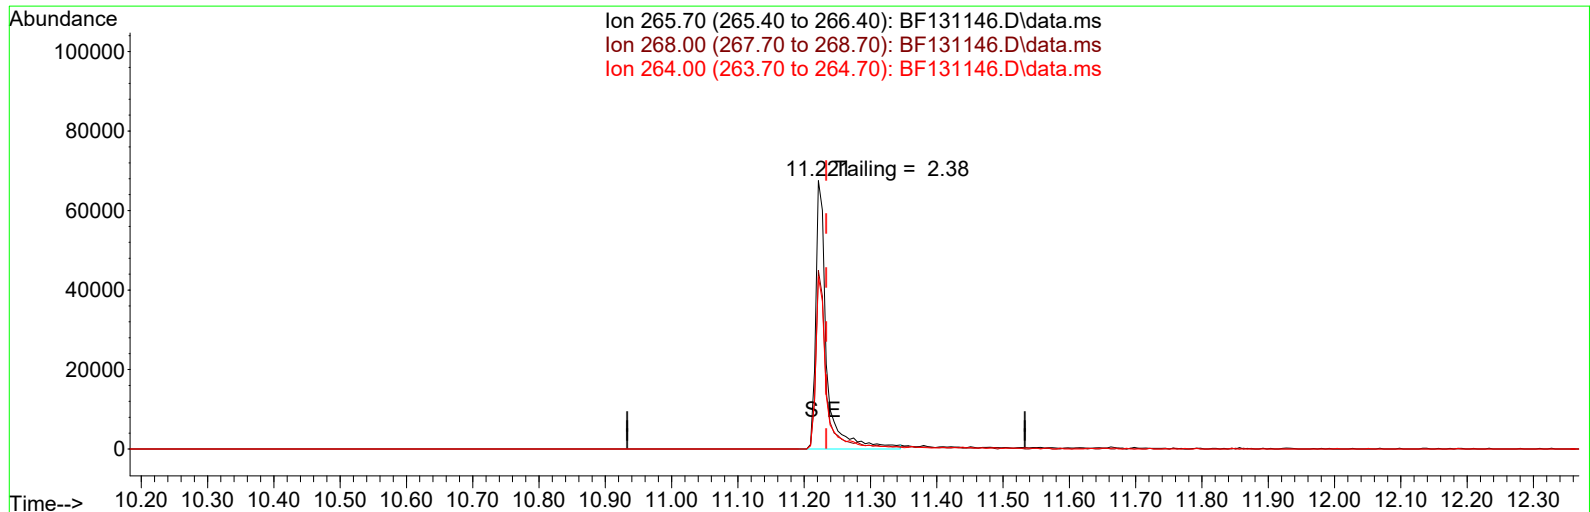

TIC: BF131146.D\data.ms

(70) Pentachlorophenol (C)




11.221min (-0.012) 25619.53 ng

response 77979

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	66.50
264.00	60.70	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
Data File : BF131146.D
Acq On : 11 Nov 2022 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 14:38:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

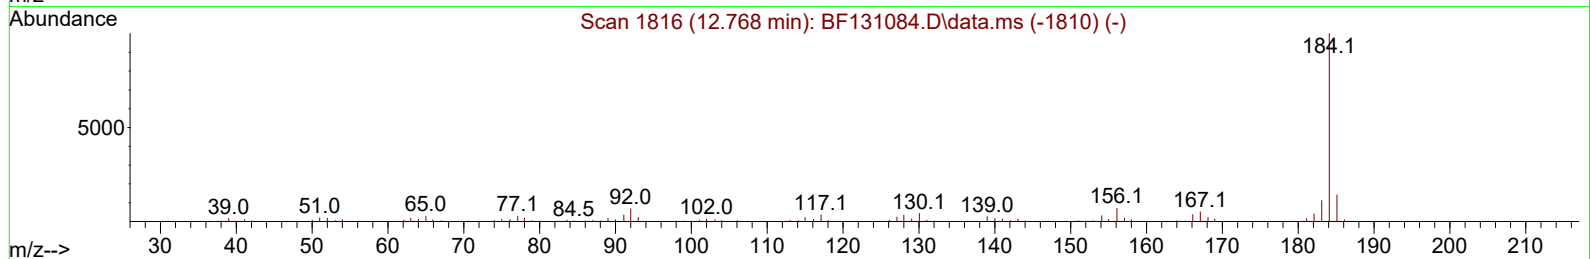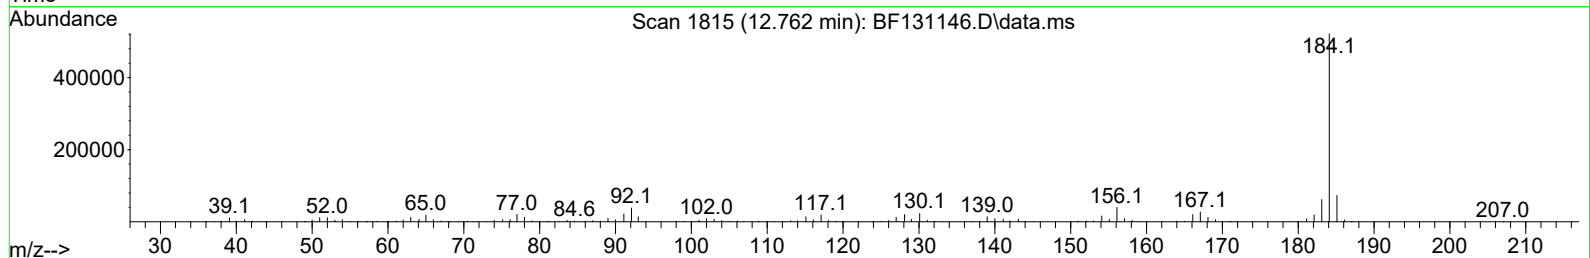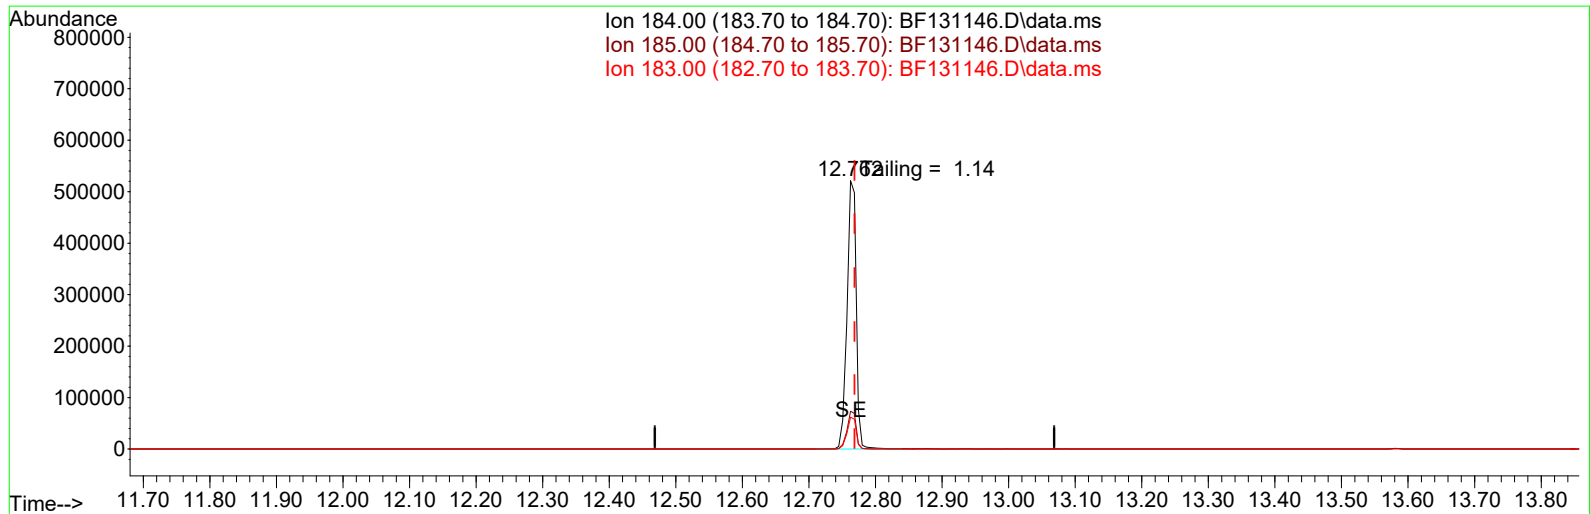

TIC: BF131146.D\data.ms

(77) Benzidine

12.762min (-0.006) 0.00 ng

response 503933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.06
183.00	11.20	11.86
0.00	0.00	0.00