
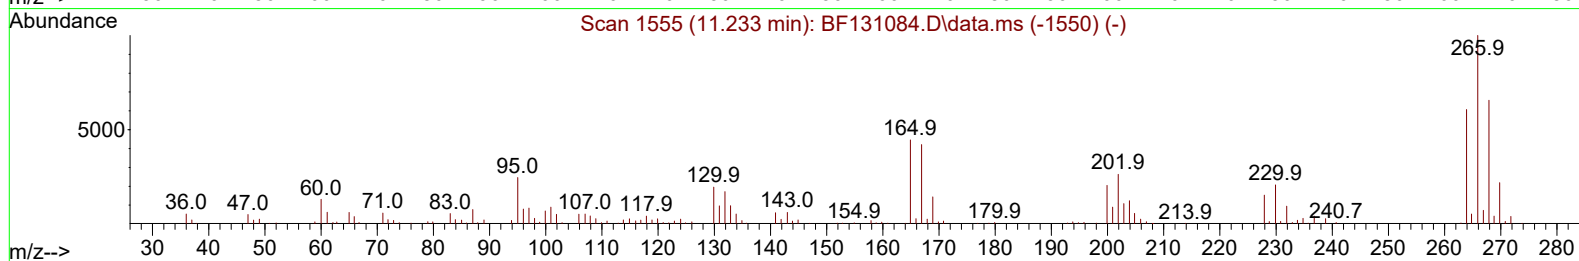
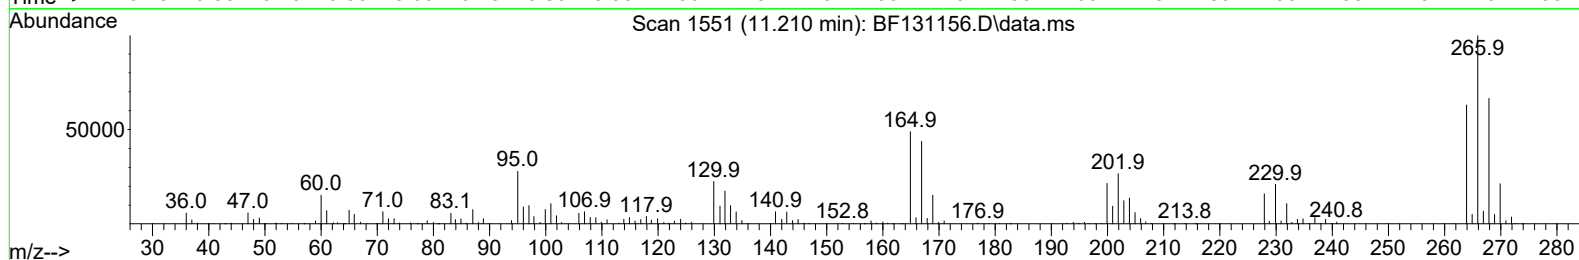


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
Data File : BF131156.D
Acq On : 11 Nov 2022 16:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 17:50:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

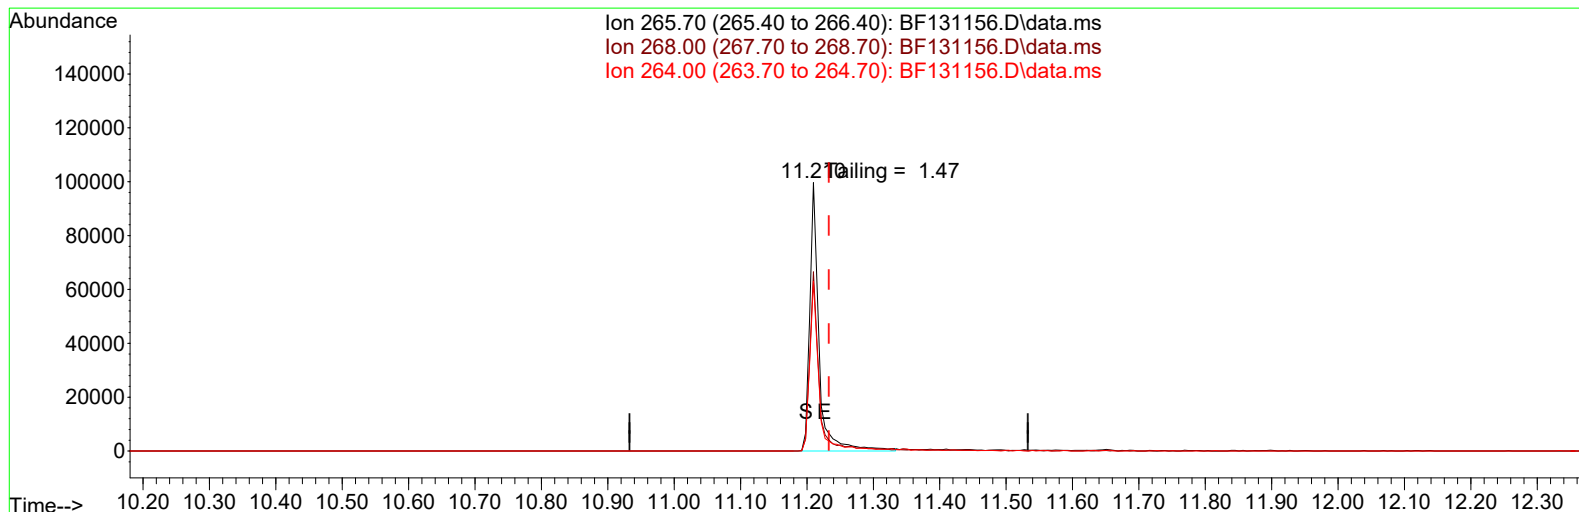

TIC: BF131156.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.023) 47683.29 ng

response 98083

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	66.81
264.00	60.70	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
Data File : BF131156.D
Acq On : 11 Nov 2022 16:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 17:50:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

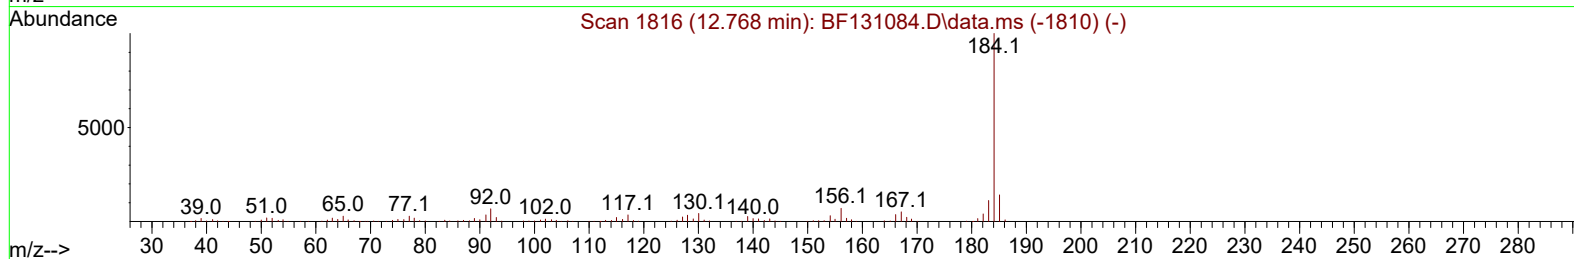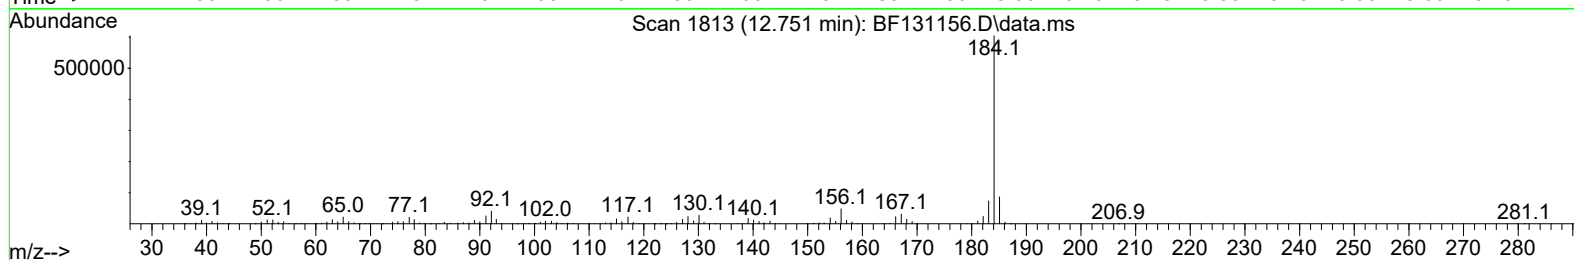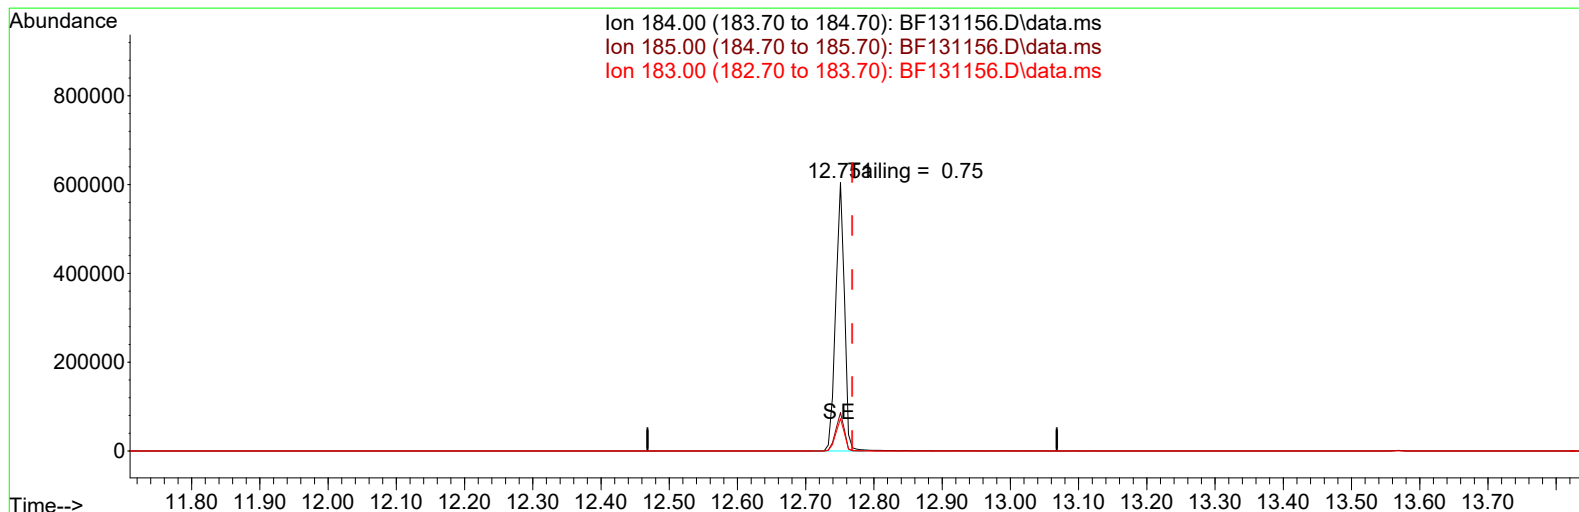

TIC: BF131156.D\data.ms

(77) Benzidine

12.751min (-0.018) 21153.13 ng

response 542303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.32
183.00	11.20	12.09
0.00	0.00	0.00