


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
 Data File : BF131146.D
 Acq On : 11 Nov 2022 10:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 12 00:03:31 2022

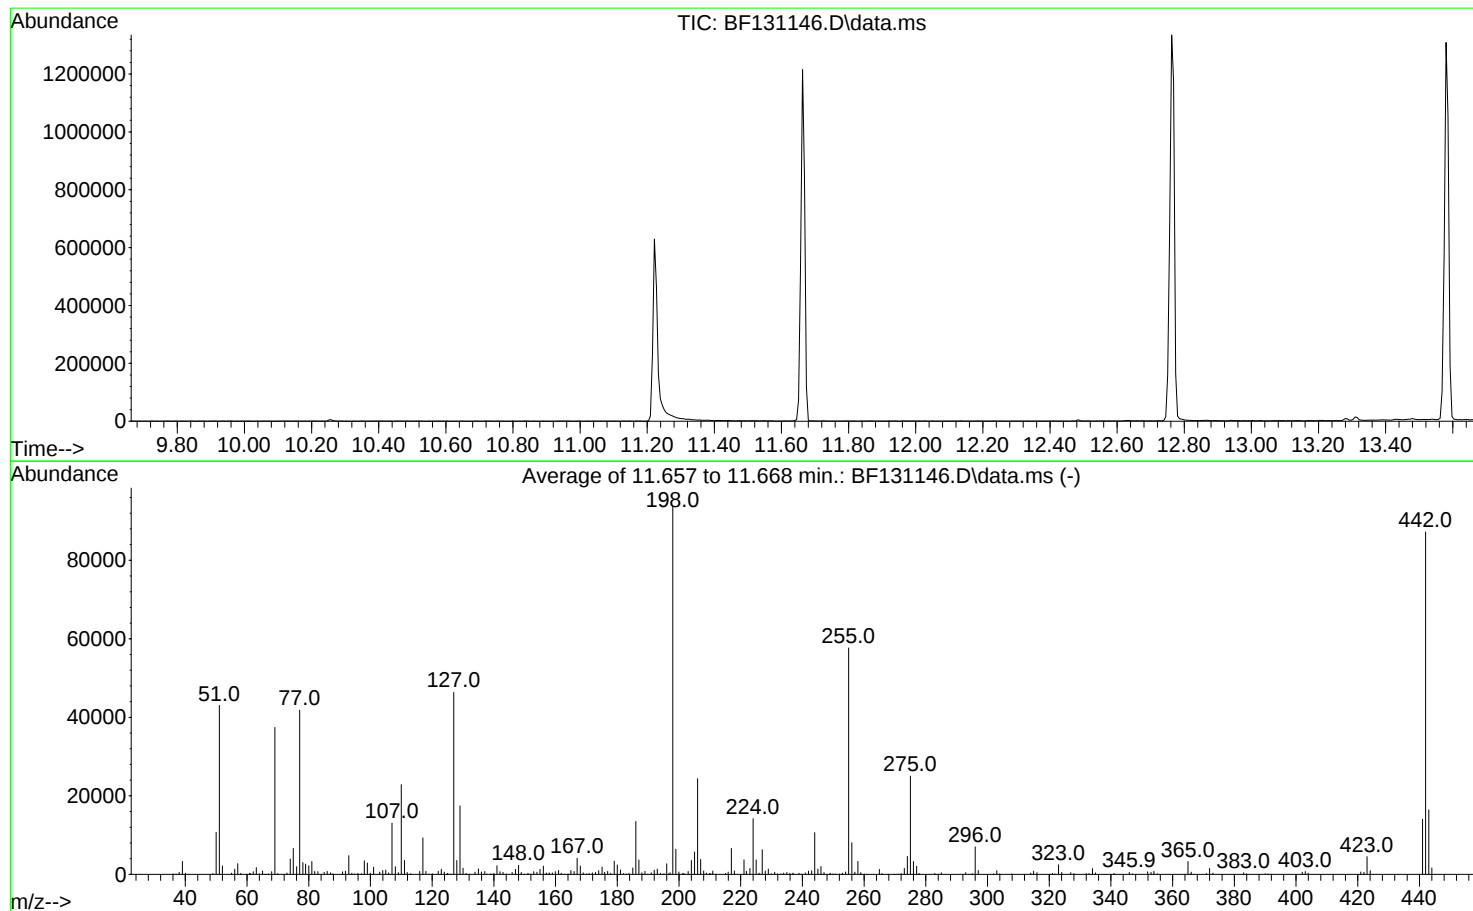




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	43040	PASS
68	69	0.00	2	1.9	701	PASS
69	198	0.00	100	39.9	37408	PASS
70	69	0.00	2	0.6	225	PASS
127	198	10	80	49.5	46363	PASS
197	198	0.00	2	0.4	417	PASS
198	198	100	100	100.0	93712	PASS
199	198	5	9	6.8	6396	PASS
275	198	10	60	26.7	25025	PASS
365	198	1	100	3.5	3290	PASS
441	198	0.01	100	15.0	14041	PASS
442	442	50	100	100.0	87213	PASS
443	442	15	24	18.8	16417	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
Data File : BF131146.D
Acq On : 11 Nov 2022 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 11 14:38:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

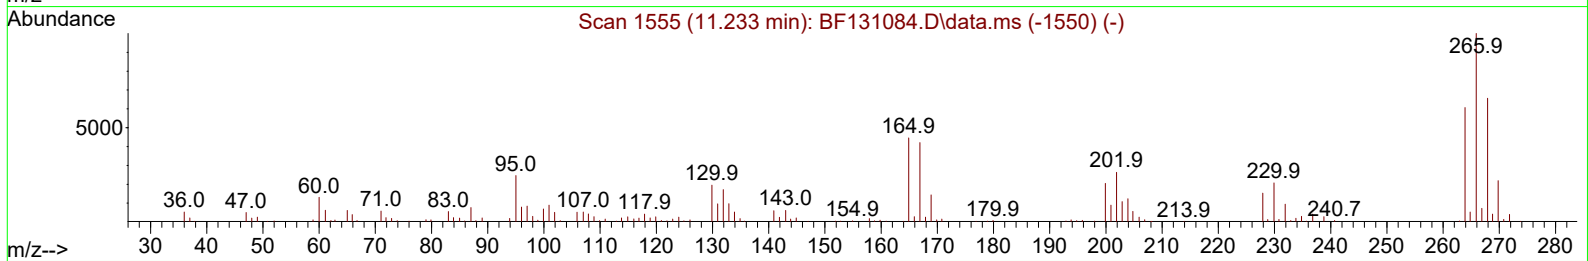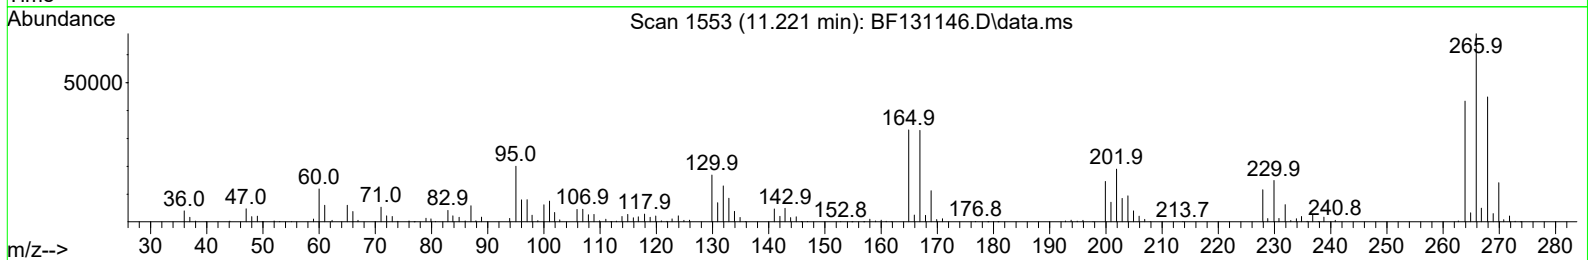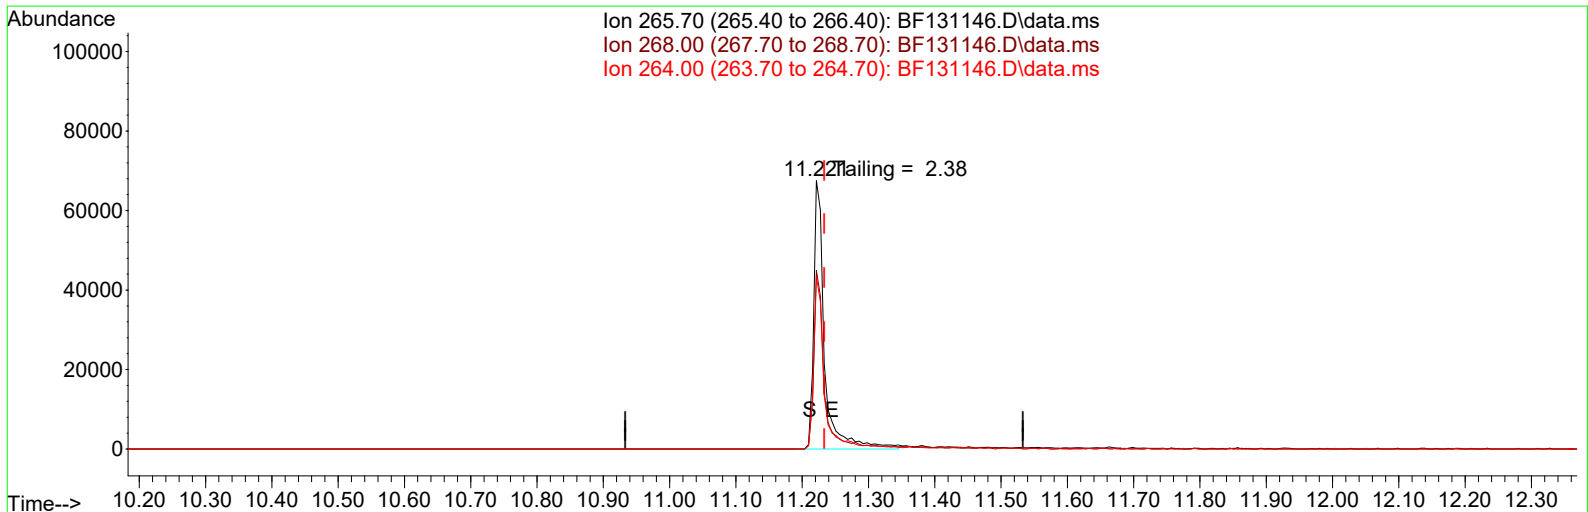

TIC: BF131146.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.012) 25619.53 ng




response 77979

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	66.50
264.00	60.70	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
Data File : BF131146.D
Acq On : 11 Nov 2022 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 11 14:38:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

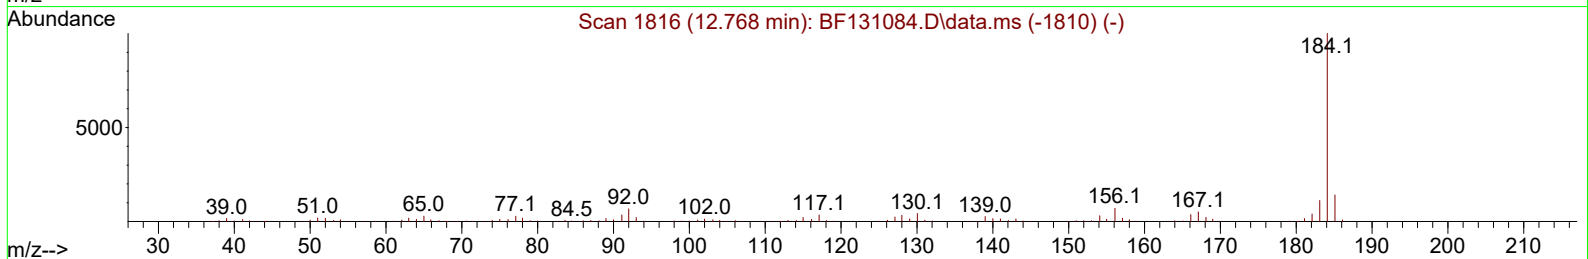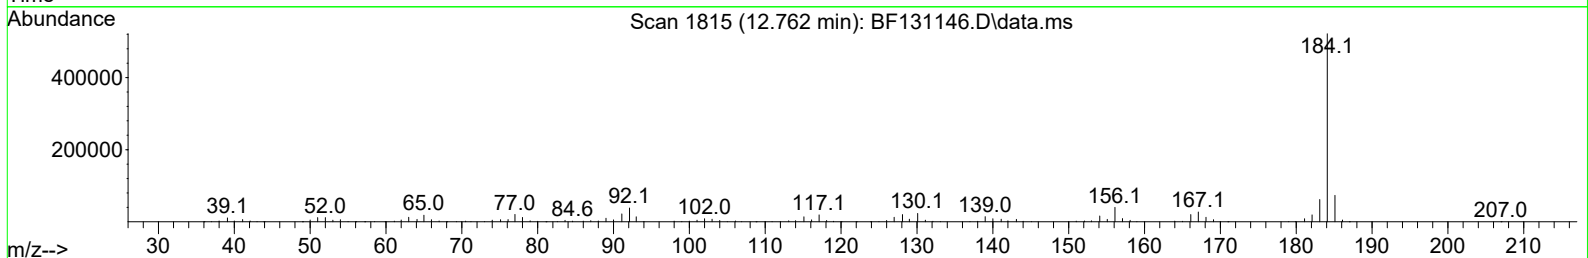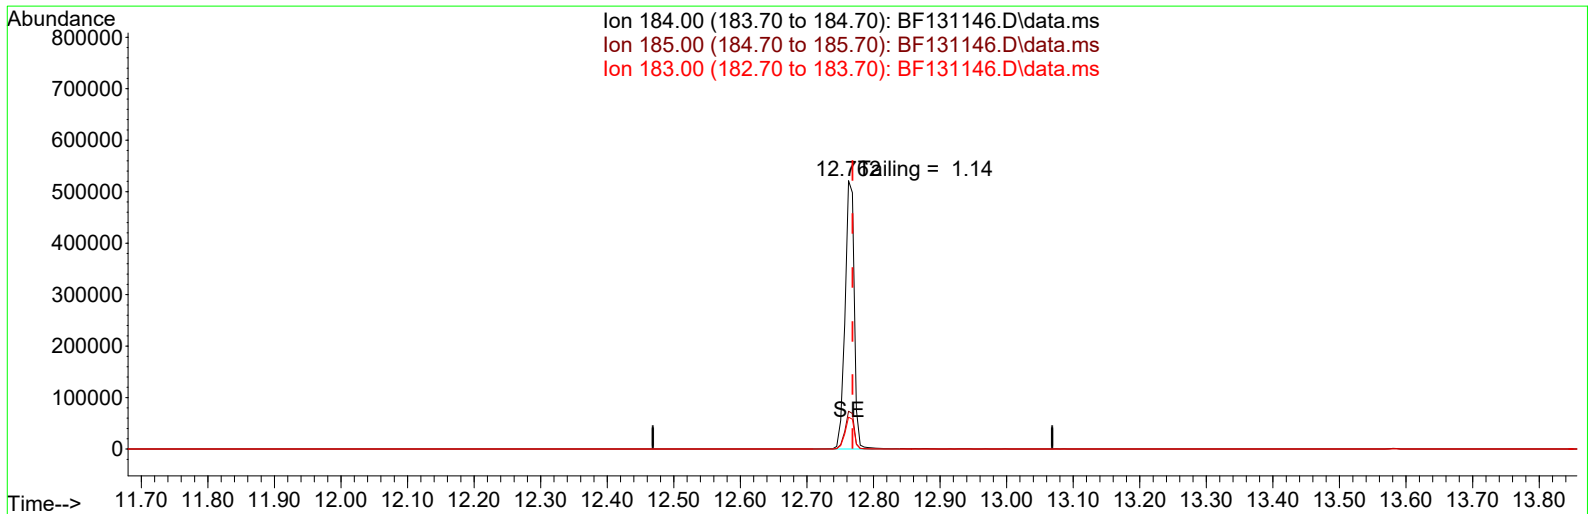

TIC: BF131146.D\data.ms

(77) Benzidine

12.762min (-0.006) 0.00 ng

response 503933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.06
183.00	11.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2022	BNA_F	<u>BF131146.D</u>
Compound Name	Response	Retention Time
DDT	223774	13.58
DDD	4316	13.315
DDE	393	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4709	228483	2.06

Instrument :
BNA_F
ClientSampleId :
DFTPP