


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
 Data File : BF131156.D
 Acq On : 11 Nov 2022 16:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 12 00:03:31 2022

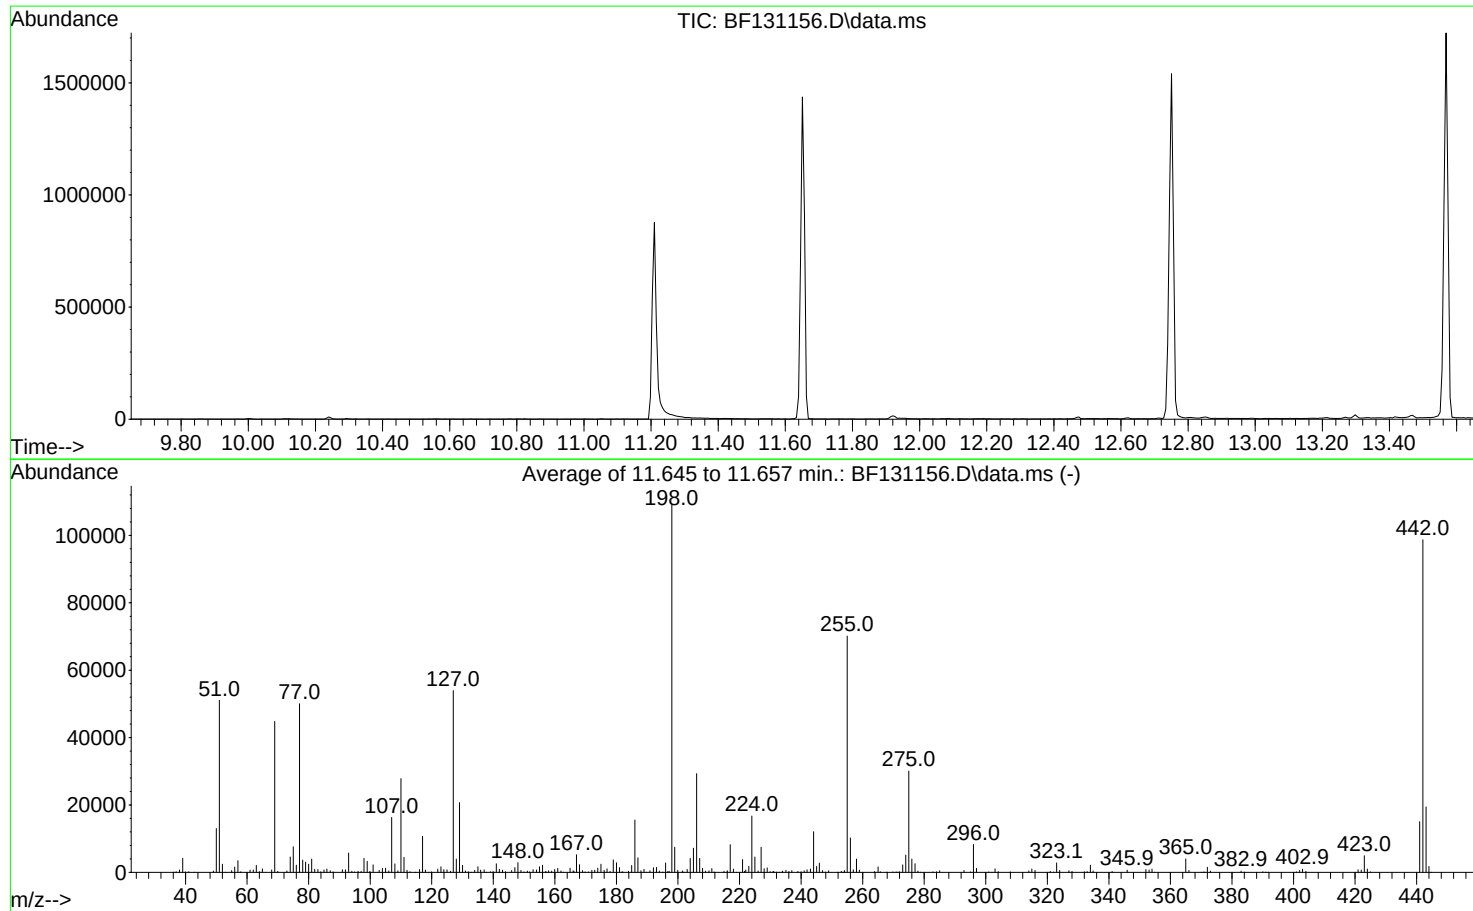




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	51043	PASS
68	69	0.00	2	1.6	728	PASS
69	198	0.00	100	41.0	44797	PASS
70	69	0.00	2	0.6	276	PASS
127	198	10	80	49.4	53952	PASS
197	198	0.00	2	0.3	330	PASS
198	198	100	100	100.0	109173	PASS
199	198	5	9	6.8	7462	PASS
275	198	10	60	27.5	30043	PASS
365	198	1	100	3.7	3986	PASS
441	198	0.01	100	13.8	15071	PASS
442	442	50	100	100.0	98744	PASS
443	442	15	24	19.7	19443	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
Data File : BF131156.D
Acq On : 11 Nov 2022 16:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 11 17:50:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

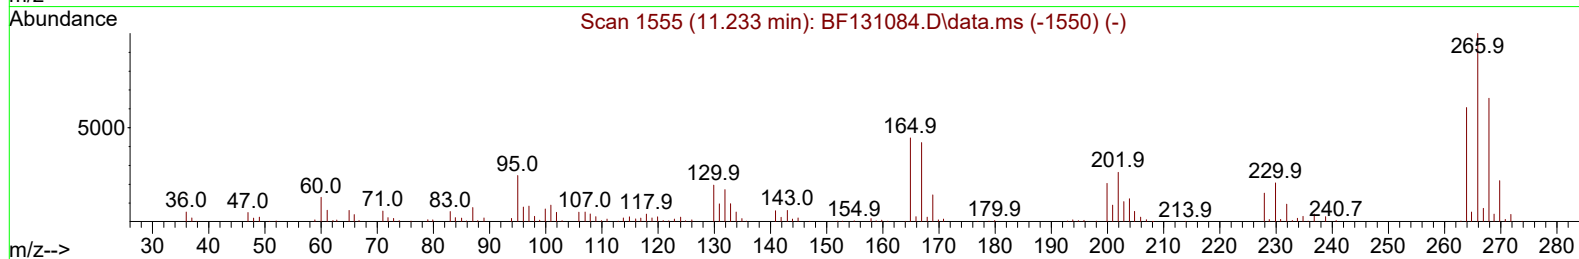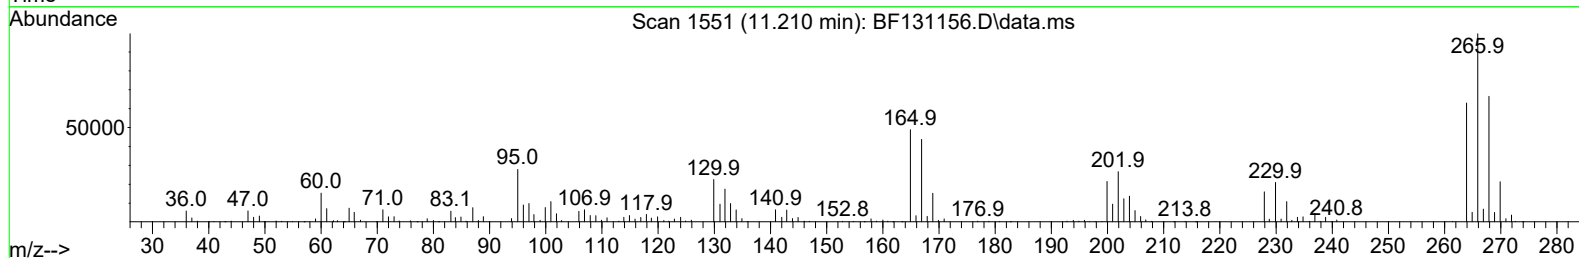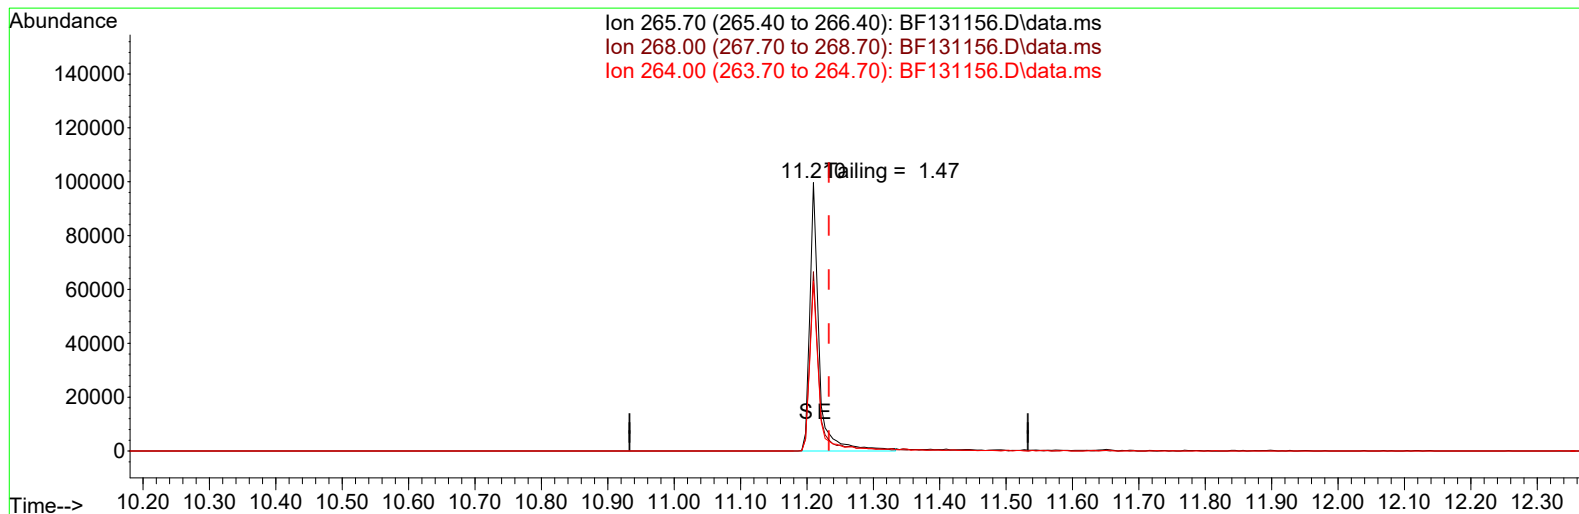

TIC: BF131156.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.023) 47683.29 ng




response 98083

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	66.81
264.00	60.70	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111122\
Data File : BF131156.D
Acq On : 11 Nov 2022 16:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 11 17:50:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 04:15:17 2022
Response via : Initial Calibration

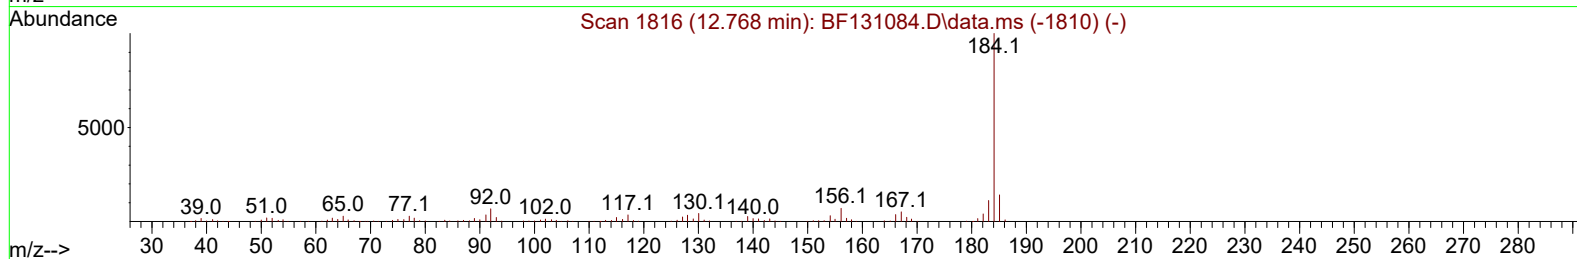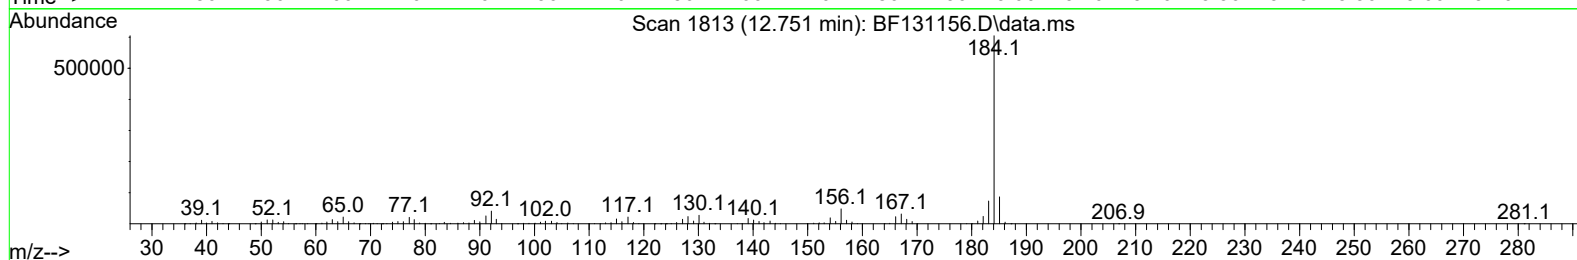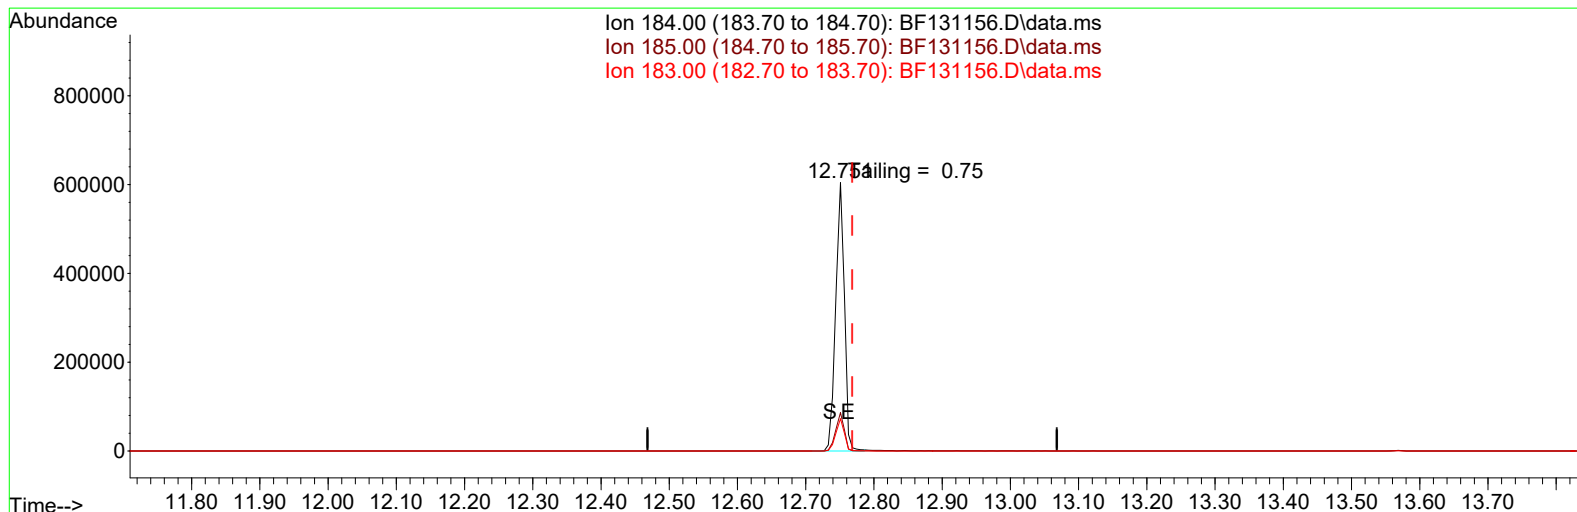

TIC: BF131156.D\data.ms

(77) Benzidine

12.751min (-0.018) 21153.13 ng

response 542303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.32
183.00	11.20	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2022	BNA_F	<u>BF131156.D</u>
Compound Name	Response	Retention Time
DDT	268586	13.568
DDD	4131	13.298
DDE	90	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4221	272807	1.55

Instrument :
BNA_F
ClientSampleId :
DFTPP