
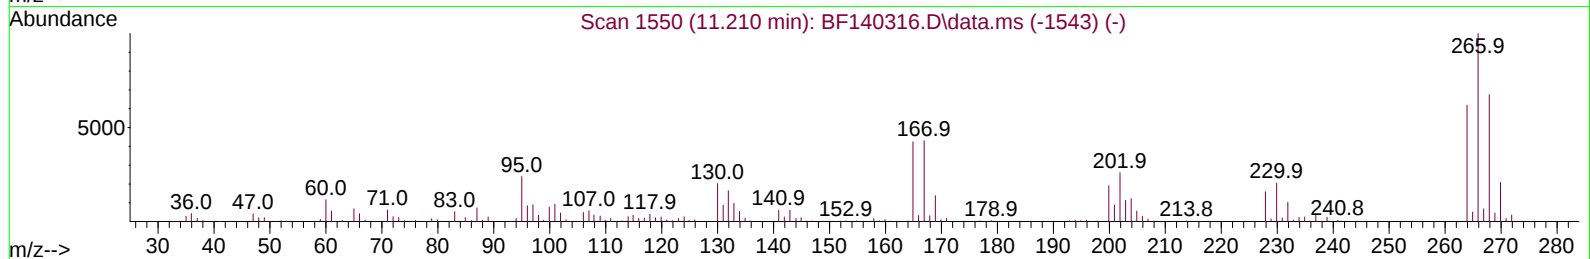
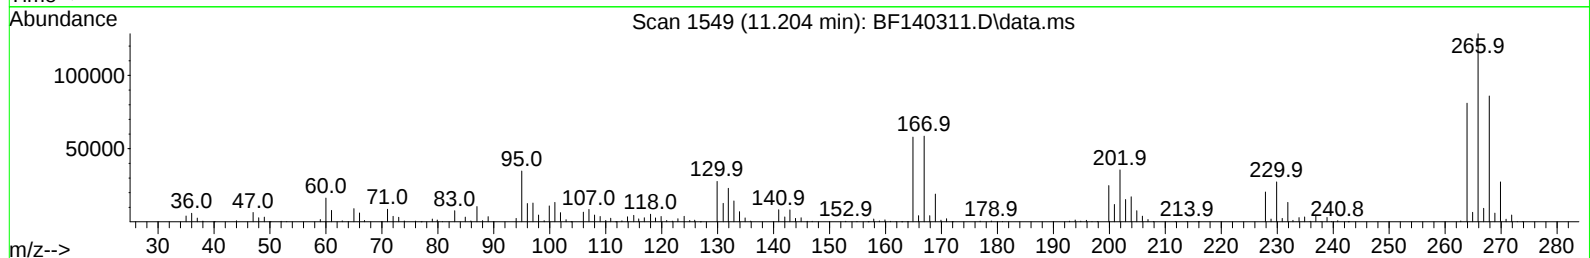


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
Data File : BF140311.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 00:12:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 00:05:37 2024
Response via : Initial Calibration

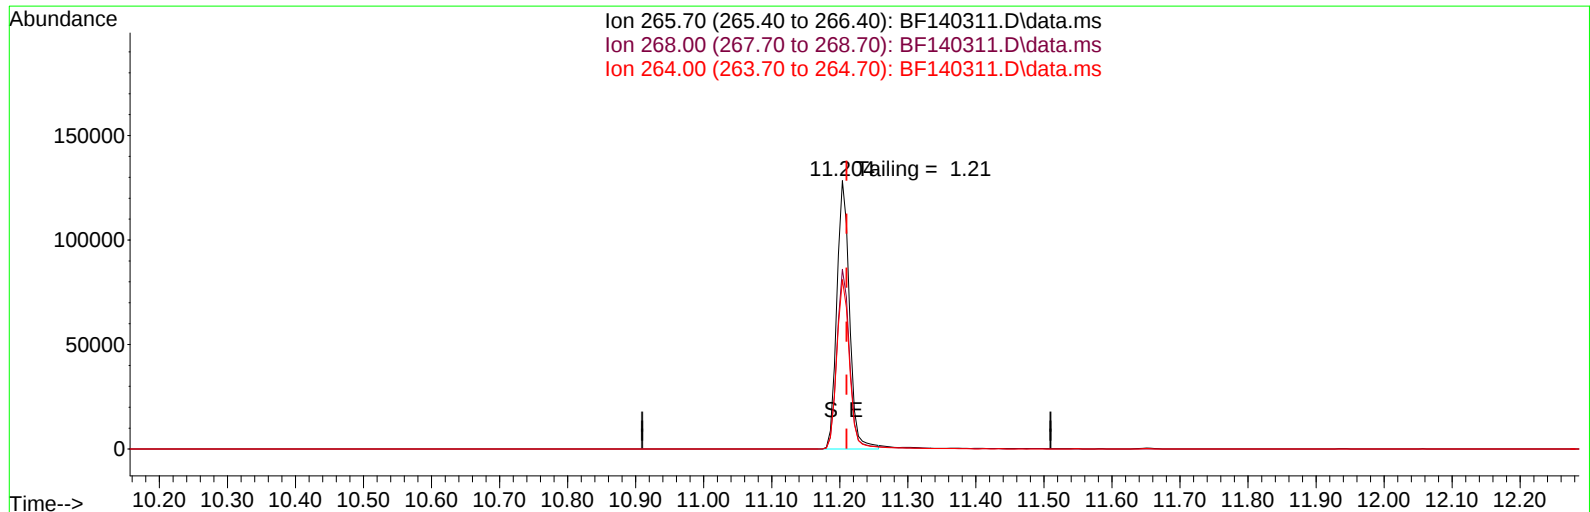




TIC: BF140311.D\data.ms

(70) Pentachlorophenol (C)**11.204min (-0.006) 28916.95 ng****response 168232**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	66.97
264.00	61.80	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
Data File : BF140311.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 00:12:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 00:05:37 2024
Response via : Initial Calibration

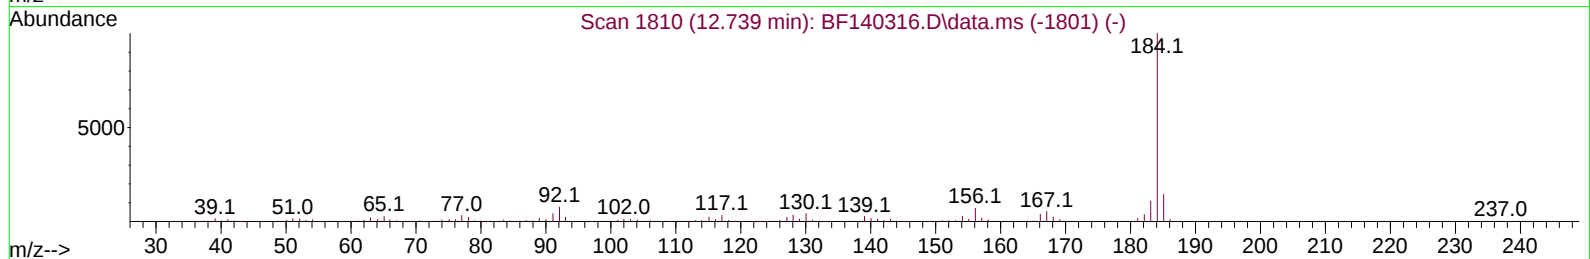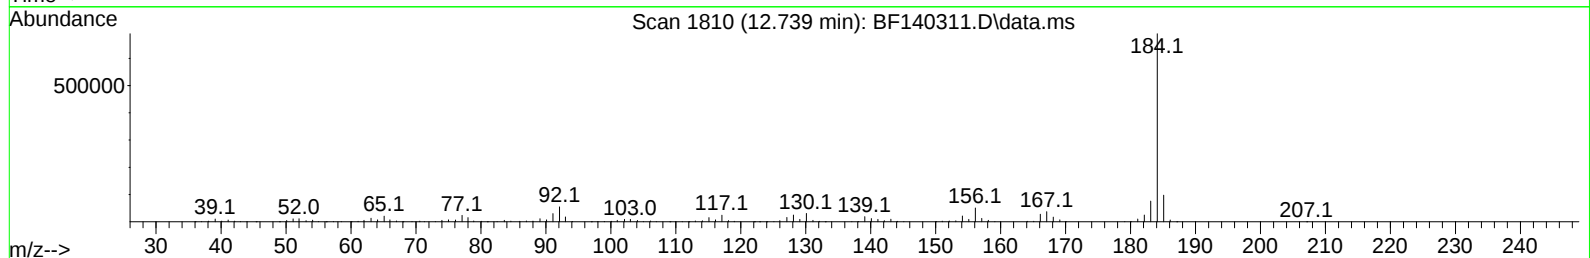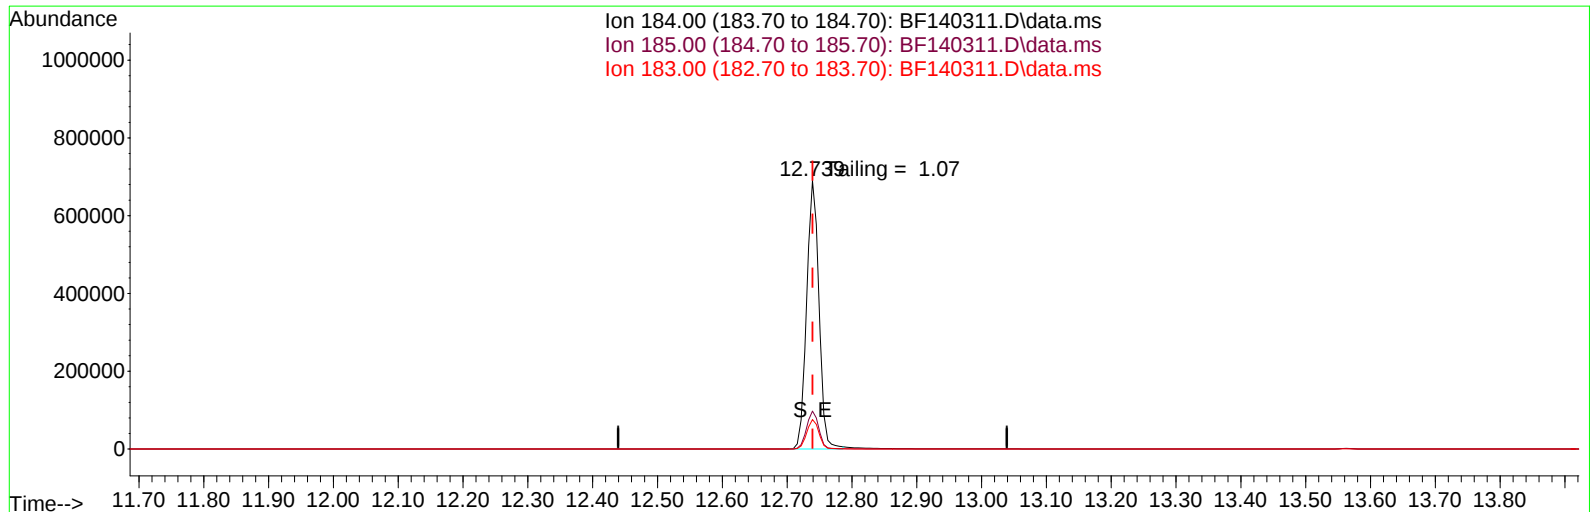

TIC: BF140311.D\data.ms

(77) Benzidine

12.739min (-0.000) 0.00 ng

response 917456

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.12
183.00	10.80	10.97
0.00	0.00	0.00