

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
Data File : BF140321.D
Acq On : 11 Nov 2024 17:01
Operator : RC/JU
Sample : PB164848BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164848BL

Quant Time: Nov 12 00:44:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 00:05:37 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	135530	20.000	ng	0.00
21) Naphthalene-d8	8.151	136	518809	20.000	ng	-0.01
39) Acenaphthene-d10	9.910	164	292211	20.000	ng	0.00
64) Phenanthrene-d10	11.398	188	564605	20.000	ng	0.00
76) Chrysene-d12	14.051	240	373526	20.000	ng	0.00
86) Perylene-d12	15.562	264	289009	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	1184686	151.018	ng	0.02
7) Phenol-d6	6.504	99	1558796	149.541	ng	0.00
23) Nitrobenzene-d5	7.434	82	1027292	102.794	ng	-0.01
42) 2,4,6-Tribromophenol	10.704	330	433212	152.600	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1848133	99.853	ng	0.00
79) Terphenyl-d14	12.992	244	2128598	97.717	ng	0.00


Target Compounds	Qvalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
Data File : BF140321.D
Acq On : 11 Nov 2024 17:01
Operator : RC/JU
Sample : PB164848BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164848BL


Quant Time: Nov 12 00:44:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 00:05:37 2024
Response via : Initial Calibration

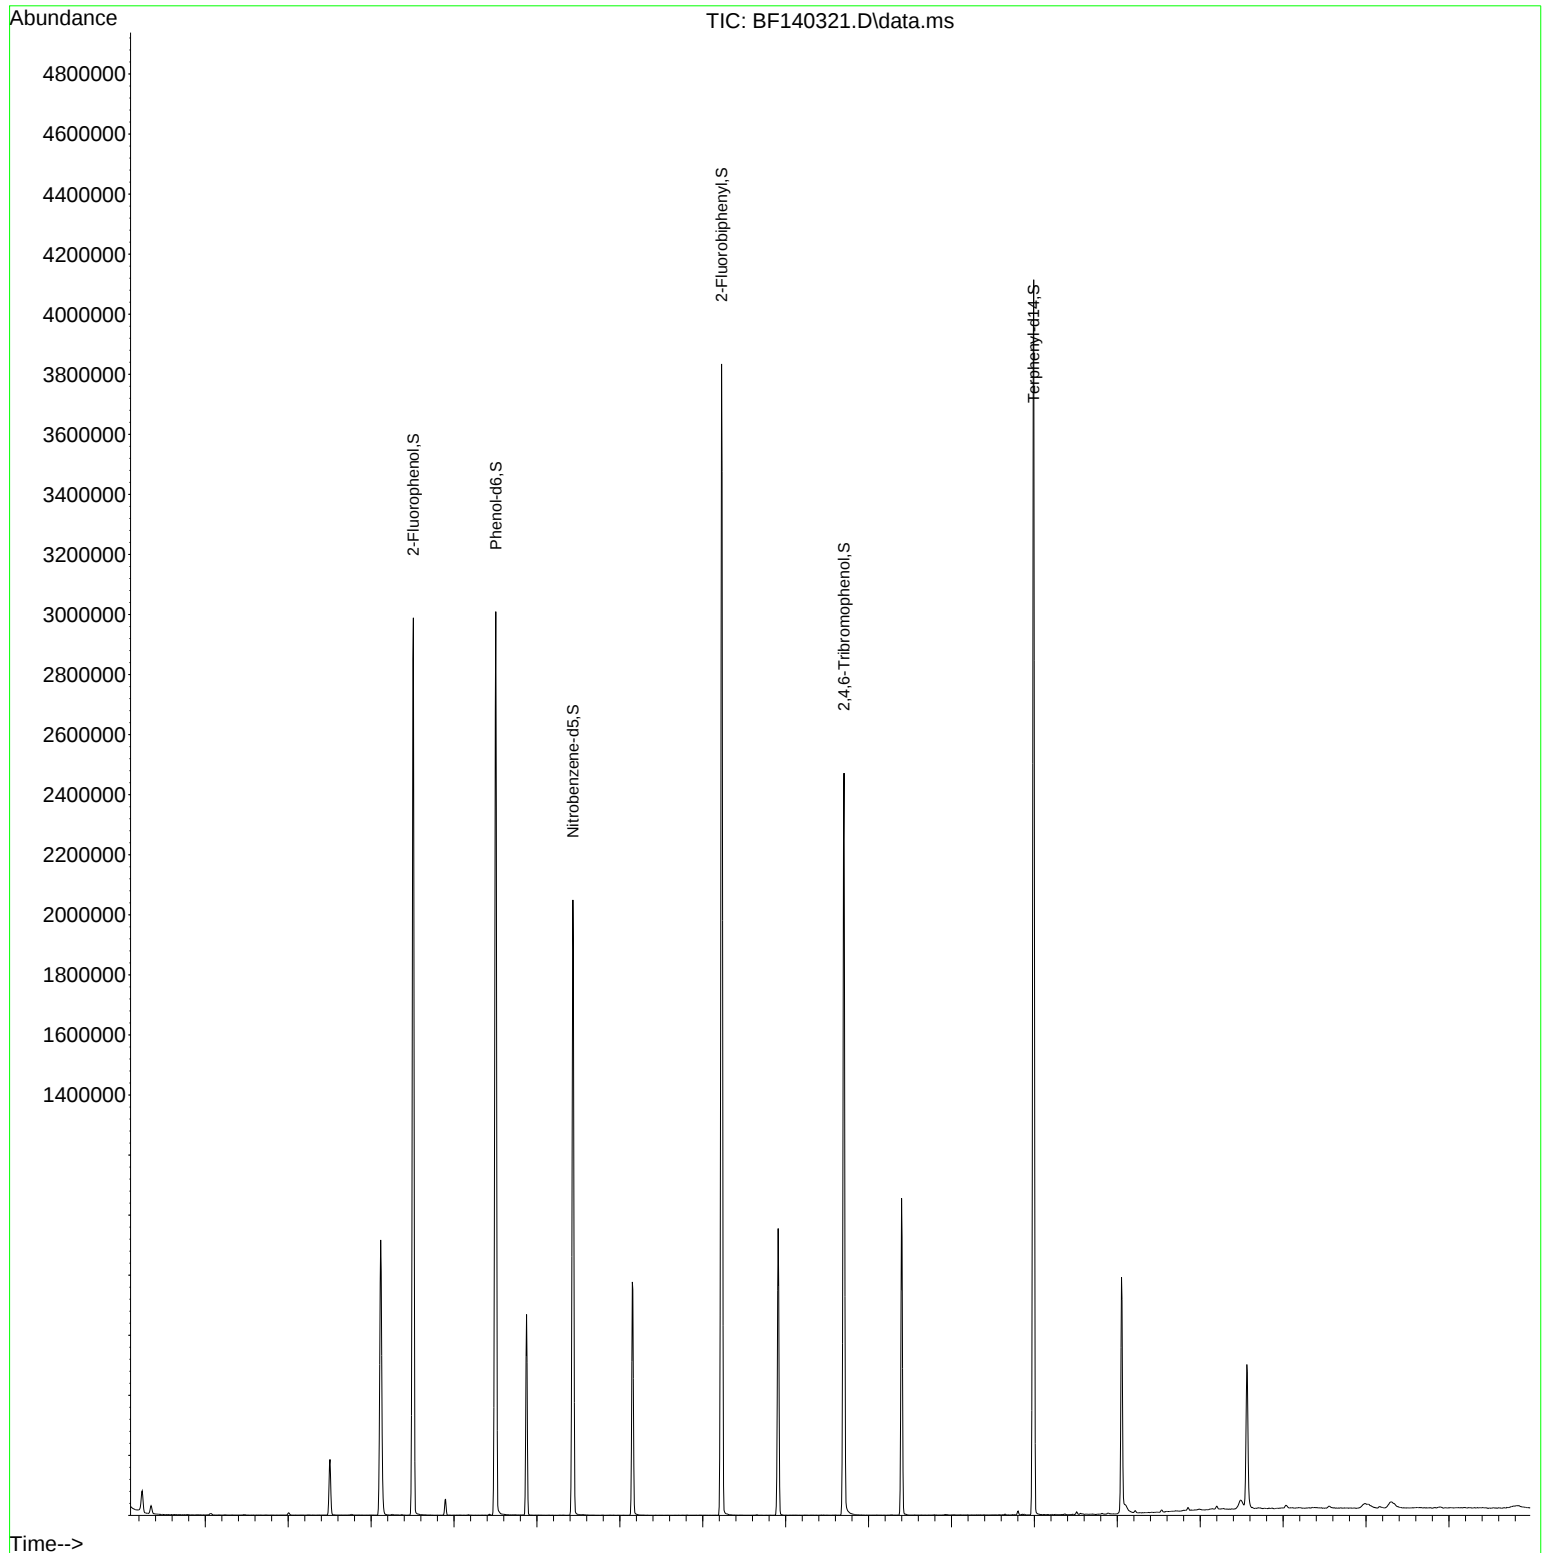



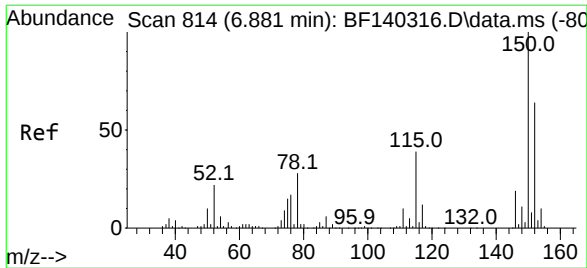


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF140321.D
Acq: 11 Nov 2024 17:01

Instrument :
BNA_F
ClientSampleId :
PB164848BL



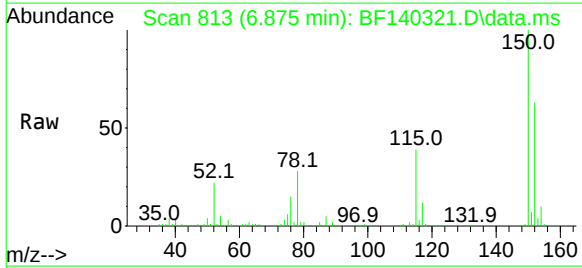



Tgt Ion:152 Resp: 135530
Ion Ratio Lower Upper
152 100
150 157.9 127.1 190.7
115 61.4 49.4 74.0

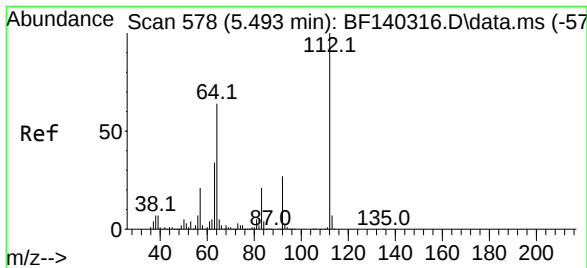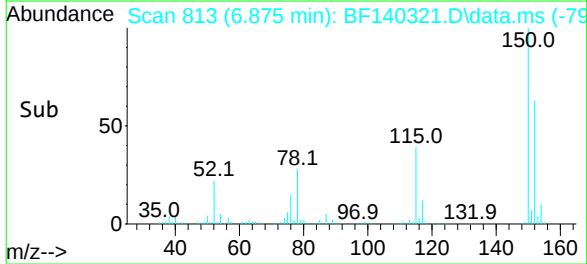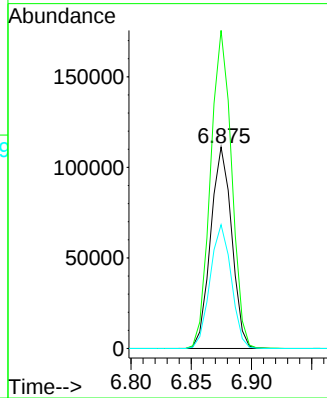

#5
2-Fluorophenol
Concen: 151.018 ng
RT: 5.510 min Scan# 581
Delta R.T. 0.018 min
Lab File: BF140321.D
Acq: 11 Nov 2024 17:01

Tgt Ion:112 Resp: 1184686
Ion Ratio Lower Upper
112 100
64 62.0 51.0 76.6
63 32.9 26.9 40.3


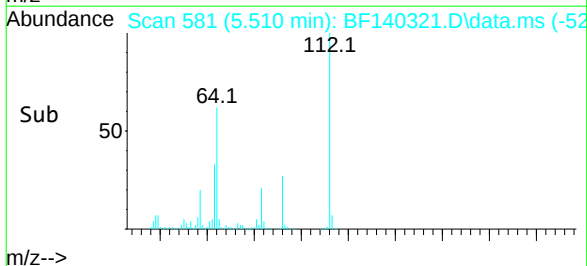
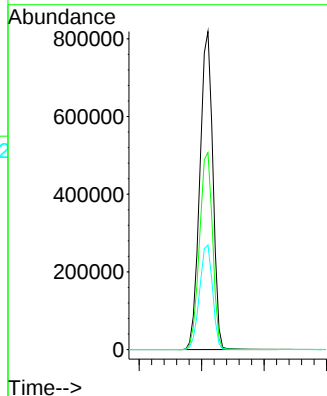
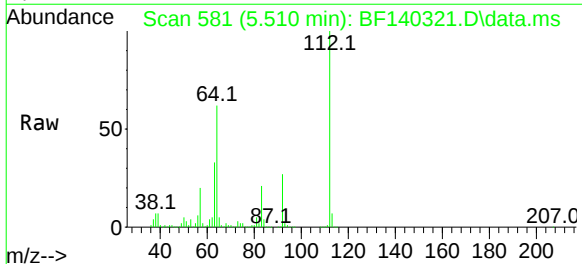


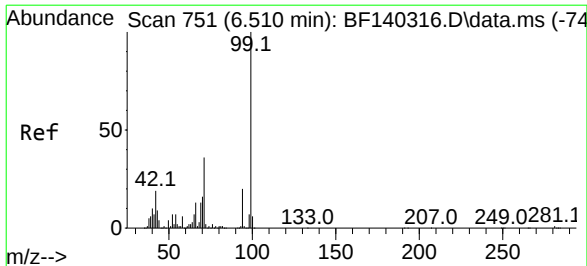

#7
Phenol-d6
Concen: 149.541 ng
RT: 6.504 min Scan# 751
Delta R.T. -0.006 min
Lab File: BF140321.D
Acq: 11 Nov 2024 17:01




Instrument :
BNA_F
ClientSampleId :
PB164848BL


Tgt Ion: 99 Resp: 1558796
Ion Ratio Lower Upper
99 100
42 19.8 15.5 23.3
71 36.5 28.8 43.2

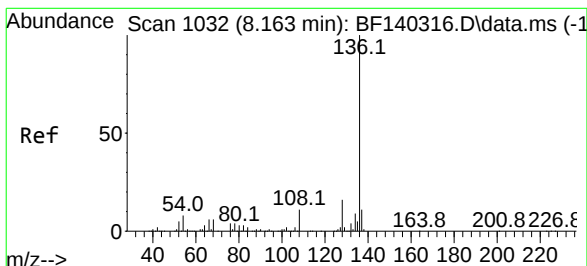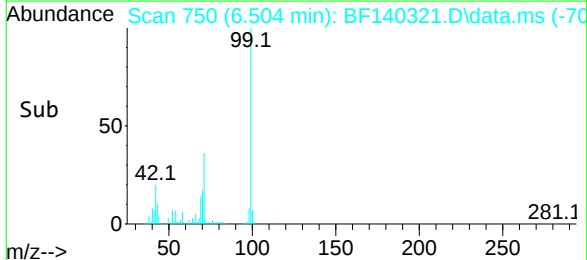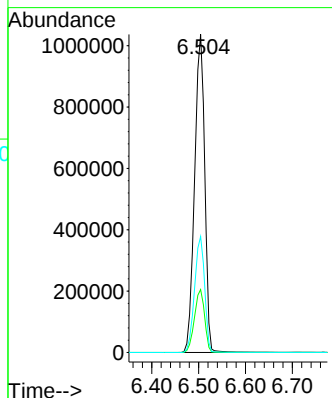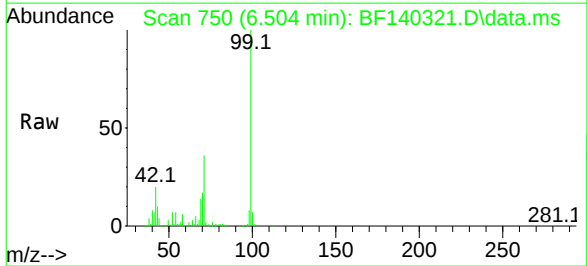

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 1030
Delta R.T. -0.012 min
Lab File: BF140321.D
Acq: 11 Nov 2024 17:01


Tgt Ion: 136 Resp: 518809
Ion Ratio Lower Upper
136 100
137 11.0 8.6 12.8
54 8.2 6.2 9.2
68 6.4 4.8 7.2

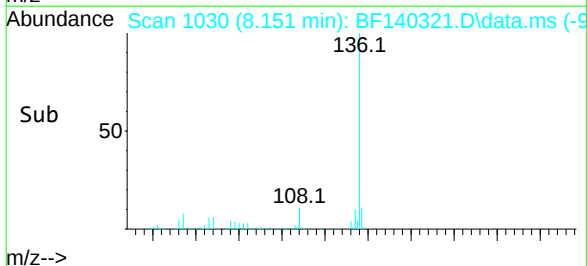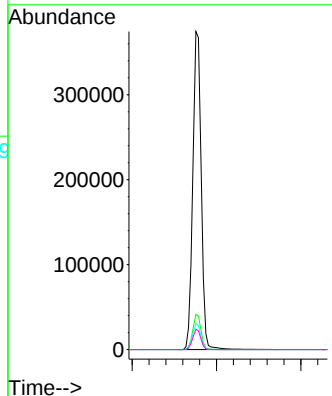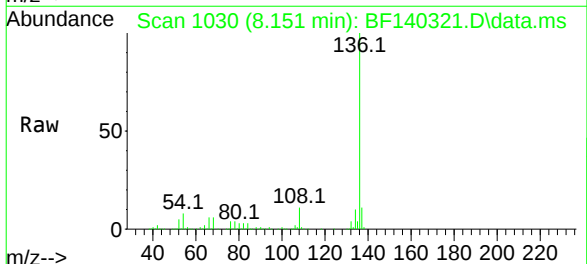



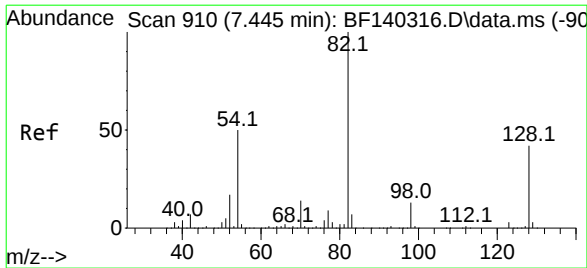


#23
Nitrobenzene-d5
Concen: 102.794 ng
RT: 7.434 min Scan# 90
Delta R.T. -0.012 min
Lab File: BF140321.D
Acq: 11 Nov 2024 17:01


Instrument :
BNA_F
ClientSampleId :
PB164848BL

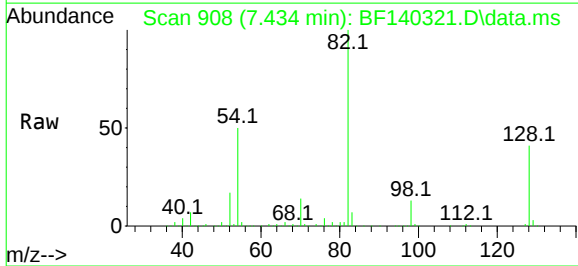



Tgt Ion: 82 Resp: 1027292
Ion Ratio Lower Upper
82 100
128 41.3 33.8 50.6
54 50.2 40.0 60.0

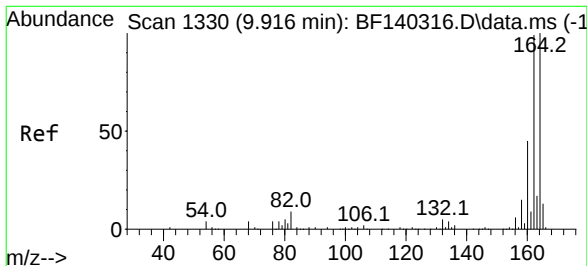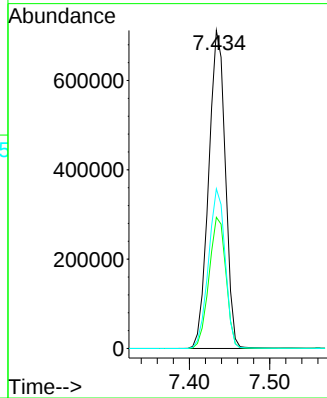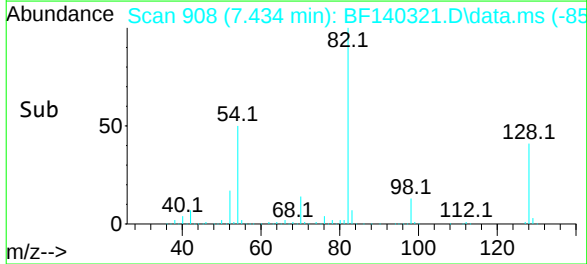


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF140321.D
Acq: 11 Nov 2024 17:01

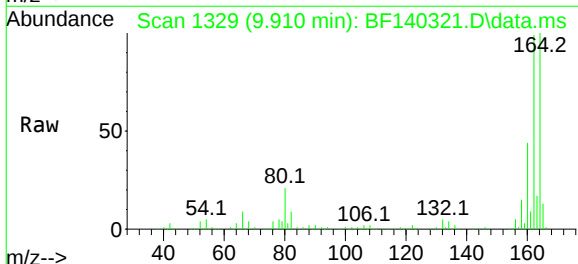


Tgt Ion: 164 Resp: 292211
Ion Ratio Lower Upper
164 100
162 99.3 79.4 119.0
160 44.0 35.6 53.4

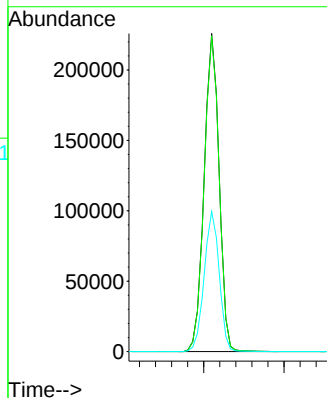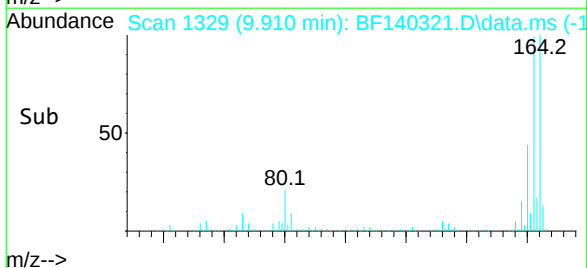



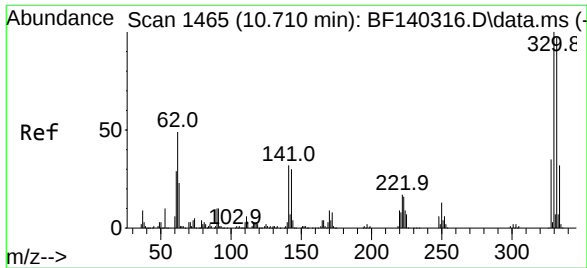


#42
2,4,6-Tribromophenol
Concen: 152.600 ng
RT: 10.704 min Scan# 1464
Delta R.T. -0.006 min
Lab File: BF140321.D
Acq: 11 Nov 2024 17:01


Instrument :
BNA_F
ClientSampleId :
PB164848BL

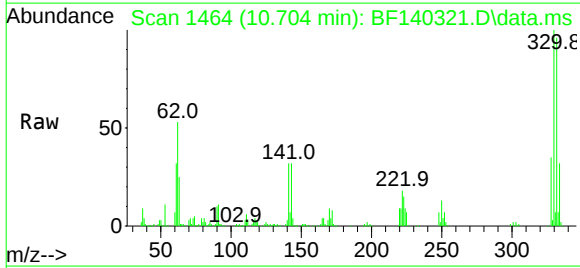



Tgt Ion: 330 Resp: 433212
Ion Ratio Lower Upper
330 100
332 96.7 77.1 115.7
141 34.0 28.3 42.5

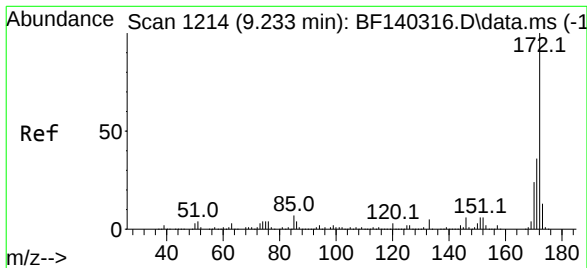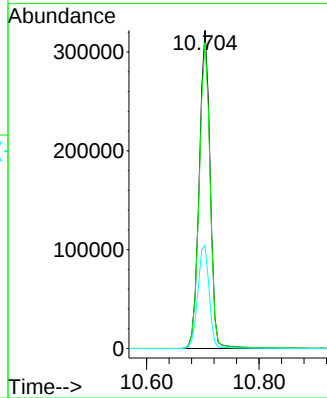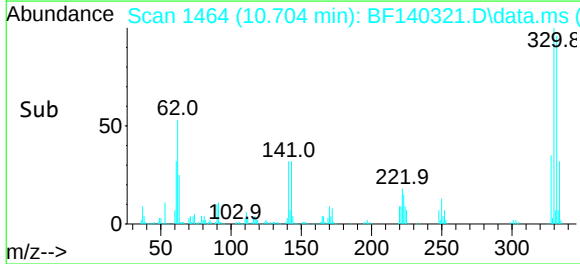


#45
2-Fluorobiphenyl
Concen: 99.853 ng
RT: 9.228 min Scan# 1213
Delta R.T. -0.006 min
Lab File: BF140321.D
Acq: 11 Nov 2024 17:01

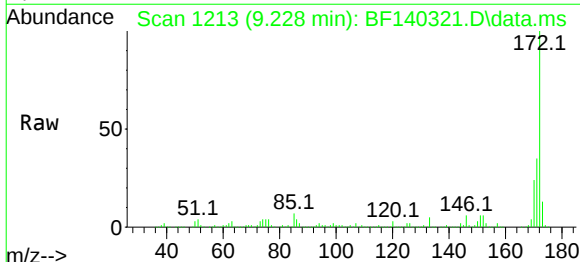

Tgt Ion: 172 Resp: 1848133
Ion Ratio Lower Upper
172 100
171 35.5 28.7 43.1
170 23.6 19.3 28.9

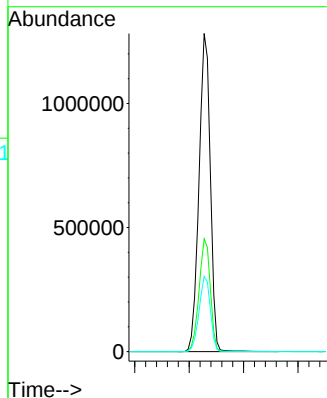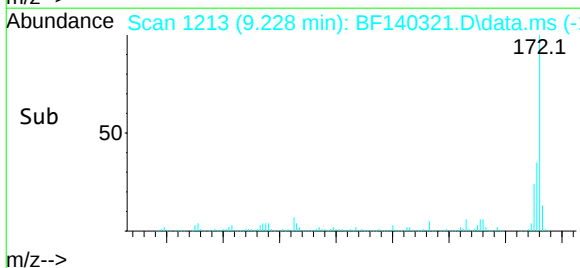

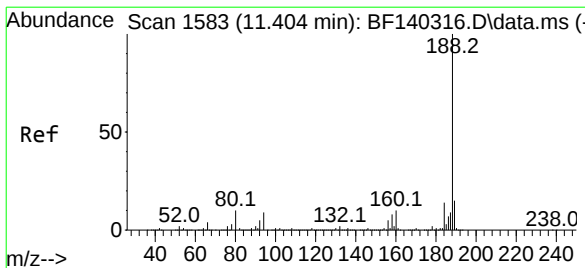

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.398 min Scan# 15

Delta R.T. -0.006 min

Lab File: BF140321.D

Acq: 11 Nov 2024 17:01

Instrument :

BNA_F

ClientSampleId :

PB164848BL





Tgt Ion:188 Resp: 564605

Ion Ratio Lower Upper

188 100

94 9.7 7.4 11.2

80 10.3 8.0 12.0

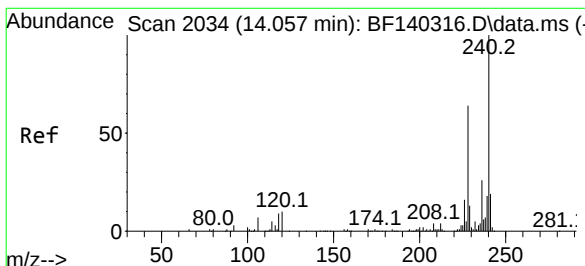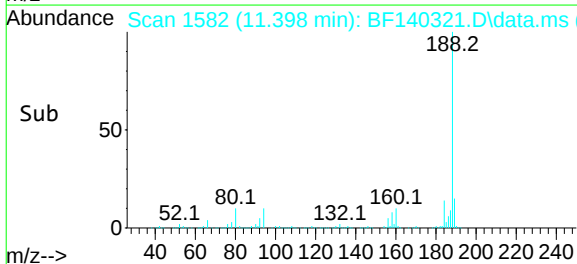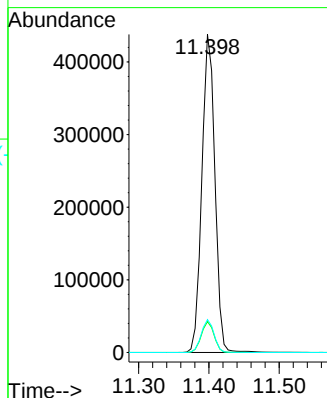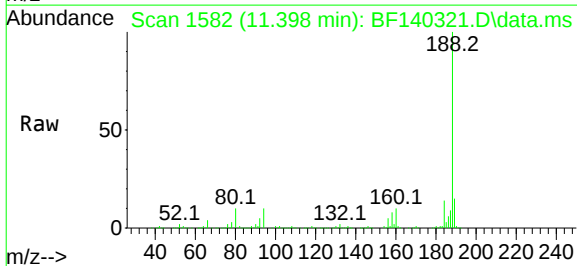

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.051 min Scan# 2033

Delta R.T. -0.006 min

Lab File: BF140321.D

Acq: 11 Nov 2024 17:01




Tgt Ion:240 Resp: 373526


Ion Ratio Lower Upper

240 100

120 10.8 8.2 12.4

236 25.7 20.9 31.3

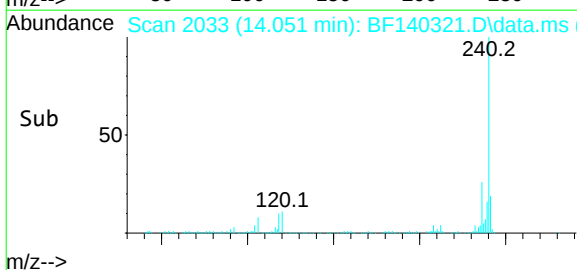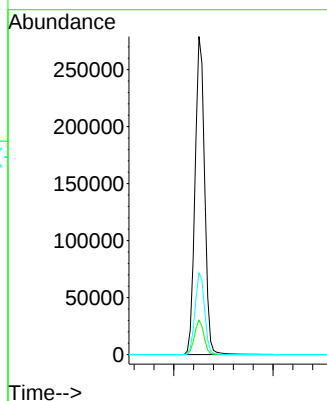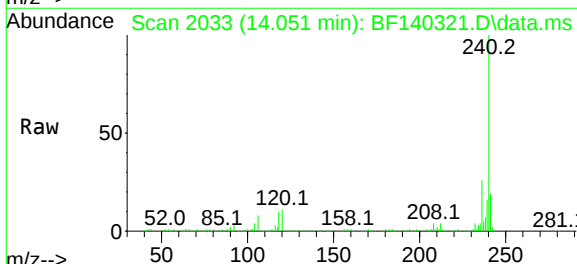

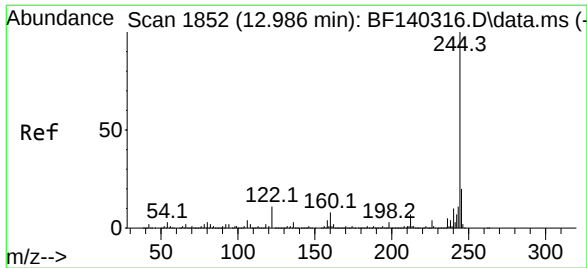

#79

Terphenyl-d14

Concen: 97.717 ng

RT: 12.992 min Scan# 18

Delta R.T. 0.006 min

Lab File: BF140321.D

Acq: 11 Nov 2024 17:01

Instrument :

BNA_F

ClientSampleId :

PB164848BL





Tgt Ion:244 Resp: 2128598

Ion Ratio Lower Upper

244 100

212 7.4 6.0 9.0

122 10.8 9.0 13.4

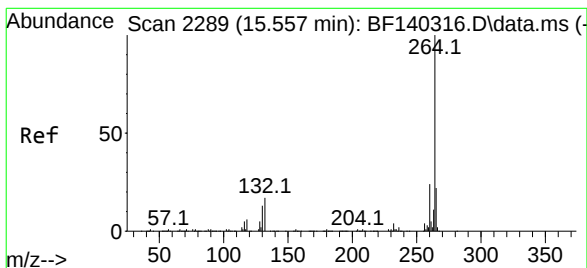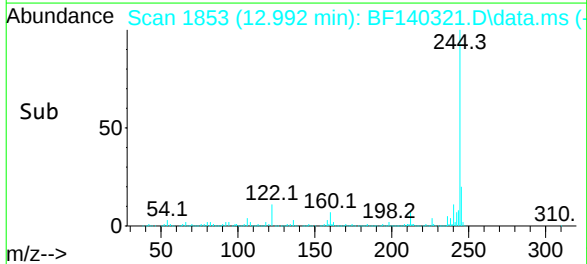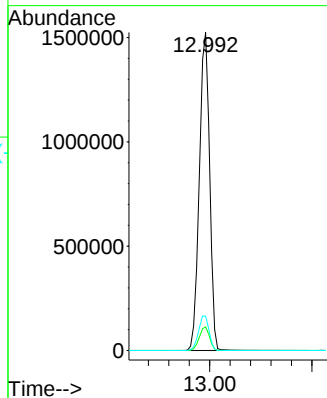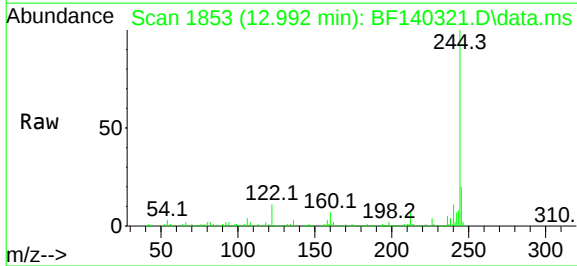

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.562 min Scan# 2290

Delta R.T. 0.006 min

Lab File: BF140321.D

Acq: 11 Nov 2024 17:01

Tgt Ion:264 Resp: 289009

Ion Ratio Lower Upper

264 100

260 23.6 19.6 29.4

265 21.1 17.6 26.4

