

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
 Data File : BF140326.D
 Acq On : 11 Nov 2024 19:18
 Operator : RC/JU
 Sample : P4788-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BP-G3

Quant Time: Nov 12 00:45:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 12 00:05:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	128368	20.000	ng	0.00
21) Naphthalene-d8	8.151	136	492184	20.000	ng	-0.01
39) Acenaphthene-d10	9.910	164	273941	20.000	ng	0.00
64) Phenanthrene-d10	11.398	188	522344	20.000	ng	0.00
76) Chrysene-d12	14.045	240	321317	20.000	ng	-0.01
86) Perylene-d12	15.539	264	262304	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	1075041	144.687	ng	0.02
7) Phenol-d6	6.504	99	1358608	137.608	ng	0.00
23) Nitrobenzene-d5	7.434	82	937213	98.853	ng	-0.01
42) 2,4,6-Tribromophenol	10.704	330	421715	158.457	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1695330	97.706	ng	0.00
79) Terphenyl-d14	12.992	244	1986006	105.984	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
Data File : BF140326.D
Acq On : 11 Nov 2024 19:18
Operator : RC/JU
Sample : P4788-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BP-G3

Quant Time: Nov 12 00:45:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 00:05:37 2024
Response via : Initial Calibration




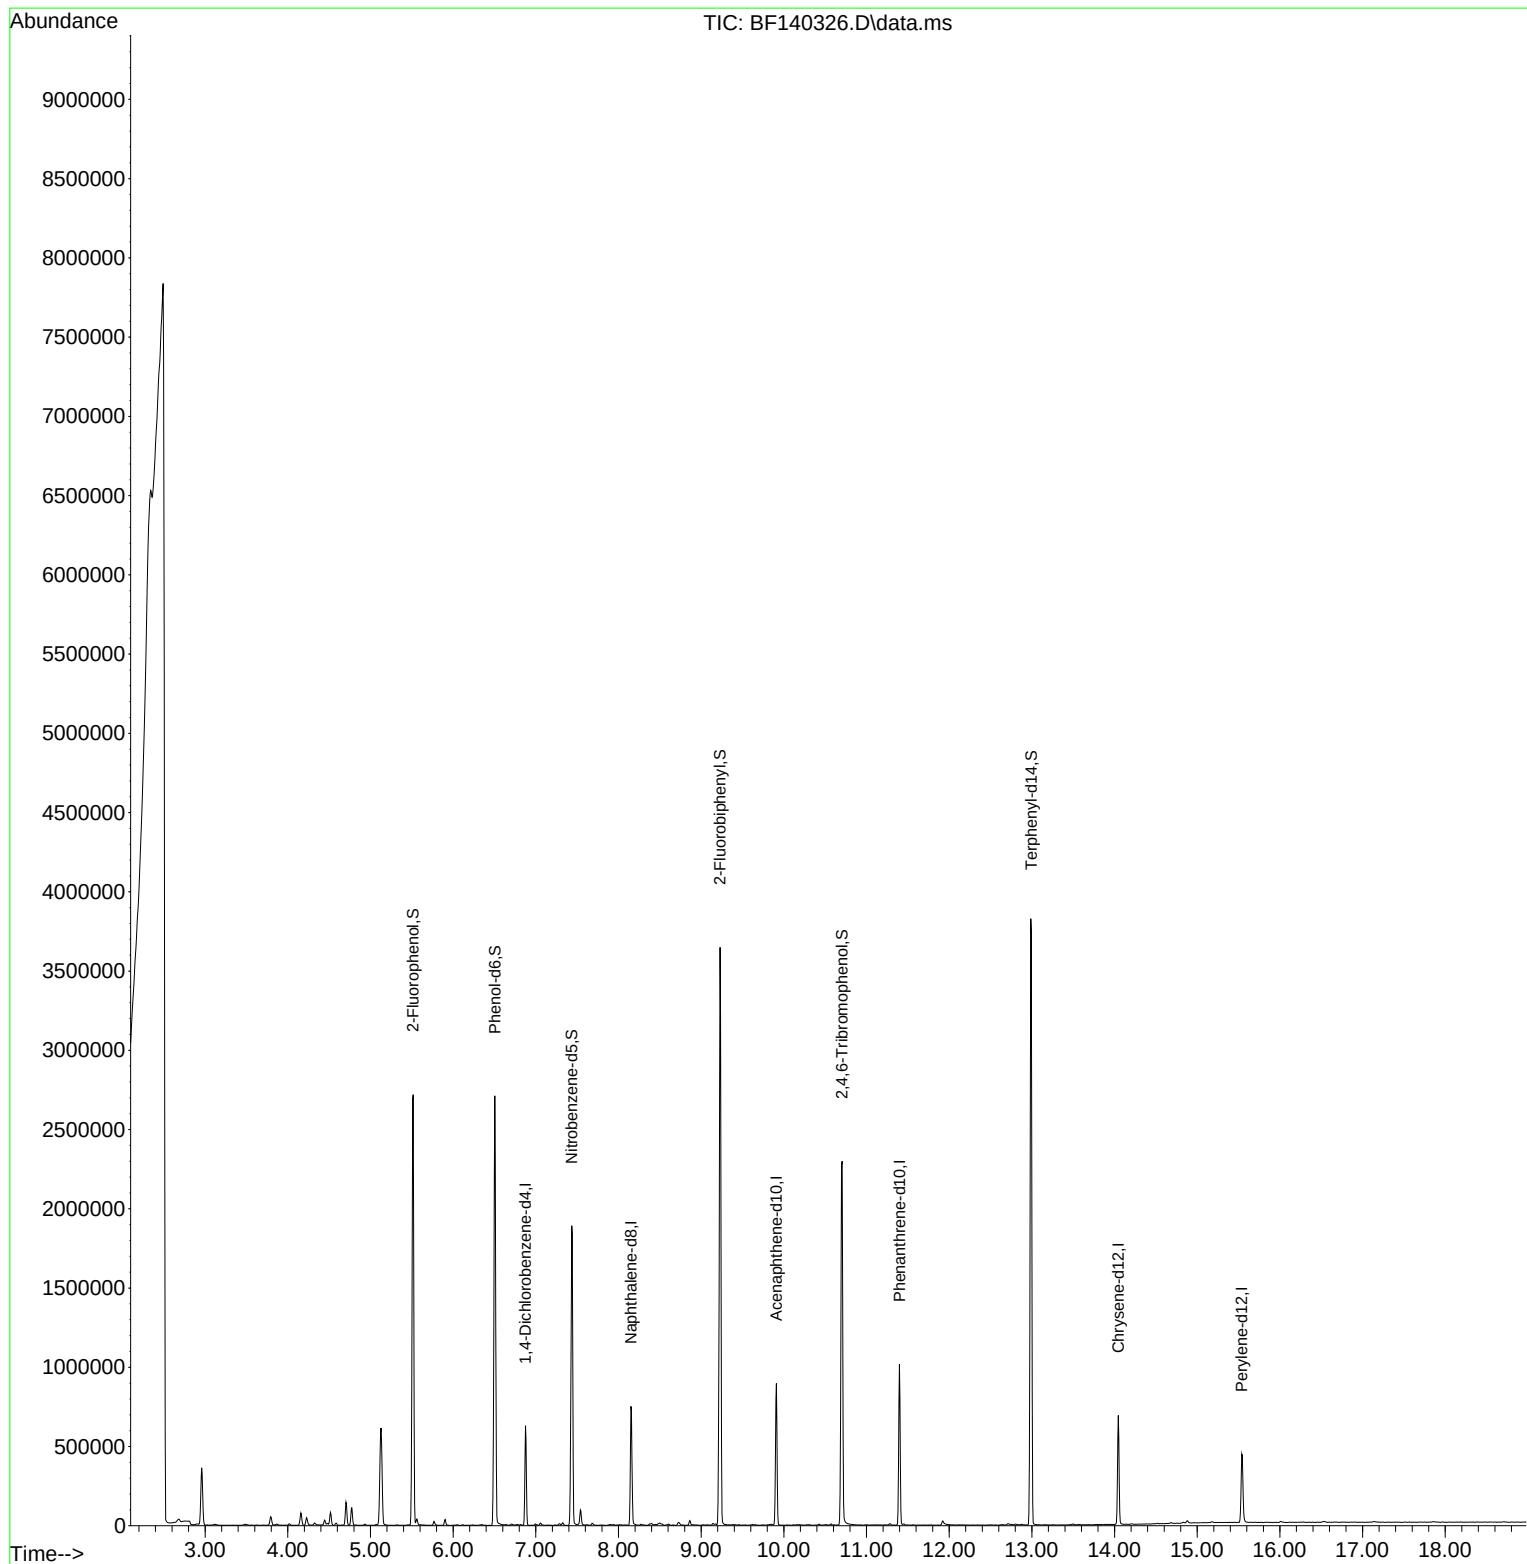


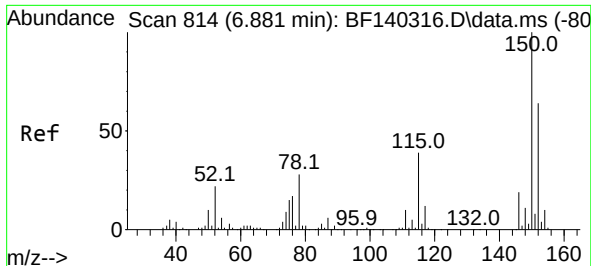

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 814
Delta R.T. -0.006 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18




Instrument :
BNA_F
ClientSampleId :
BP-G3


Tgt Ion:152 Resp: 128368
Ion Ratio Lower Upper
152 100
150 156.1 127.1 190.7
115 61.1 49.4 74.0

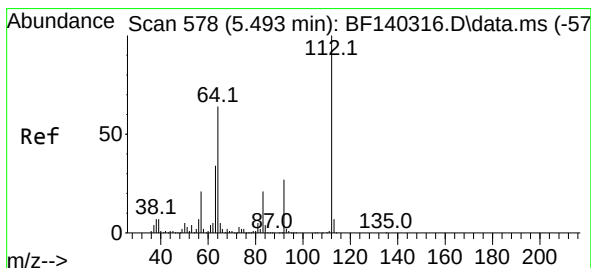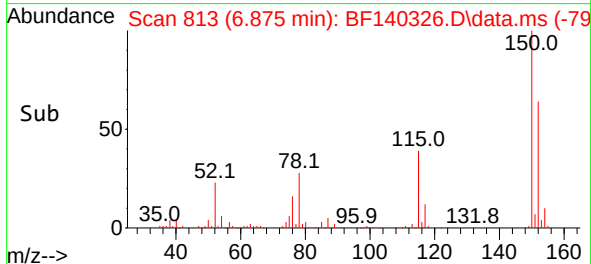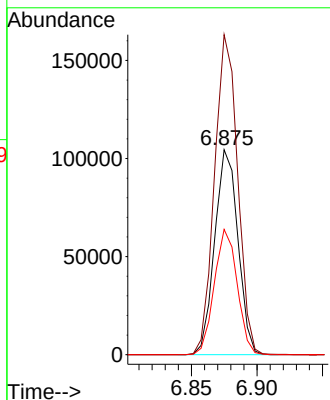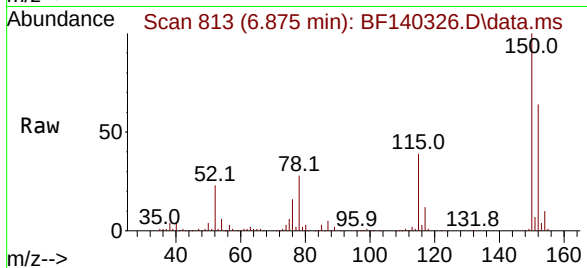

#5
2-Fluorophenol
Concen: 144.687 ng
RT: 5.516 min Scan# 582
Delta R.T. 0.024 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18

Tgt Ion:112 Resp: 1075041
Ion Ratio Lower Upper
112 100
64 61.0 51.0 76.6
63 32.3 26.9 40.3


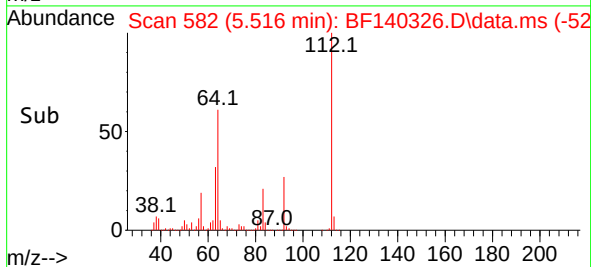
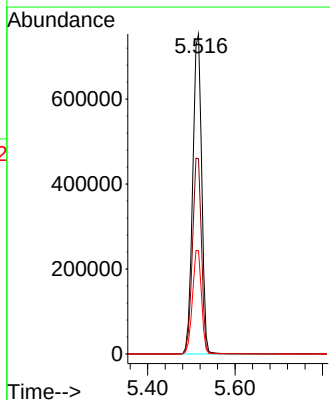
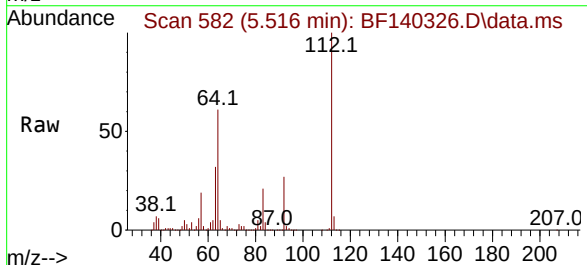


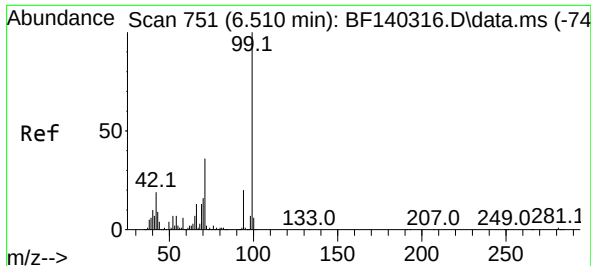

#7
Phenol-d6
Concen: 137.608 ng
RT: 6.504 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18




Instrument :
BNA_F
ClientSampleId :
BP-G3


Tgt Ion: 99 Resp: 1358608
Ion Ratio Lower Upper
99 100
42 19.4 15.5 23.3
71 35.7 28.8 43.2

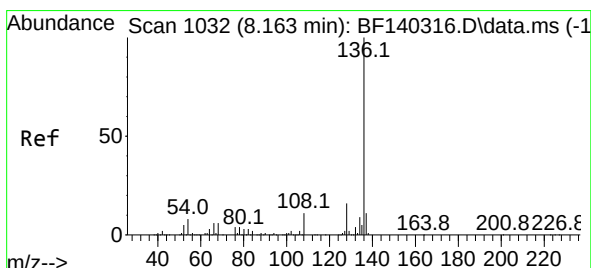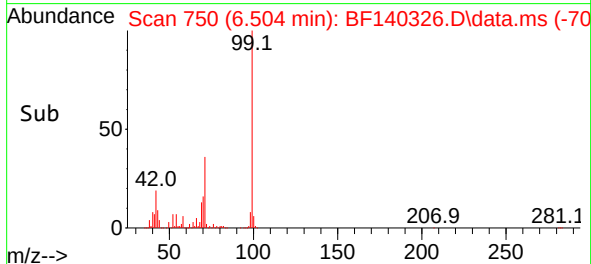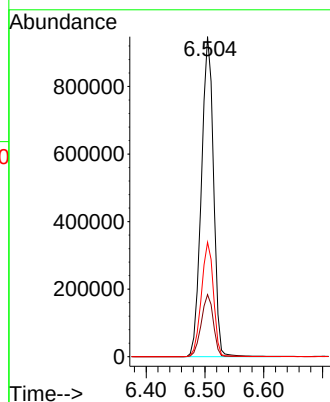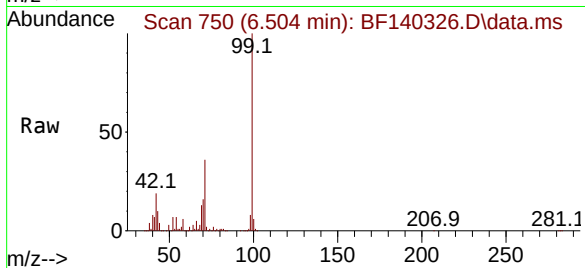

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 1030
Delta R.T. -0.012 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18

Tgt Ion: 136 Resp: 492184
Ion Ratio Lower Upper
136 100
137 10.9 8.6 12.8
54 8.2 6.2 9.2
68 6.2 4.8 7.2


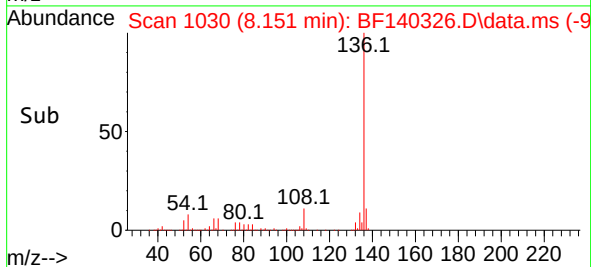
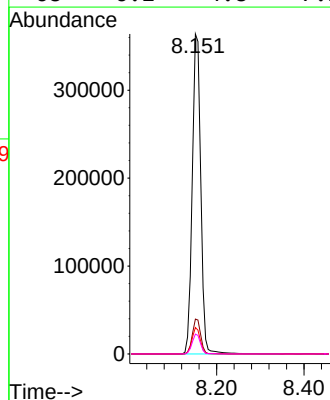
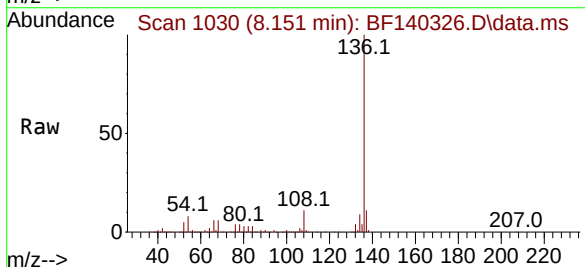


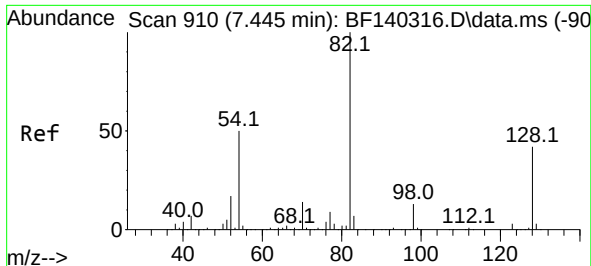

#23
Nitrobenzene-d5
Concen: 98.853 ng
RT: 7.434 min Scan# 90
Delta R.T. -0.012 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18




Instrument :
BNA_F
ClientSampleId :
BP-G3


Tgt Ion: 82 Resp: 937213
Ion Ratio Lower Upper
82 100
128 41.3 33.8 50.6
54 50.2 40.0 60.0

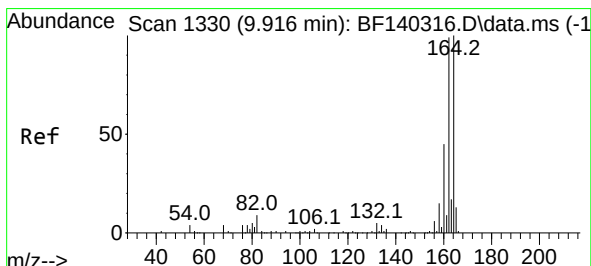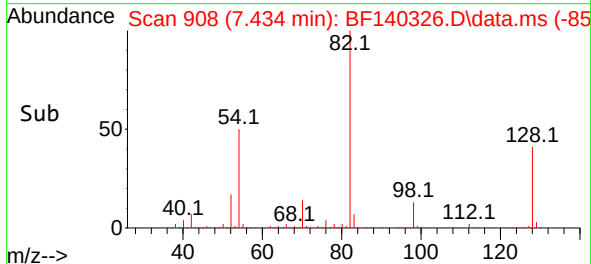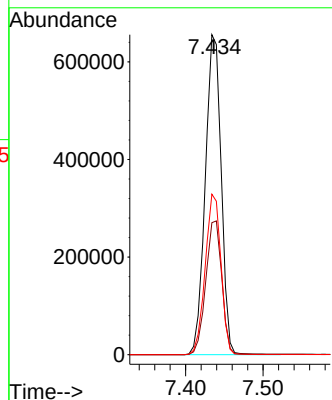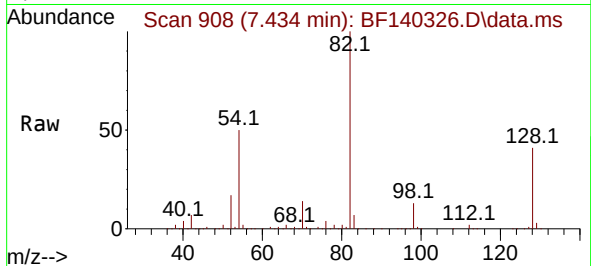

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18

Tgt Ion:164 Resp: 273941
Ion Ratio Lower Upper
164 100
162 98.9 79.4 119.0
160 44.1 35.6 53.4


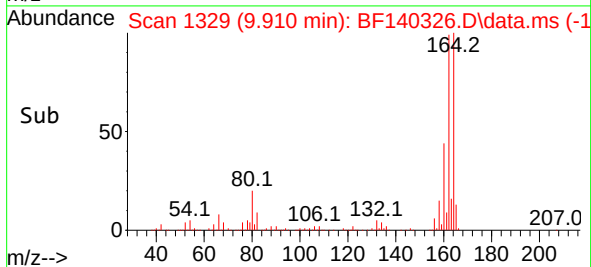
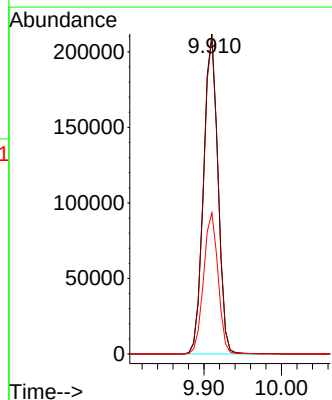
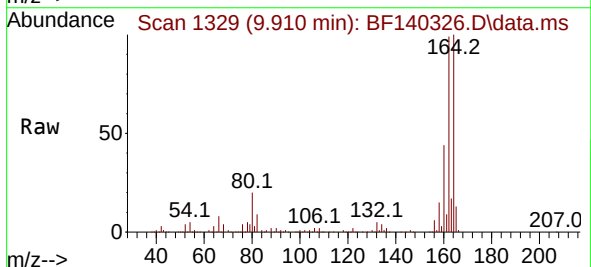


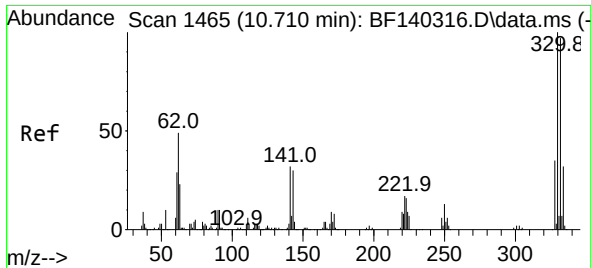

#42
2,4,6-Tribromophenol
Concen: 158.457 ng
RT: 10.704 min Scan# 1464
Delta R.T. -0.006 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18




Instrument :
BNA_F
ClientSampleId :
BP-G3


Tgt Ion:330 Resp: 421715
Ion Ratio Lower Upper
330 100
332 97.2 77.1 115.7
141 33.9 28.3 42.5

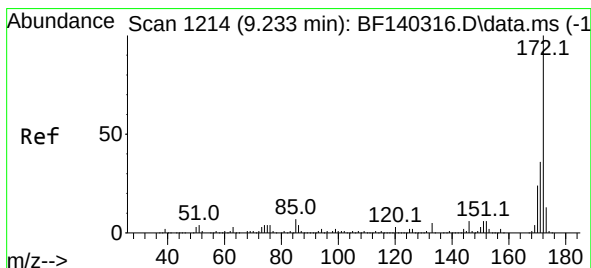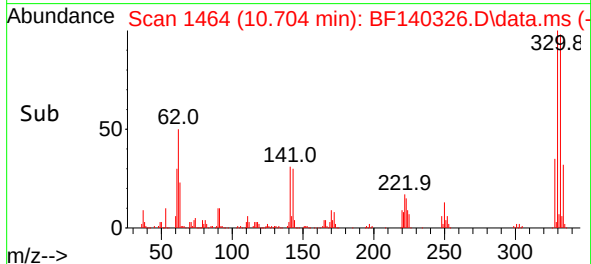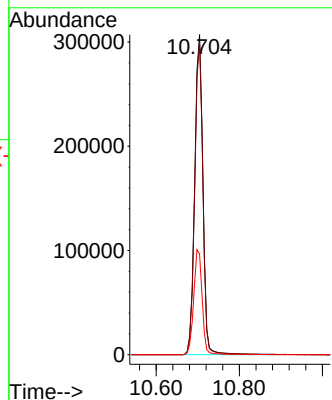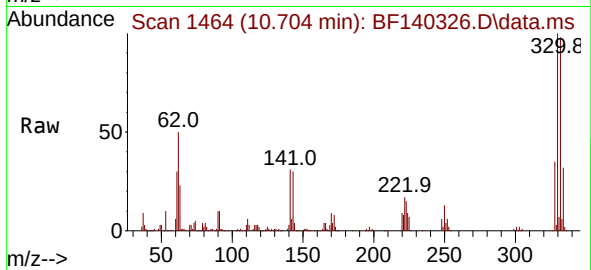

#45
2-Fluorobiphenyl
Concen: 97.706 ng
RT: 9.228 min Scan# 1213
Delta R.T. -0.006 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18

Tgt Ion:172 Resp: 1695330
Ion Ratio Lower Upper
172 100
171 35.5 28.7 43.1
170 24.0 19.3 28.9


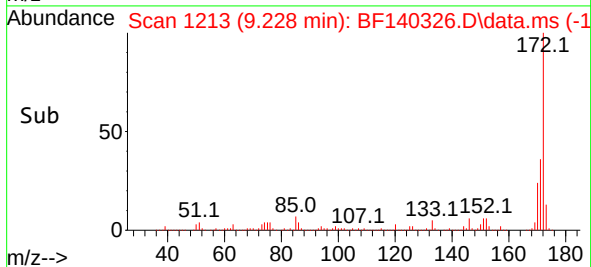
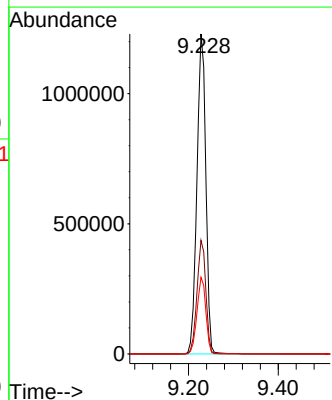
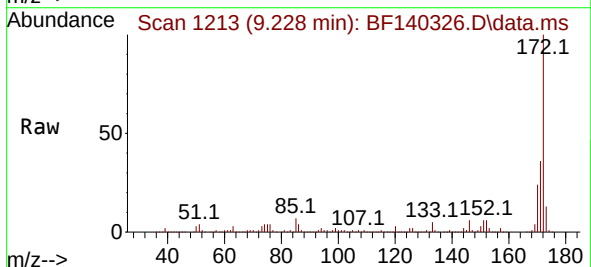


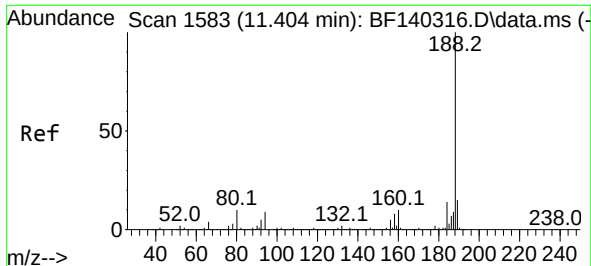

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18




Instrument :
BNA_F
ClientSampleId :
BP-G3


Tgt Ion:188 Resp: 522344
Ion Ratio Lower Upper
188 100
94 9.3 7.4 11.2
80 10.2 8.0 12.0

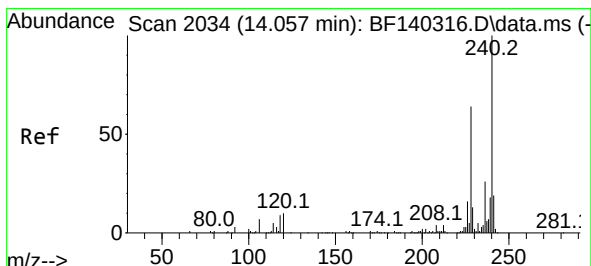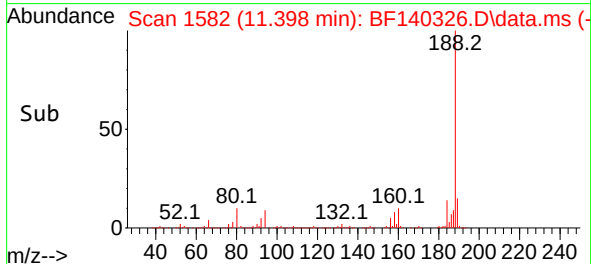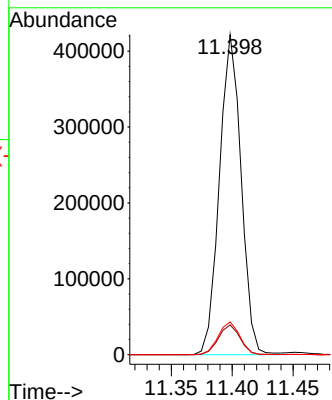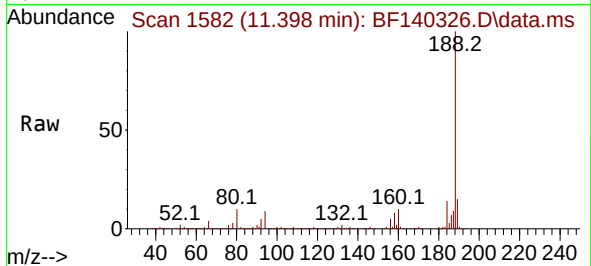

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 2032
Delta R.T. -0.012 min
Lab File: BF140326.D
Acq: 11 Nov 2024 19:18

Tgt Ion:240 Resp: 321317
Ion Ratio Lower Upper
240 100
120 10.5 8.2 12.4
236 26.3 20.9 31.3


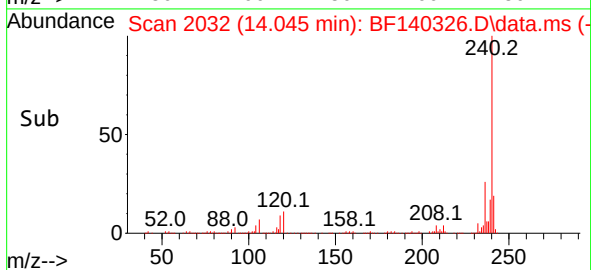
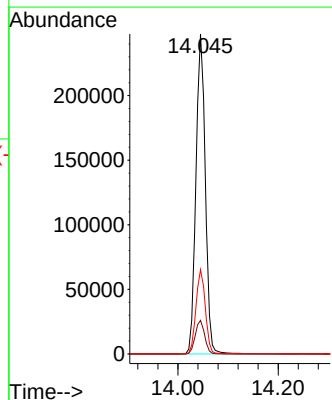
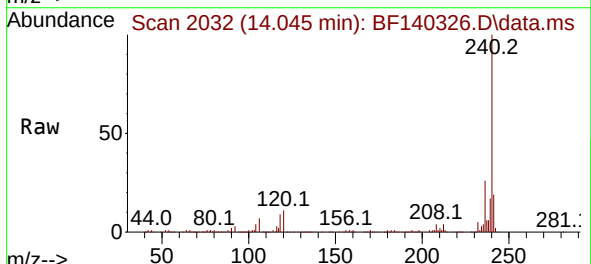


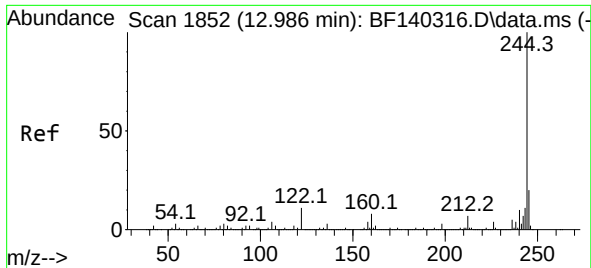

#79
 Terphenyl-d14
 Concen: 105.984 ng
 RT: 12.992 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: BF140326.D
 Acq: 11 Nov 2024 19:18

Instrument :
 BNA_F
 ClientSampleId :
 BP-G3

Tgt Ion:244 Resp: 1986006
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.0 9.0
 122 10.5 9.0 13.4

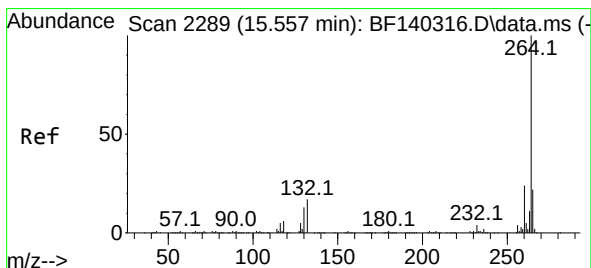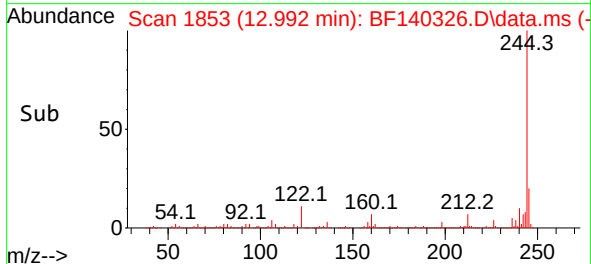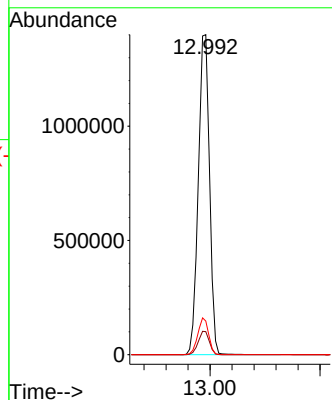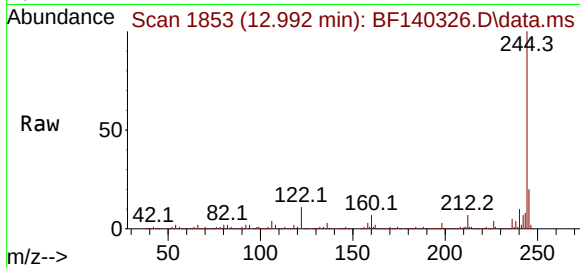

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.539 min Scan# 2286
 Delta R.T. -0.018 min
 Lab File: BF140326.D
 Acq: 11 Nov 2024 19:18

Tgt Ion:264 Resp: 262304
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.6 29.4
 265 21.3 17.6 26.4

