
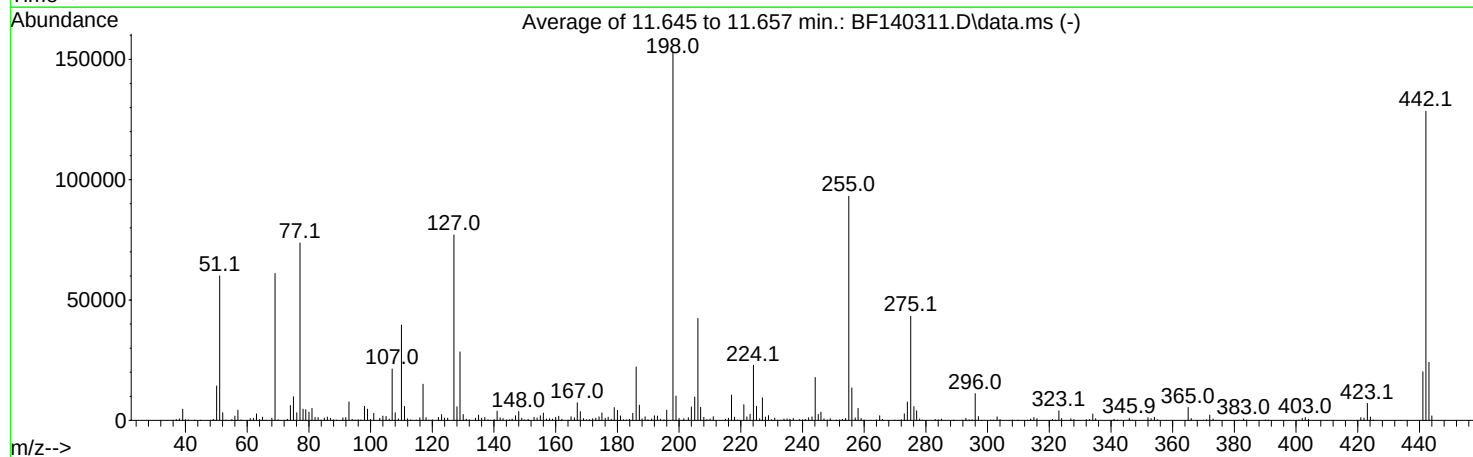


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
Data File : BF140311.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 12 00:05:37 2024

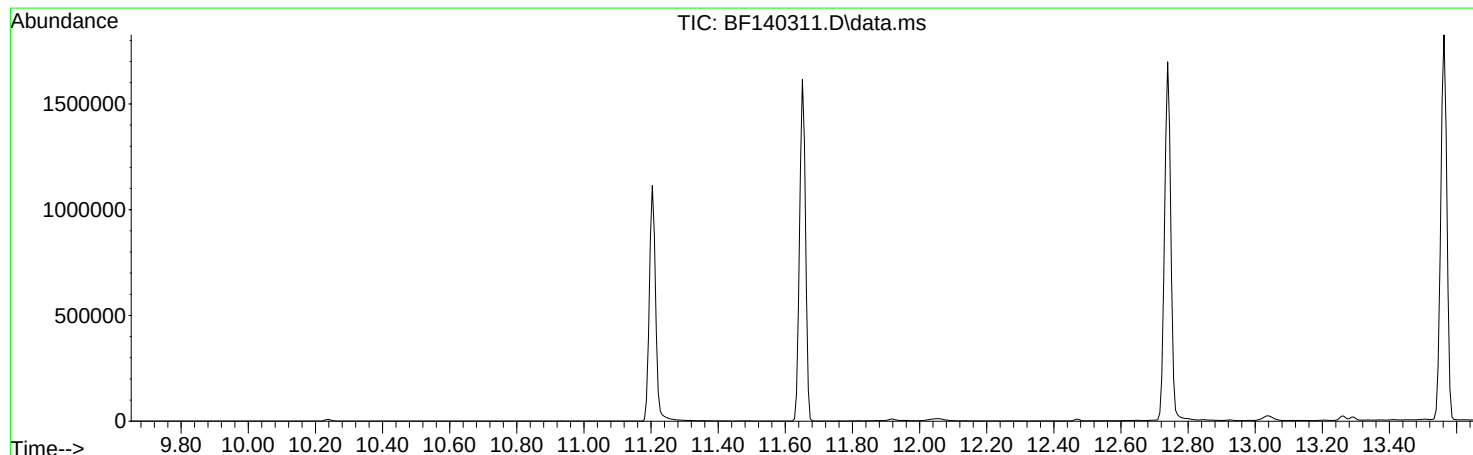




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	60024	PASS
68	69	0.00	2	1.5	931	PASS
69	198	0.00	100	39.9	61048	PASS
70	69	0.00	2	0.5	289	PASS
127	198	10	80	50.4	77032	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	152853	PASS
199	198	5	9	6.6	10135	PASS
275	198	10	60	28.3	43237	PASS
365	198	1	100	3.5	5362	PASS
441	198	0.01	100	13.2	20184	PASS
442	442	50	100	100.0	128477	PASS
443	442	15	24	18.8	24117	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
Data File : BF140311.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 12 00:12:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 00:05:37 2024
Response via : Initial Calibration

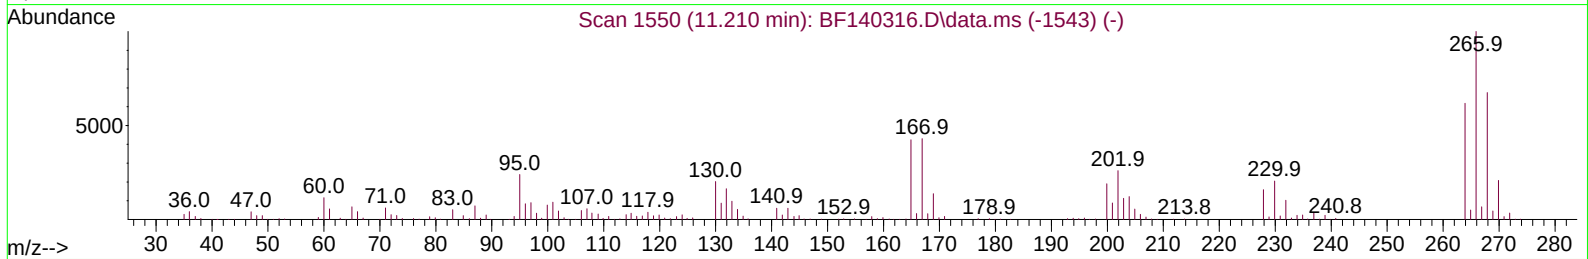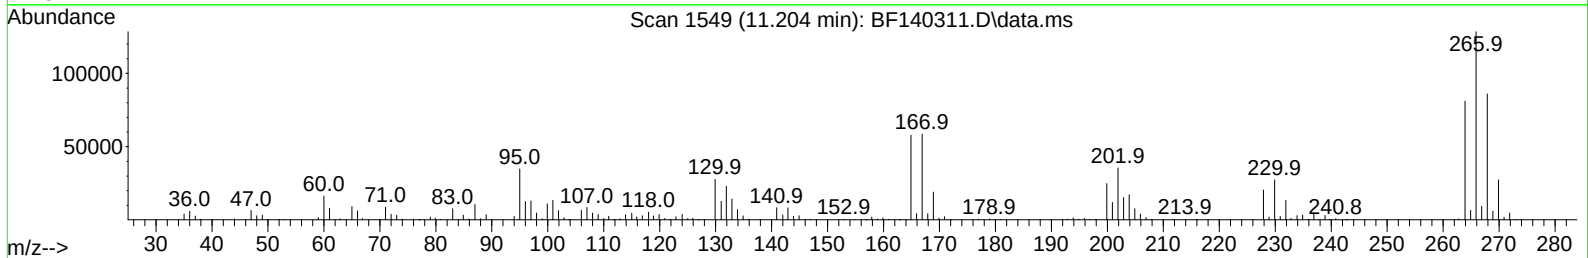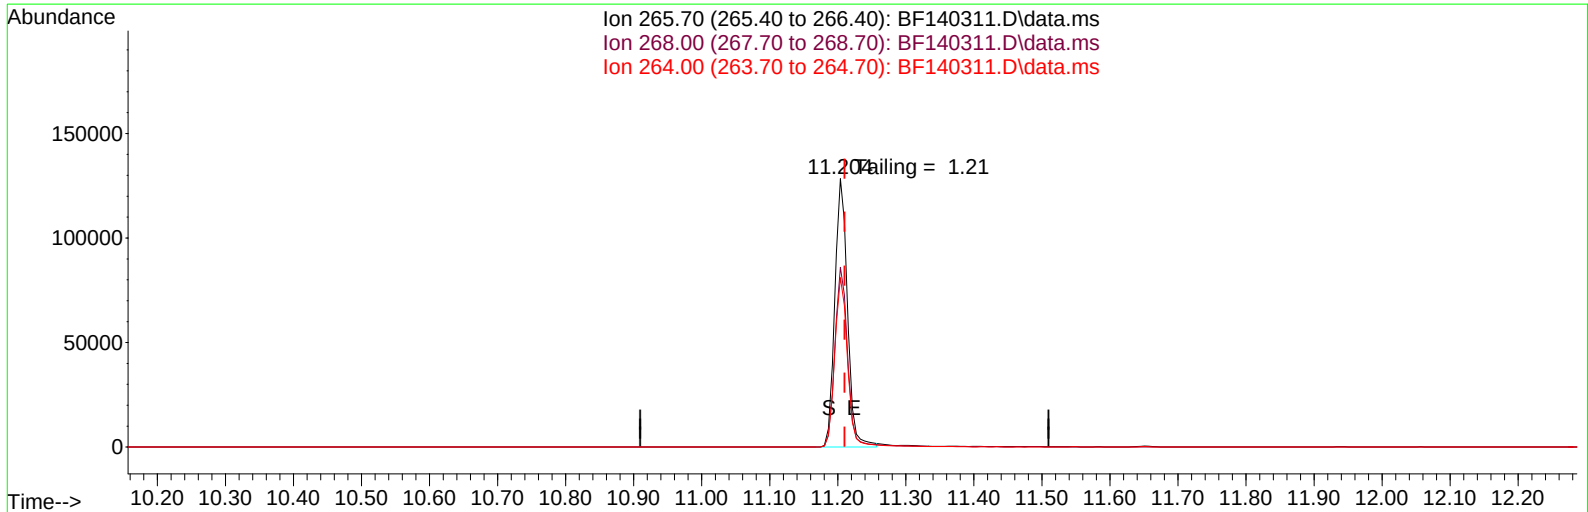

TIC: BF140311.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 28916.95 ng




response 168232

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	66.97
264.00	61.80	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111124\
Data File : BF140311.D
Acq On : 11 Nov 2024 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 12 00:12:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 12 00:05:37 2024
Response via : Initial Calibration

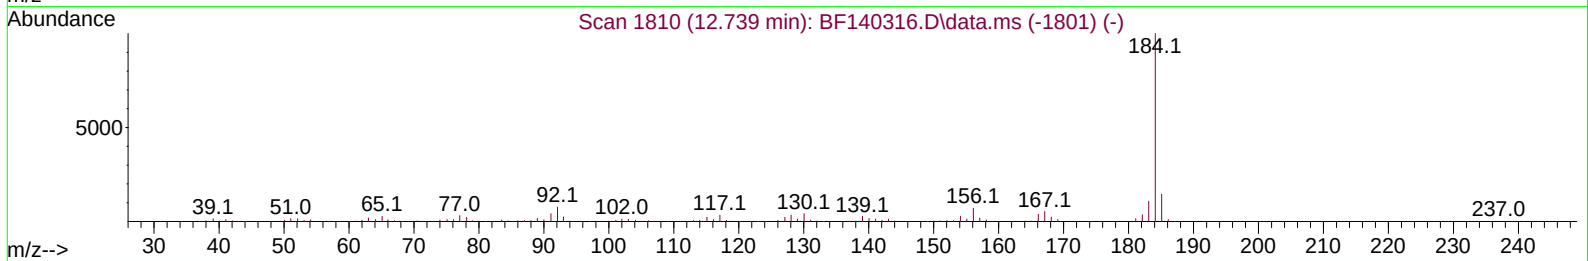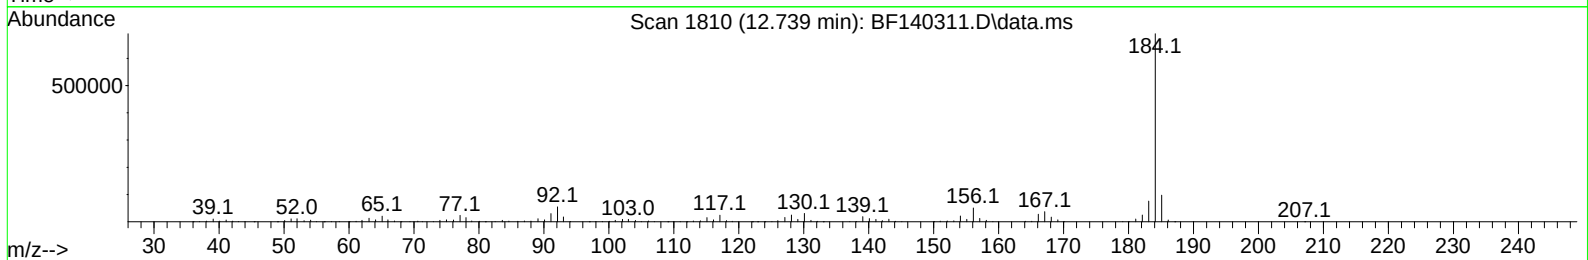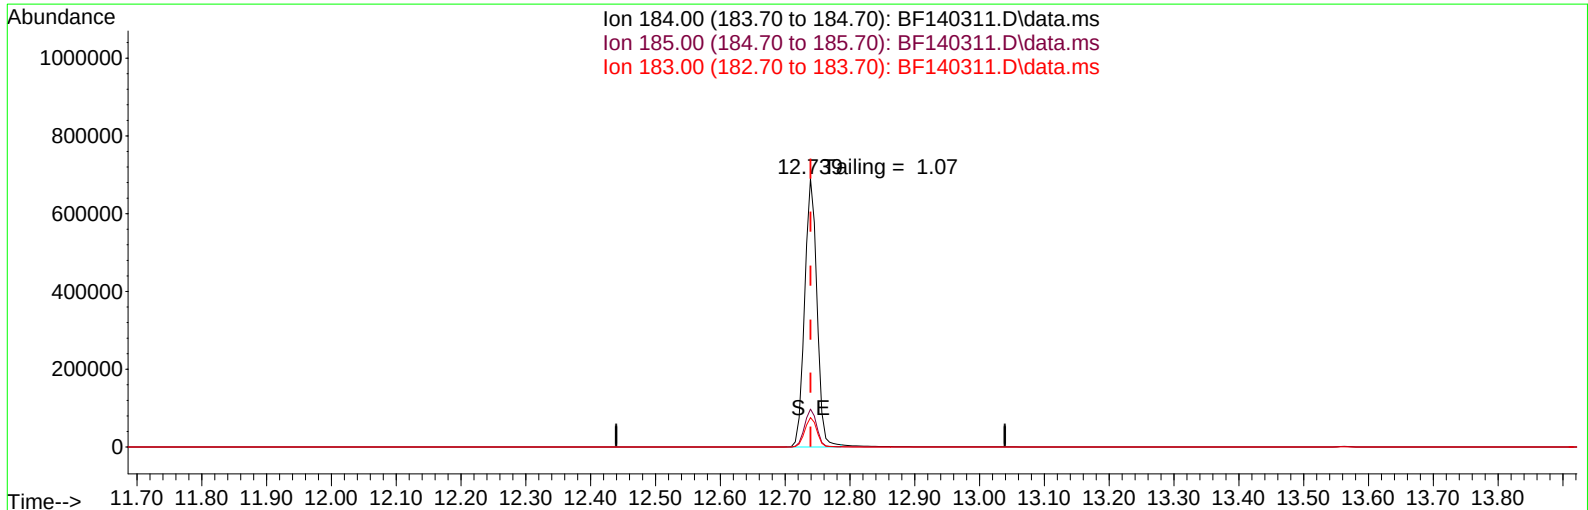

TIC: BF140311.D\data.ms

(77) Benzidine

12.739min (-0.000) 0.00 ng

response 917456

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.12
183.00	10.80	10.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2024	BNA_F	<u>BF140311.D</u>
Compound Name	Response	Retention Time
DDT	442013	13.563
DDD	10577	13.263
DDE	958	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11535	453548	2.54

Instrument :
BNA_F
ClientSampleId :
DFTPP