

Data File : BF100489.D
Acq On : 12 Nov 2017 15:00
Operator : SJ/JU
Sample : I6403-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110817-JETT-F-D-S

Quant Time: Nov 13 06:20:10 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:44:40 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	130757	20.00	ng	0.00
21) Naphthalene-d8	8.18	136	485164	20.00	ng	0.00
38) Acenaphthene-d10	9.94	164	203537	20.00	ng	0.00
63) Phenanthrene-d10	11.42	188	326099	20.00	ng	0.00
75) Chrysene-d12	14.06	240	270463	20.00	ng	0.00
86) Perylene-d12	15.54	264	192603	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	333945	40.94	ng	0.00
7) Phenol-d6	6.52	99	249359	24.79	ng	-0.01
23) Nitrobenzene-d5	7.46	82	809843	110.36	ng	0.00
41) 2,4,6-Tribromophenol	10.73	330	179828	86.70	ng	0.00
44) 2-Fluorobiphenyl	9.26	172	1378609	103.14	ng	0.00
78) Terphenyl-d14	13.01	244	969233	82.34	ng	0.00


Target Compounds						Qvalue
10) Phenol	6.53	94	31874	3.02	ng	97
19) n-Nitroso-di-n-propylamine	7.46	70	108072	15.49	ng	# 82
25) Isophorone	7.46	82	807738	52.38	ng	# 64
47) 2-Nitroaniline	9.65	65	731	2.97	ng	# 1
49) Dimethylphthalate	9.65	163	88008	5.66	ng	# 99
56) 2,4-Dinitrotoluene	9.94	165	26281	6.77	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.73	198	278	8.71	ng	# 1
66) 4-Bromophenyl-phenylether	10.72	248	11596	3.32	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

ALS Vial : 58 Sample Multiplier: 1

110817-JETT-F-D-S

Response via : Initial Calibration




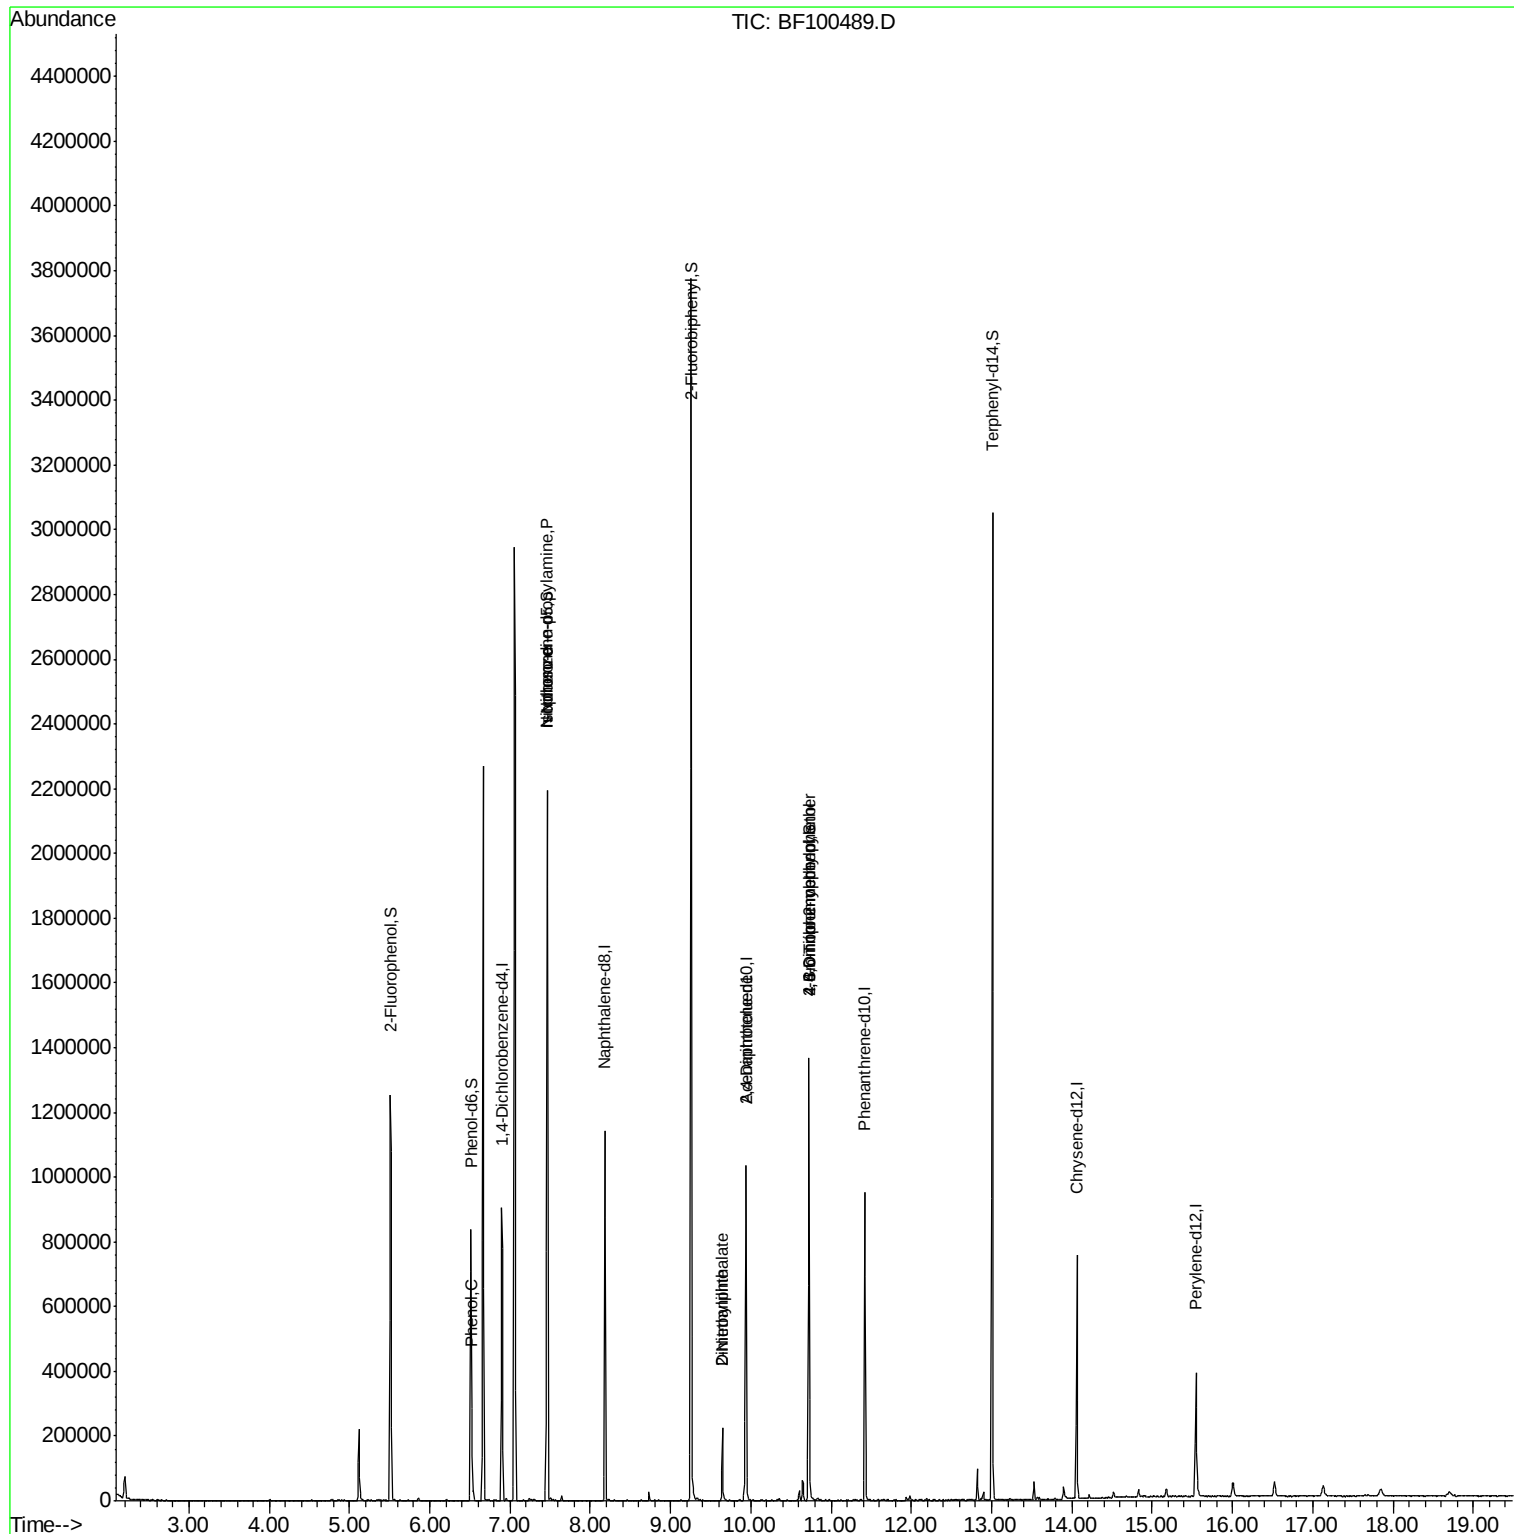


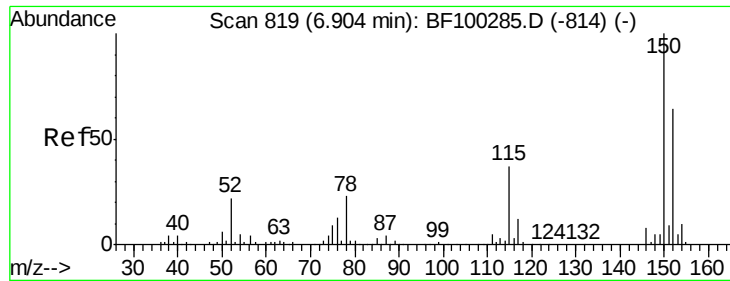

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.90 min Scan# 819
 Delta R.T. -0.01 min
 Lab File: BF100489.D
 Acq: 12 Nov 2017 15:00




Instrument :
 BNA_F
 ClientSampleId :
 110817-JETT-F-D-S

Tgt Ion:152 Resp: 130757
 Ion Ratio Lower Upper
 152 100
 150 156.5 124.6 186.8
 115 60.3 50.1 75.1

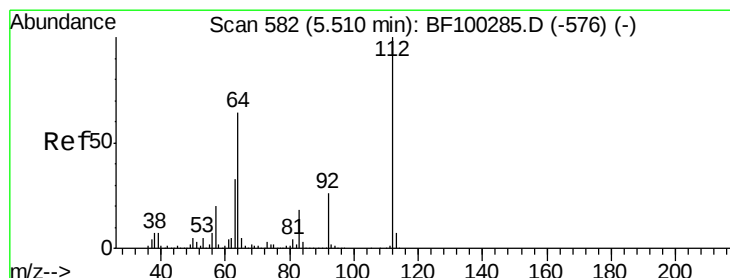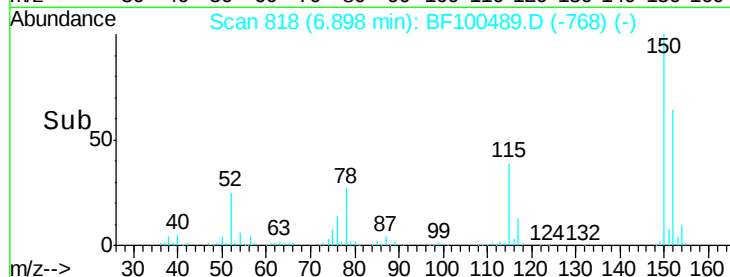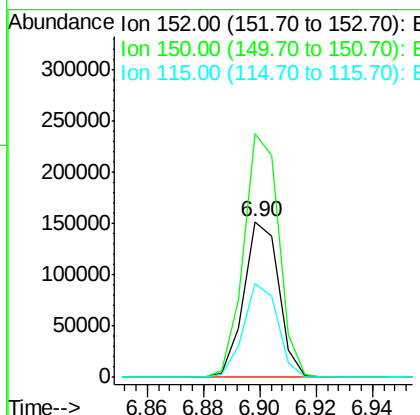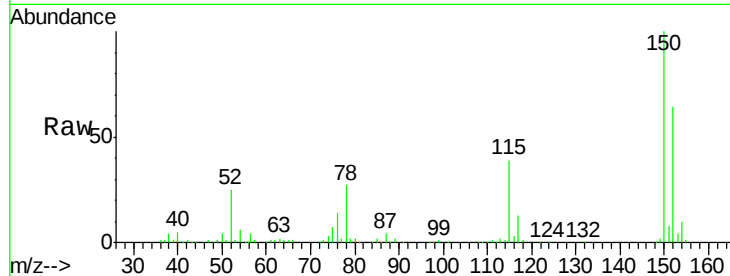

#5
 2-Fluorophenol
 Concen: 40.94 ng
 RT: 5.51 min Scan# 582
 Delta R.T. -0.01 min
 Lab File: BF100489.D
 Acq: 12 Nov 2017 15:00

Tgt Ion:112 Resp: 333945
 Ion Ratio Lower Upper
 112 100
 64 62.5 47.9 71.9
 63 31.5 23.7 35.5

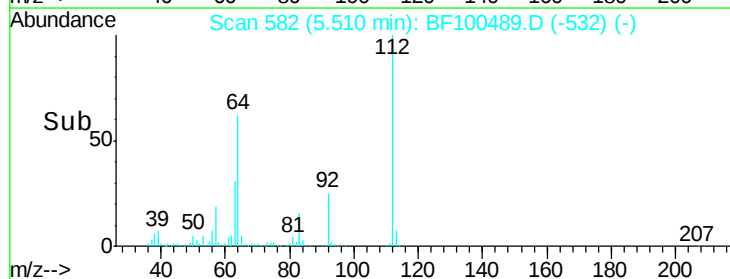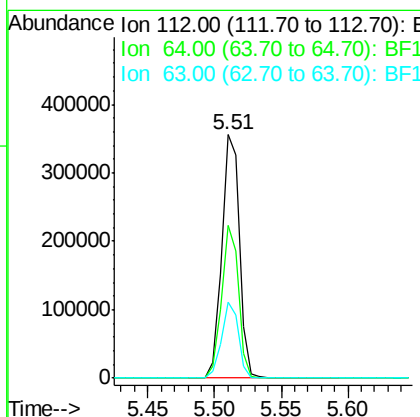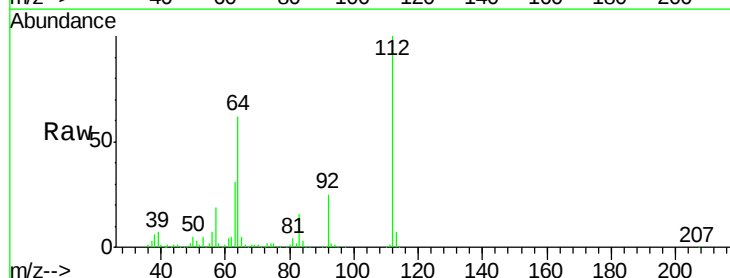



#7

Phenol-d6

Concen: 24.79 ng

RT: 6.52 min Scan# 753

Delta R.T. -0.01 min

Lab File: BF100489.D

Acq: 12 Nov 2017 15:00

Instrument :

BNA_F

ClientSampleId :

110817-JETT-F-D-S





Tgt Ion: 99 Resp: 249359

Ion Ratio Lower Upper

99 100

42 18.1 14.5 21.7

71 30.5 25.4 38.0

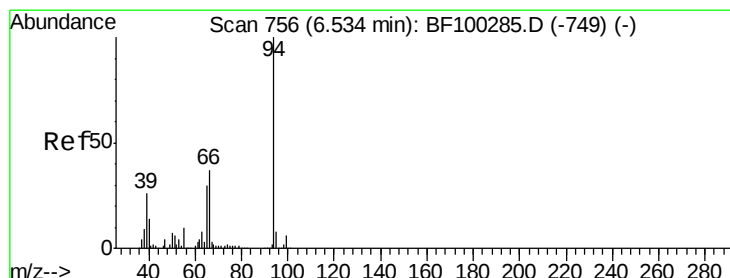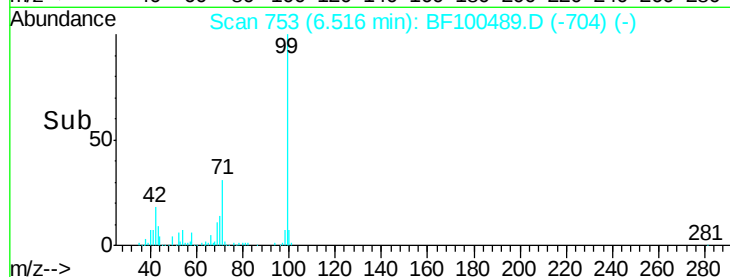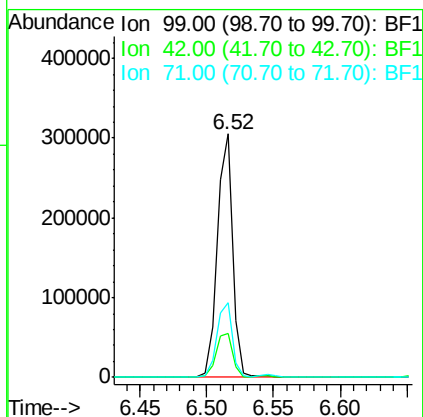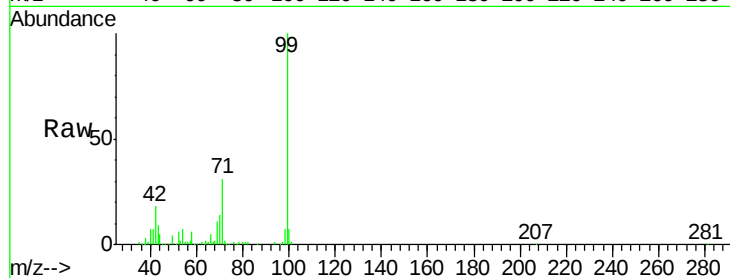

#10

Phenol

Concen: 3.02 ng

RT: 6.53 min Scan# 755

Delta R.T. -0.01 min

Lab File: BF100489.D

Acq: 12 Nov 2017 15:00




Tgt Ion: 94 Resp: 31874

Ion Ratio Lower Upper

94 100

65 26.6 7.9 47.9

66 34.1 16.2 56.2

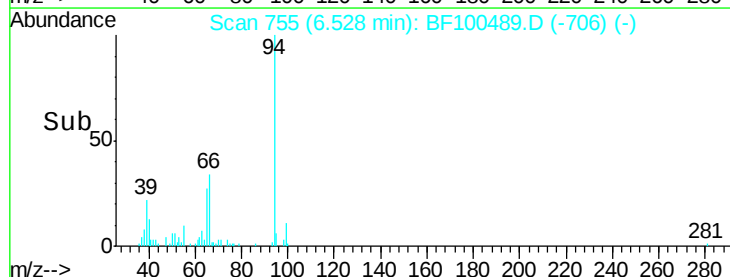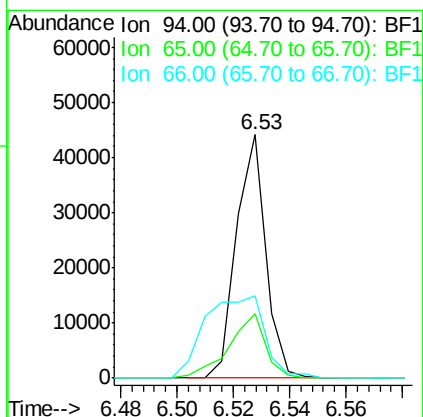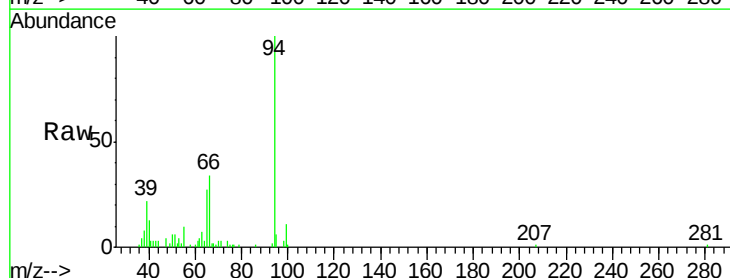



#19

n-Nitroso-di-n-propylamine

Concen: 15.49 ng

RT: 7.46 min Scan# 914

Delta R.T. 0.15 min

Lab File: BF100489.D

Acq: 12 Nov 2017 15:00

Instrument :

BNA_F

ClientSampleId :

110817-JETT-F-D-S

Tgt Ion: 70 Resp: 108072


Ion Ratio Lower Upper

70 100

42 52.3 47.5 71.3

101 0.0 7.4 11.2#

130 2.2 16.6 25.0#




Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1


Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E



Time-->

7.46

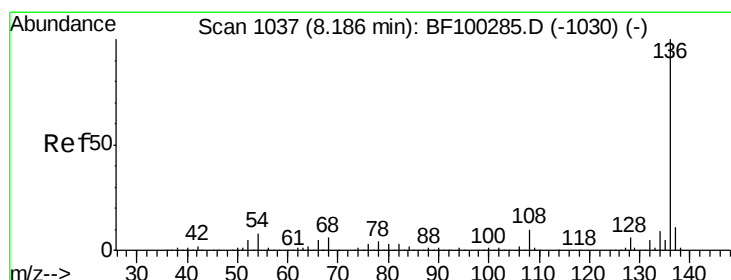

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 1036

Delta R.T. -0.01 min

Lab File: BF100489.D

Acq: 12 Nov 2017 15:00

Tgt Ion: 136 Resp: 485164


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 8.8 6.6 9.8

68 6.6 5.0 7.4




Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E


Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



Time-->





8.18

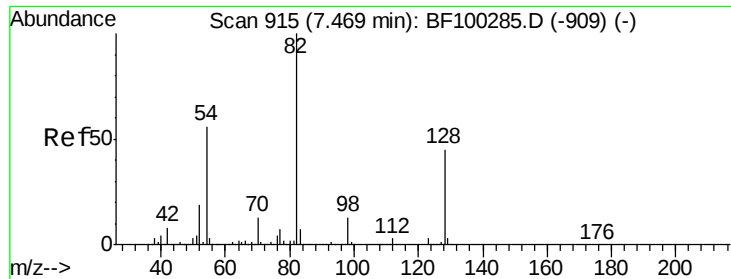

#23
 Nitrobenzene-d5
 Concen: 110.36 ng
 RT: 7.46 min Scan# 914
 Delta R.T. -0.01 min
 Lab File: BF100489.D
 Acq: 12 Nov 2017 15:00




Instrument :
 BNA_F
 ClientSampleId :
 110817-JETT-F-D-S

Tgt Ion	Ratio	Lower	Upper
82	100		
128	44.2	36.1	54.1
54	54.9	41.4	62.2

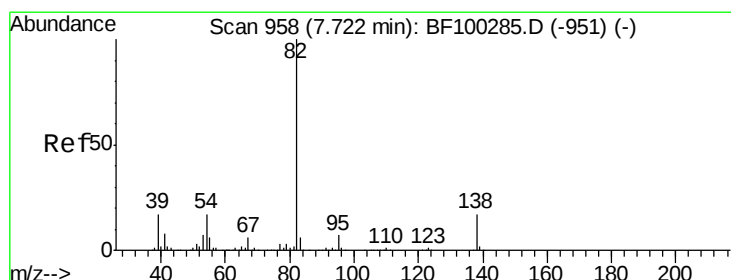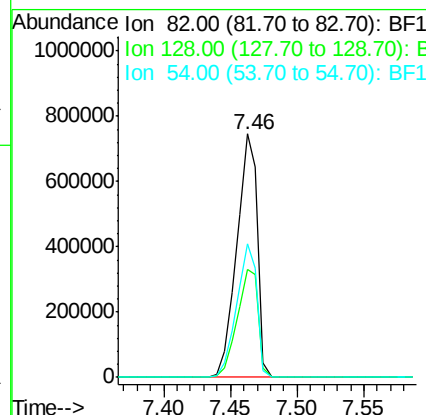

#25
 Isophorone
 Concen: 52.38 ng
 RT: 7.46 min Scan# 914
 Delta R.T. -0.26 min
 Lab File: BF100489.D
 Acq: 12 Nov 2017 15:00

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.2	7.8#
138	0.0	14.9	22.3#


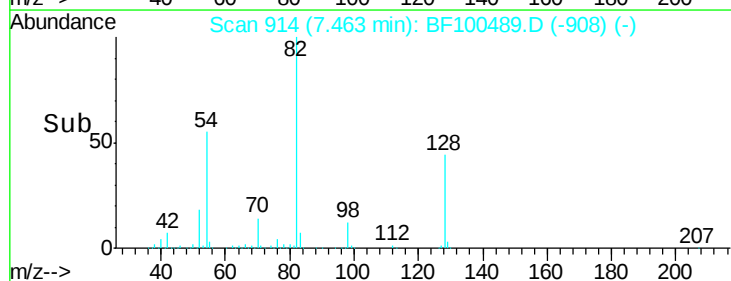
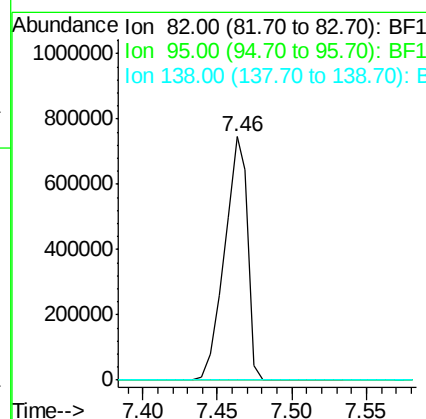
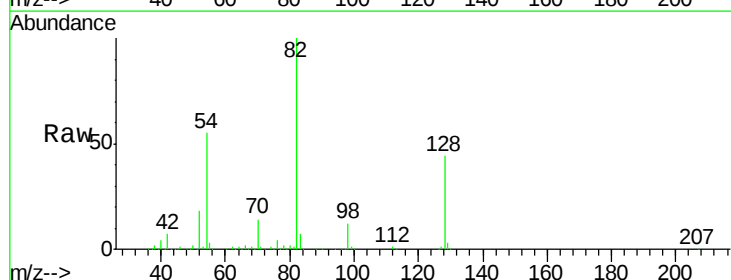




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.94 min Scan# 1335
 Delta R.T. -0.01 min
 Lab File: BF100489.D
 Acq: 12 Nov 2017 15:00




Instrument :
 BNA_F
 ClientSampleId :
 110817-JETT-F-D-S


Tgt Ion:164 Resp: 203537
 Ion Ratio Lower Upper
 164 100
 162 103.9 86.1 129.1
 160 46.8 38.3 57.5

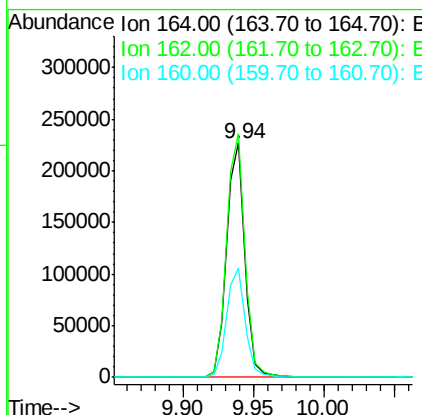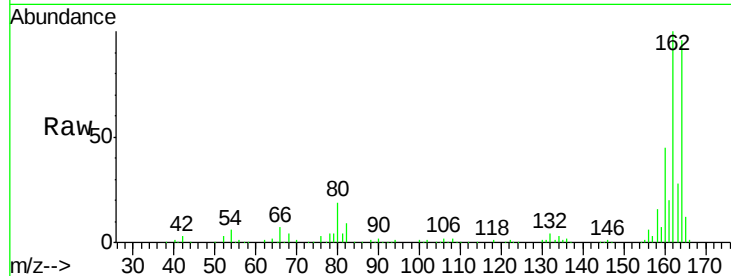

#41
 2,4,6-Tribromophenol
 Concen: 86.70 ng
 RT: 10.73 min Scan# 1469
 Delta R.T. -0.01 min
 Lab File: BF100489.D
 Acq: 12 Nov 2017 15:00

Tgt Ion:330 Resp: 179828
 Ion Ratio Lower Upper
 330 100
 332 95.6 77.0 115.6
 141 30.9 29.9 44.9



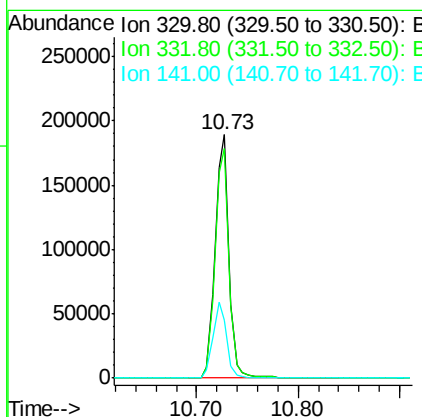



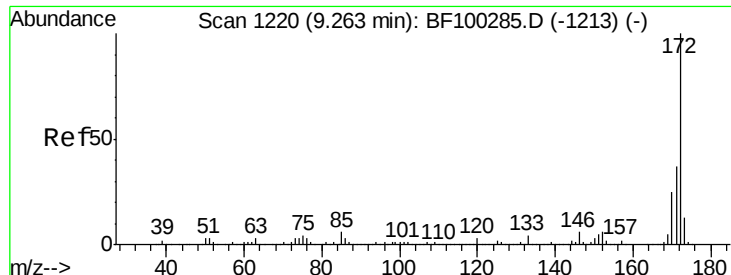

#44
 2-Fluorobiphenyl
 Concen: 103.14 ng
 RT: 9.26 min Scan# 1219
 Delta R.T. -0.01 min
 Lab File: BF100489.D
 Acq: 12 Nov 2017 15:00




Instrument :
 BNA_F
 ClientSampleId :
 110817-JETT-F-D-S


Tgt Ion: 172 Resp: 1378609
 Ion Ratio Lower Upper
 172 100
 171 36.9 29.7 44.5
 170 24.8 19.6 29.4

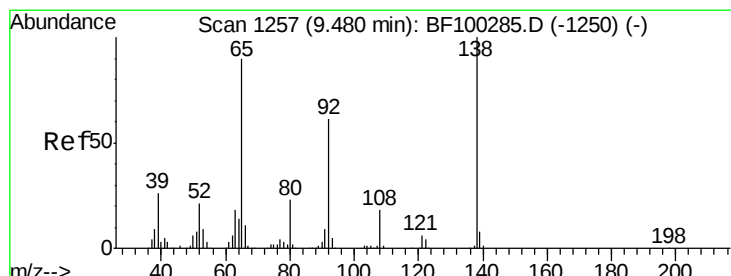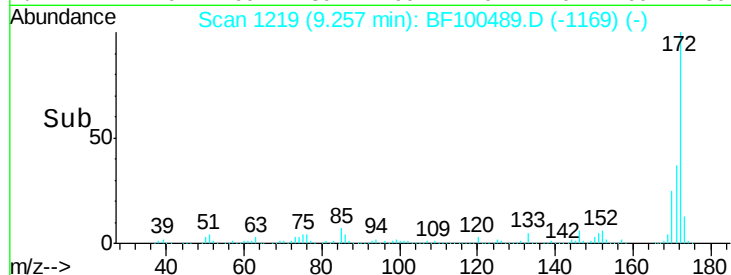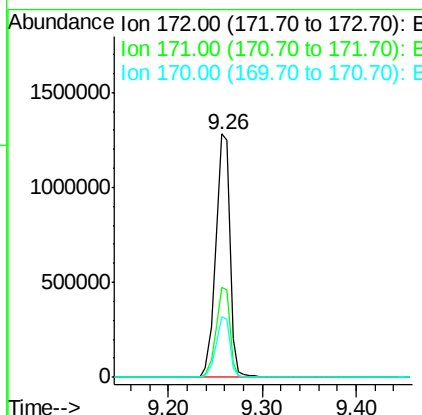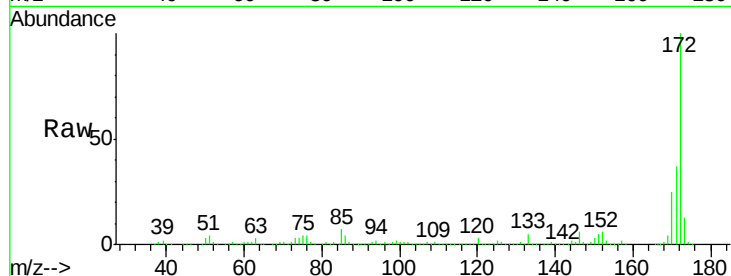

#47
 2-Nitroaniline
 Concen: 2.97 ng
 RT: 9.65 min Scan# 1285
 Delta R.T. 0.16 min
 Lab File: BF100489.D
 Acq: 12 Nov 2017 15:00

Tgt Ion: 65 Resp: 731
 Ion Ratio Lower Upper
 65 100
 92 797.5 55.8 83.6#
 138 0.0 91.2 136.8#

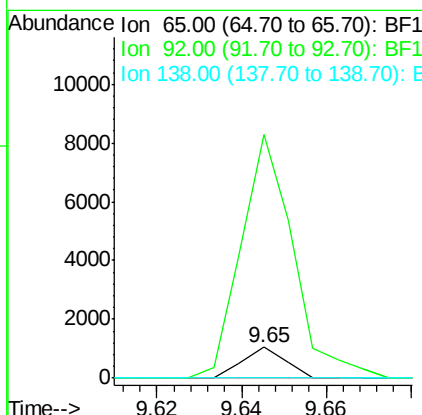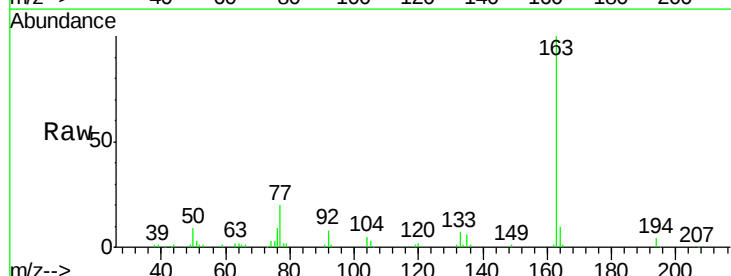


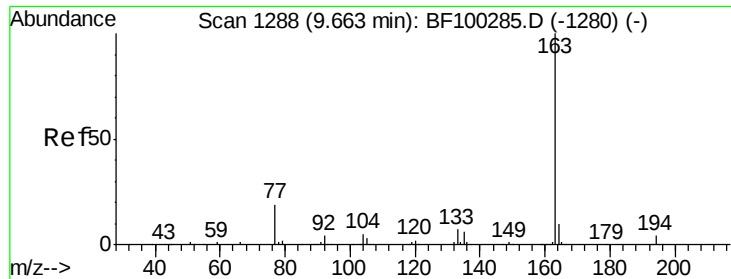




#49
Dimethylphthalate
Concen: 5.66 ng
RT: 9.65 min Scan# 1285
Delta R.T. -0.02 min
Lab File: BF100489.D
Acq: 12 Nov 2017 15:00

Instrument :
BNA_F
ClientSampleId :
110817-JETT-F-D-S

Tgt Ion:163 Resp: 88008
Ion Ratio Lower Upper
163 100
194 4.2 2.7 4.1#
164 10.3 8.2 12.2

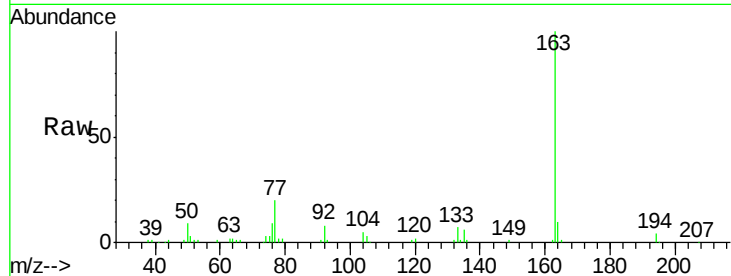


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

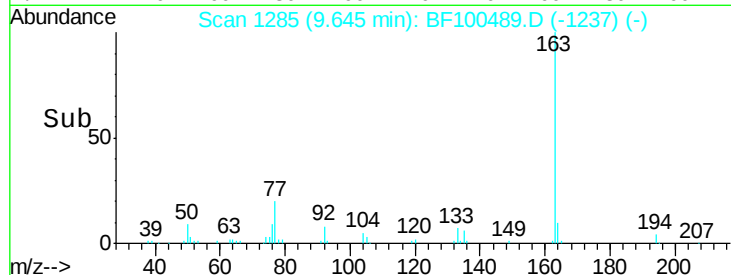
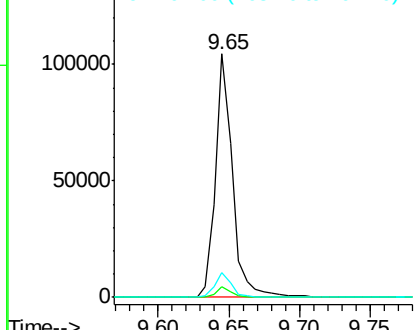



#56
2,4-Dinitrotoluene
Concen: 6.77 ng
RT: 9.94 min Scan# 1335
Delta R.T. -0.19 min
Lab File: BF100489.D
Acq: 12 Nov 2017 15:00

Tgt Ion:165 Resp: 26281
Ion Ratio Lower Upper
165 100
63 0.0 36.4 54.6#
89 1.8 57.8 86.6#
182 0.0 1.6 2.4#



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1
Ion 182.00 (181.70 to 182.70): E




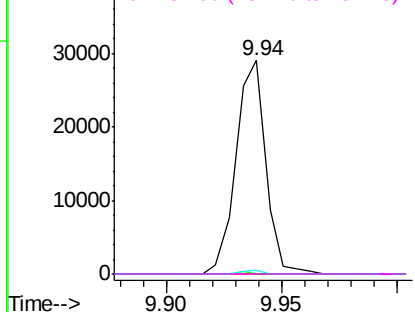




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.42 min Scan# 1587
Delta R.T. -0.01 min
Lab File: BF100489.D
Acq: 12 Nov 2017 15:00




Instrument :
BNA_F
ClientSampleId :
110817-JETT-F-D-S


Tgt Ion:188 Resp: 326099
Ion Ratio Lower Upper
188 100
94 10.1 8.5 12.7
80 11.0 9.2 13.8

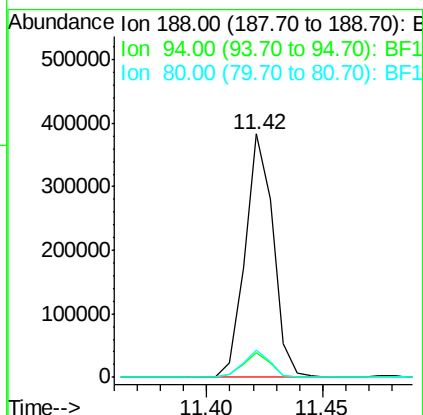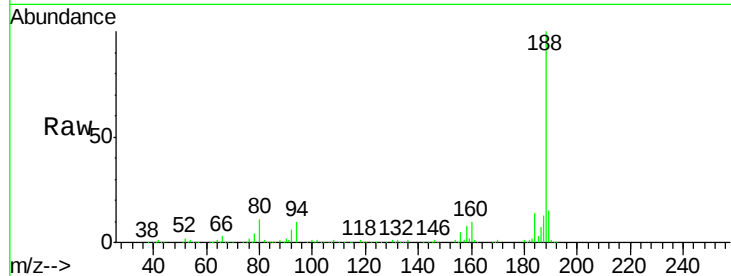

#64
4,6-Dinitro-2-methylphenol
Concen: 8.71 ng
RT: 10.73 min Scan# 1469
Delta R.T. 0.19 min
Lab File: BF100489.D
Acq: 12 Nov 2017 15:00

Tgt Ion:198 Resp: 278
Ion Ratio Lower Upper
198 100
51 188.3 37.7 77.7#
105 166.5 36.3 76.3#

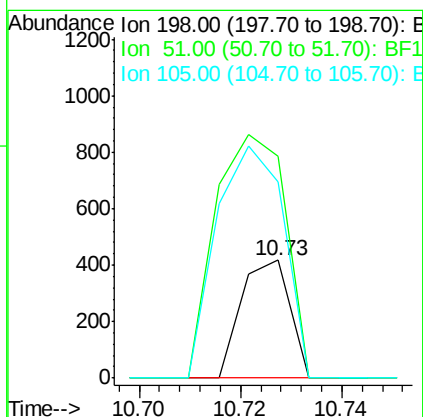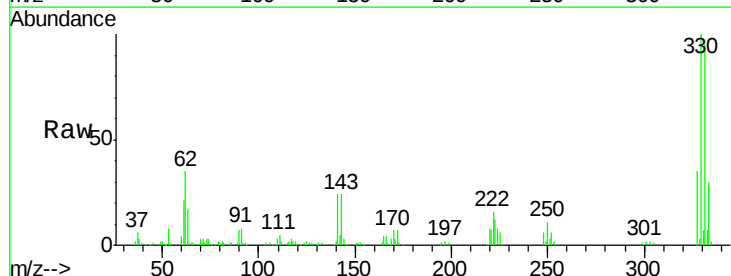


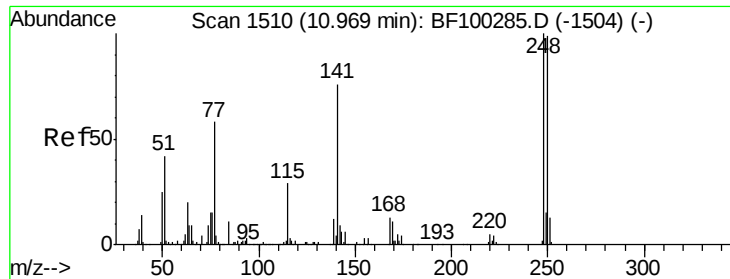




#66
4-Bromophenyl-phenylether
Concen: 3.32 ng
RT: 10.72 min Scan# 1468
Delta R.T. -0.25 min
Lab File: BF100489.D
Acq: 12 Nov 2017 15:00

Instrument :
BNA_F
ClientSampleId :
110817-JETT-F-D-S

Tgt Ion:248 Resp: 11596
Ion Ratio Lower Upper
248 100
250 178.5 76.9 115.3#
141 505.8 74.4 111.6#

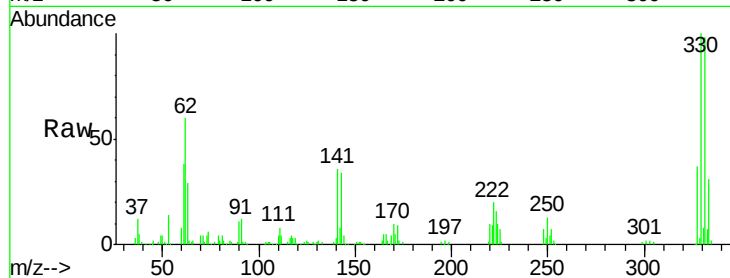


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

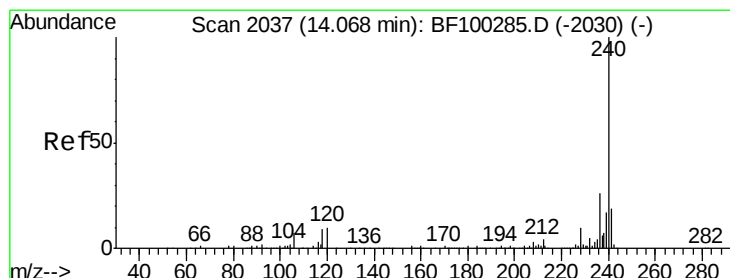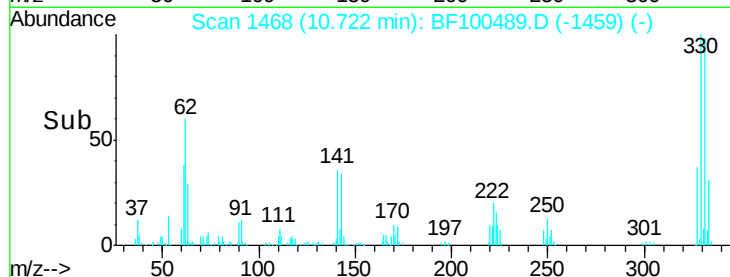
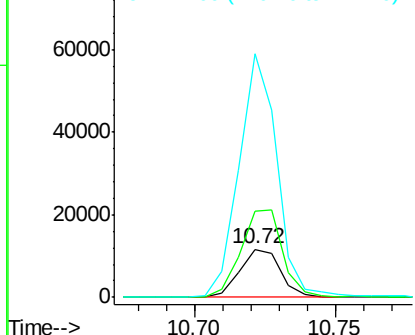



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.06 min Scan# 2036
Delta R.T. -0.01 min
Lab File: BF100489.D
Acq: 12 Nov 2017 15:00

Tgt Ion:240 Resp: 270463
Ion Ratio Lower Upper
240 100
120 11.6 9.5 14.3
236 24.9 20.7 31.1

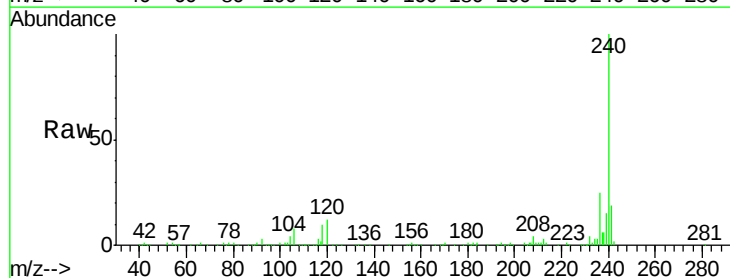

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

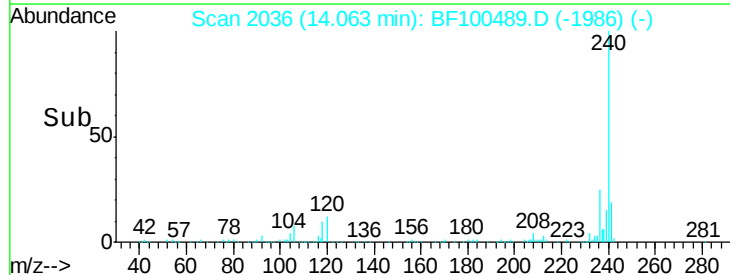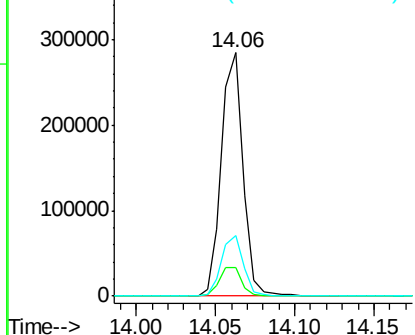



#78

Terphenyl-d14

Concen: 82.34 ng

RT: 13.01 min Scan# 1857

Delta R.T. -0.00 min

Lab File: BF100489.D

Acq: 12 Nov 2017 15:00

Instrument :

BNA_F

ClientSampleId :

110817-JETT-F-D-S


Tgt Ion:244 Resp: 969233

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0




122 11.1 11.0 16.4

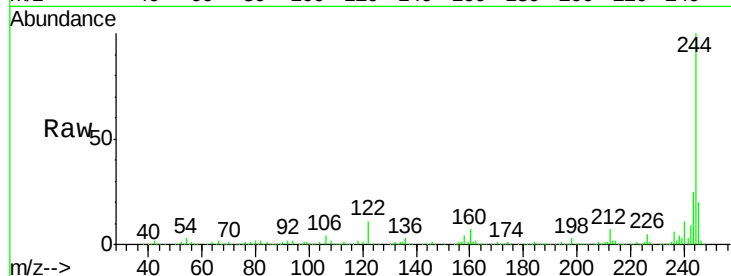

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

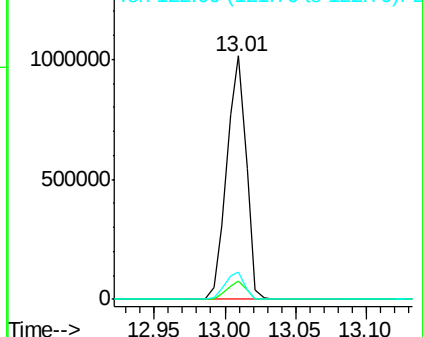

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.54 min Scan# 2288

Delta R.T. -0.00 min

Lab File: BF100489.D

Acq: 12 Nov 2017 15:00


Tgt Ion:264 Resp: 192603

Ion Ratio Lower Upper

264 100

260 22.7 19.2 28.8

265 21.1 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

