


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF111217\
 Data File : BF100479.D
 Acq On : 12 Nov 2017 10:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 13 14:08:38 2017

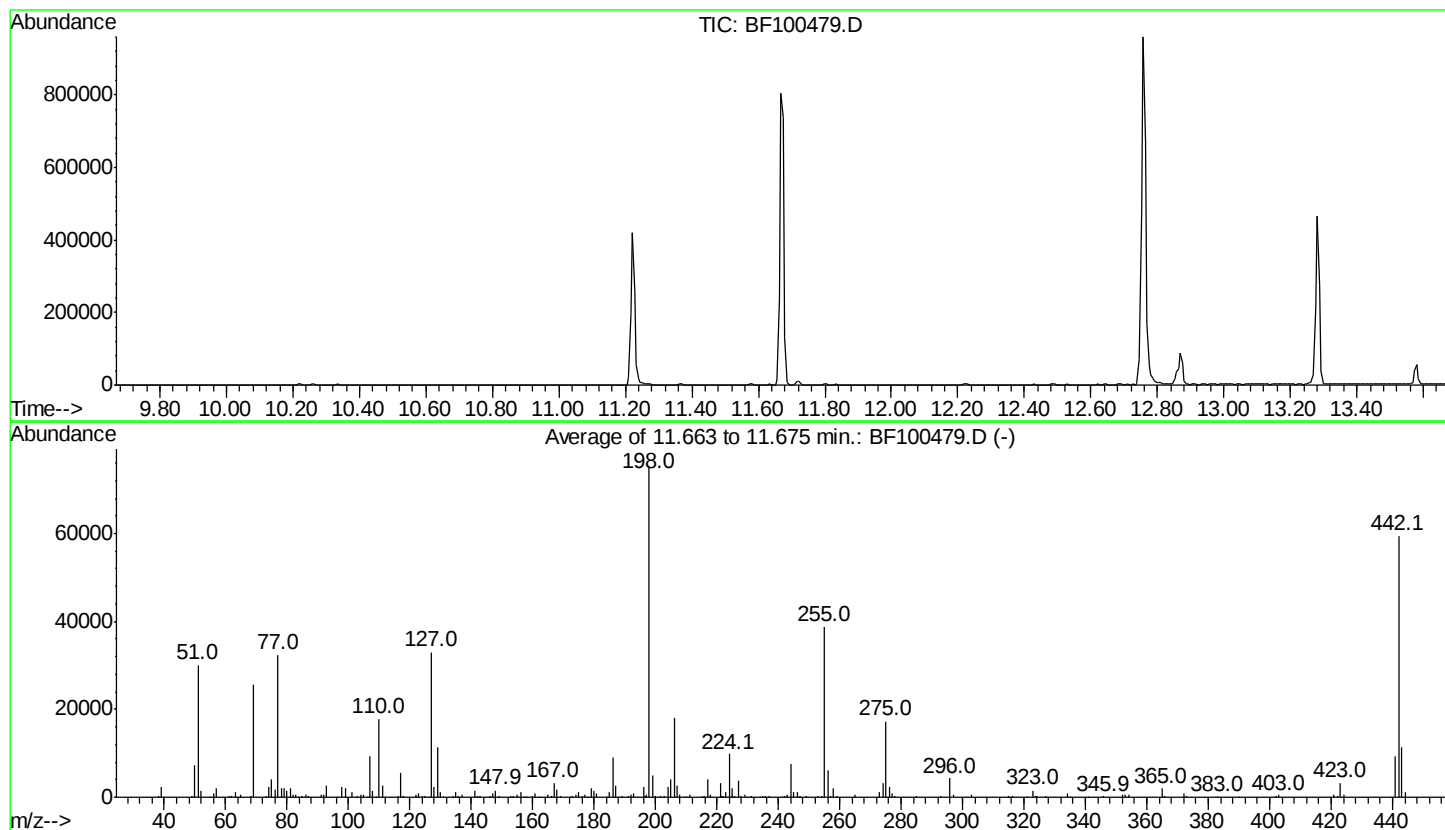

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	30085	PASS
68	69	0.00	2	0.9	234	PASS
69	198	0.00	100	34.0	25644	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.8	33034	PASS
197	198	0.00	2	0.8	611	PASS
198	198	100	100	100.0	75450	PASS
199	198	5	9	6.7	5061	PASS
275	198	10	60	22.8	17198	PASS
365	198	1	100	2.7	2022	PASS
441	443	0.01	100	81.3	9225	PASS
442	198	50	100	78.8	59482	PASS
443	442	15	24	19.1	11347	PASS