
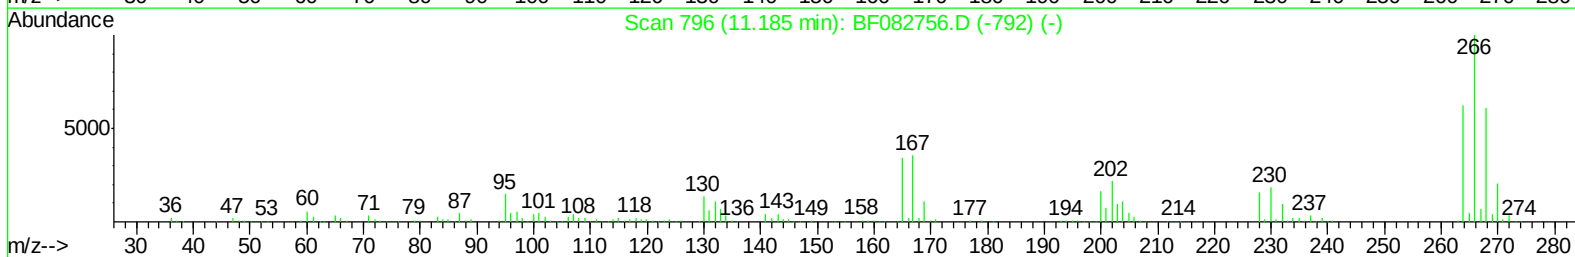
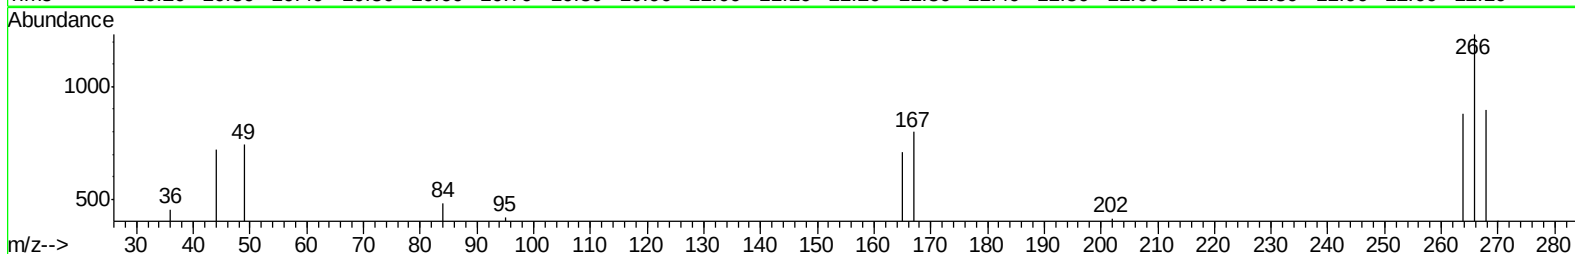


Data Path : Z:\HPCHEM1\BNA_F\Data\BF111315\
 Data File : BF082892.D
 Acq On : 13 Nov 2015 11:37
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 07:26:49 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 07 02:32:49 2015
 Response via : Initial Calibration

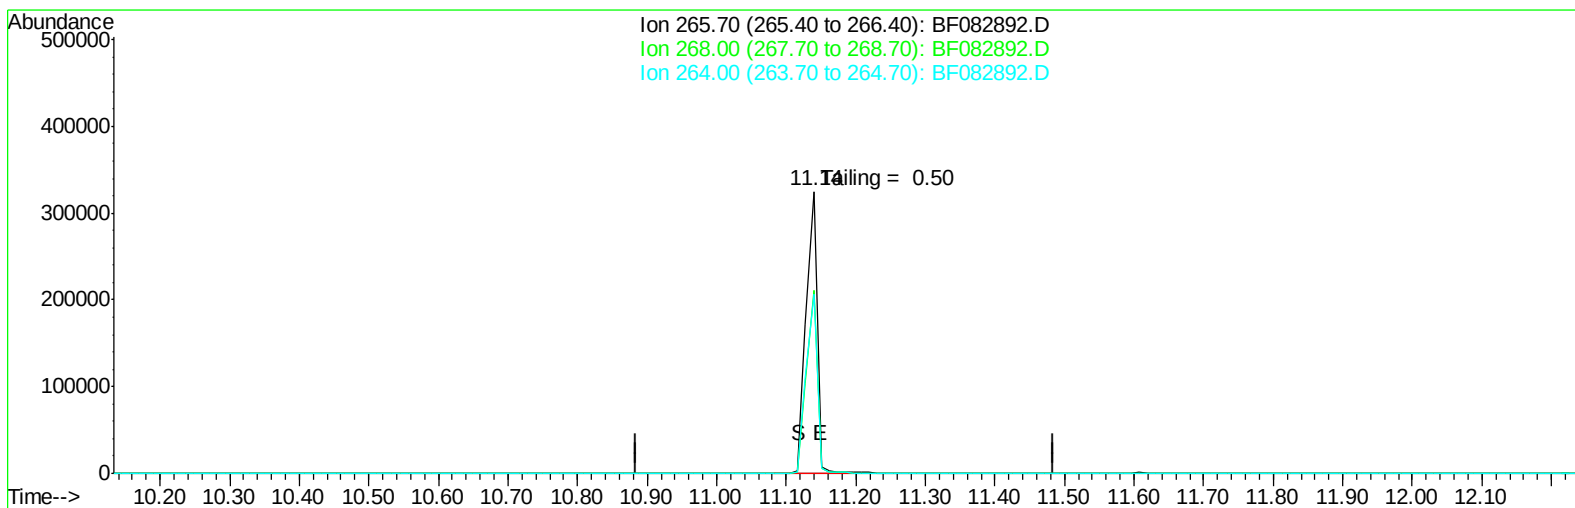

TIC: BF082892.D

(69) Pentachlorophenol (C)




11.185min (-11.185) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.80	0.00#
264.00	63.20	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF111315\
Data File : BF082892.D
Acq On : 13 Nov 2015 11:37
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 07:26:49 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

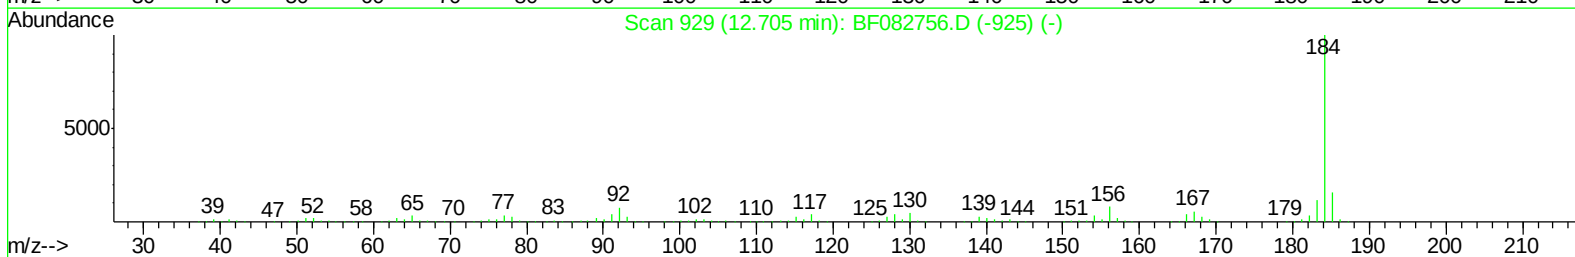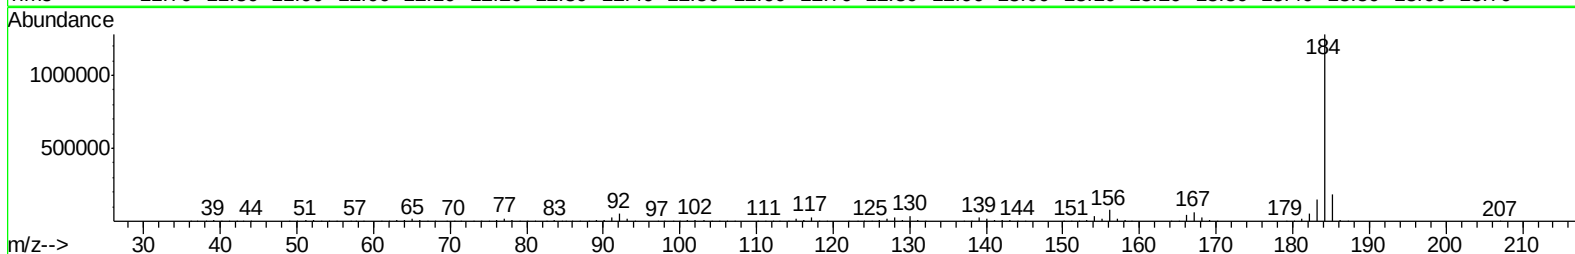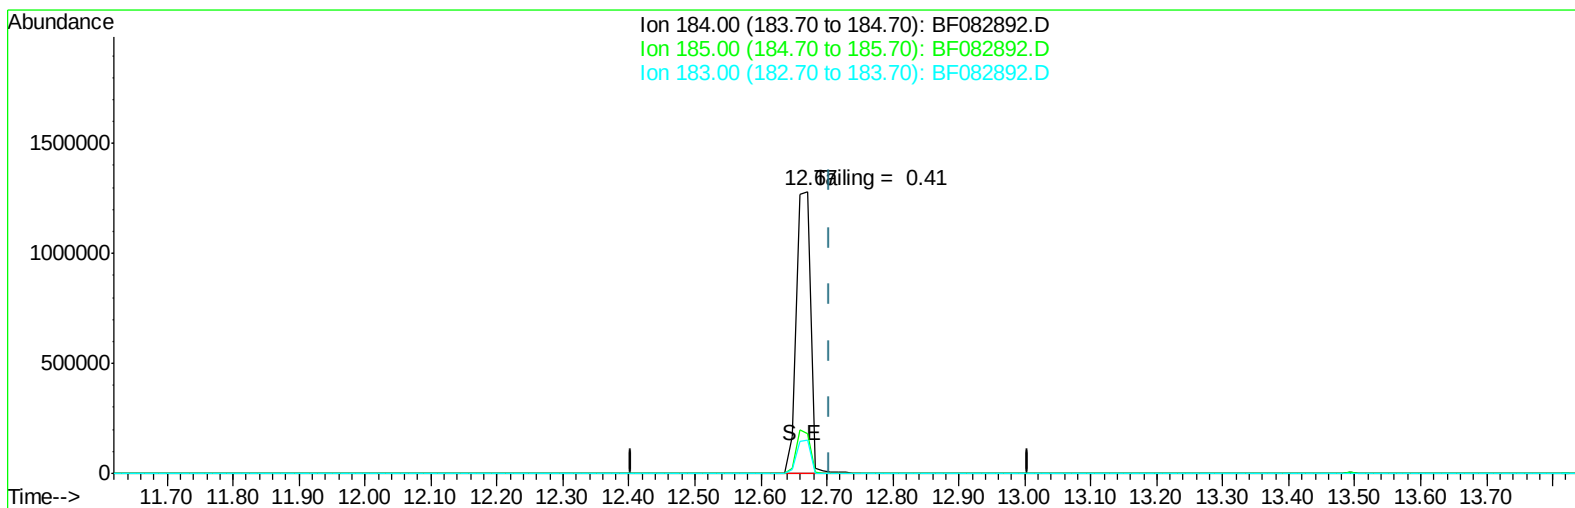

TIC: BF082892.D

(76) Benzidine

12.671min (-0.034) 0.00ng

response 1908784

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.22
183.00	12.00	11.67
0.00	0.00	0.00