
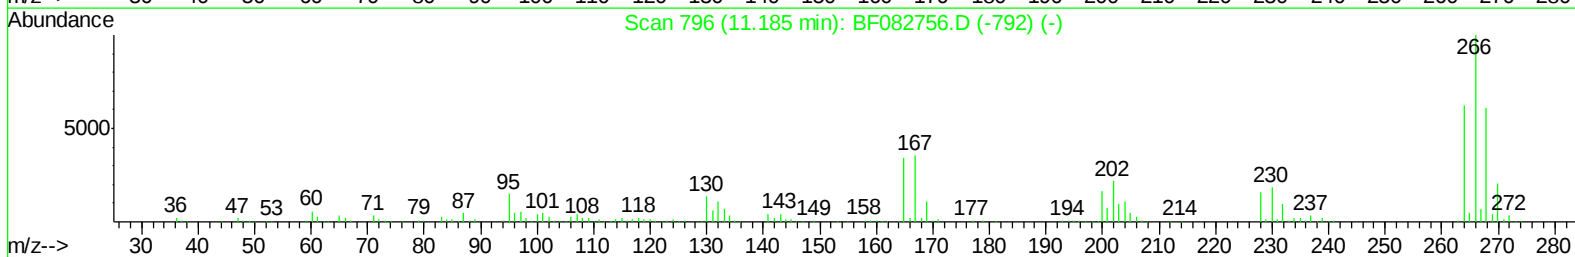
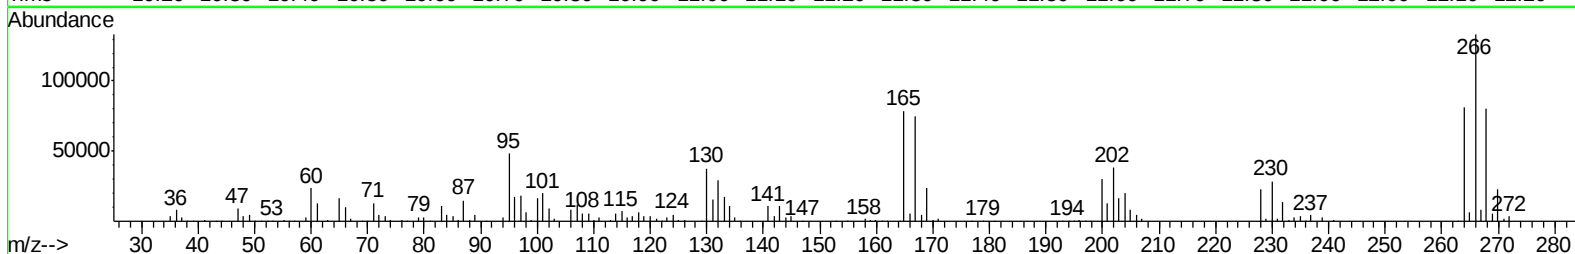


Data Path : Z:\HPCHEM1\BNA_F\Data\BF111315\
Data File : BF082915.D
Acq On : 14 Nov 2015 00:52
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 07:33:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

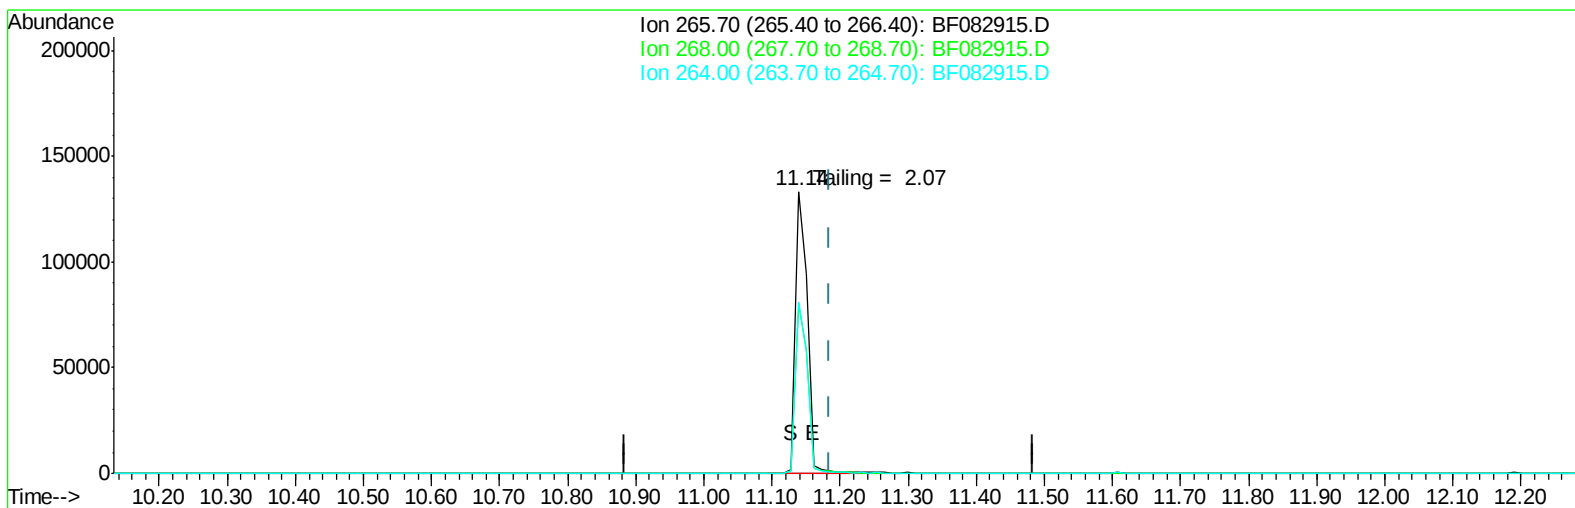

TIC: BF082915.D

(69) Pentachlorophenol (C)




11.139min (-0.046) 16818.69ng

response 163680

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	60.21
264.00	63.20	60.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF111315\
Data File : BF082915.D
Acq On : 14 Nov 2015 00:52
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 07:33:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

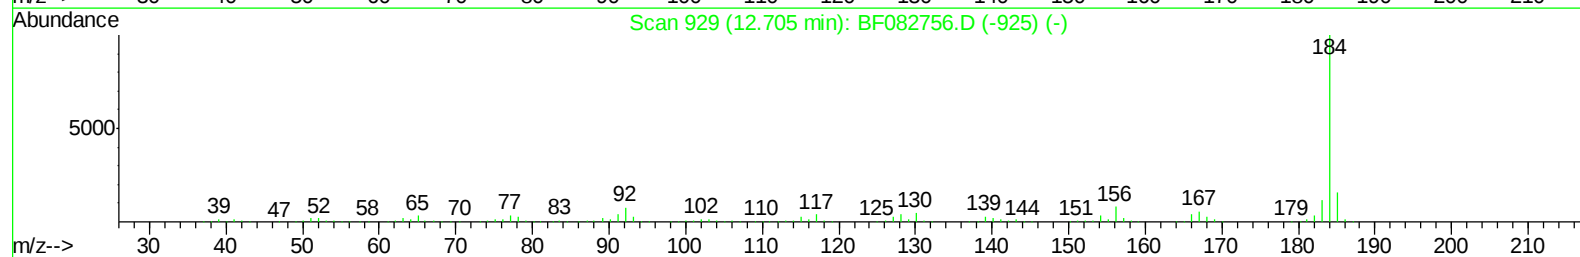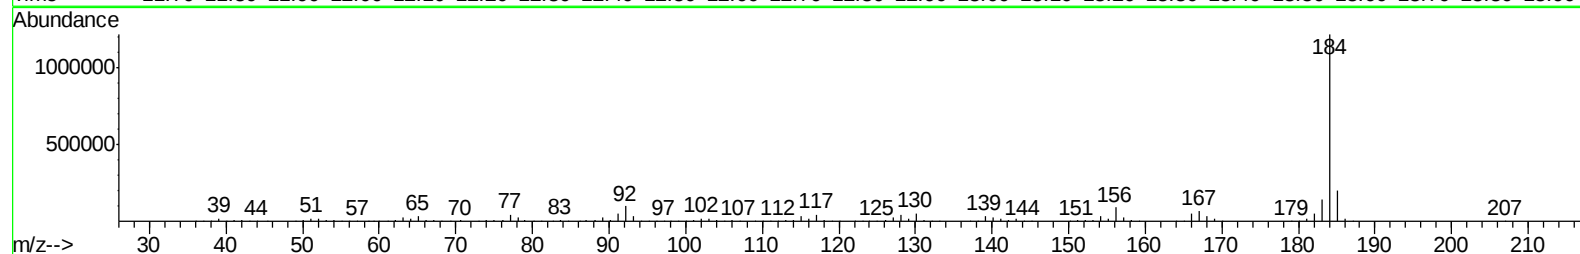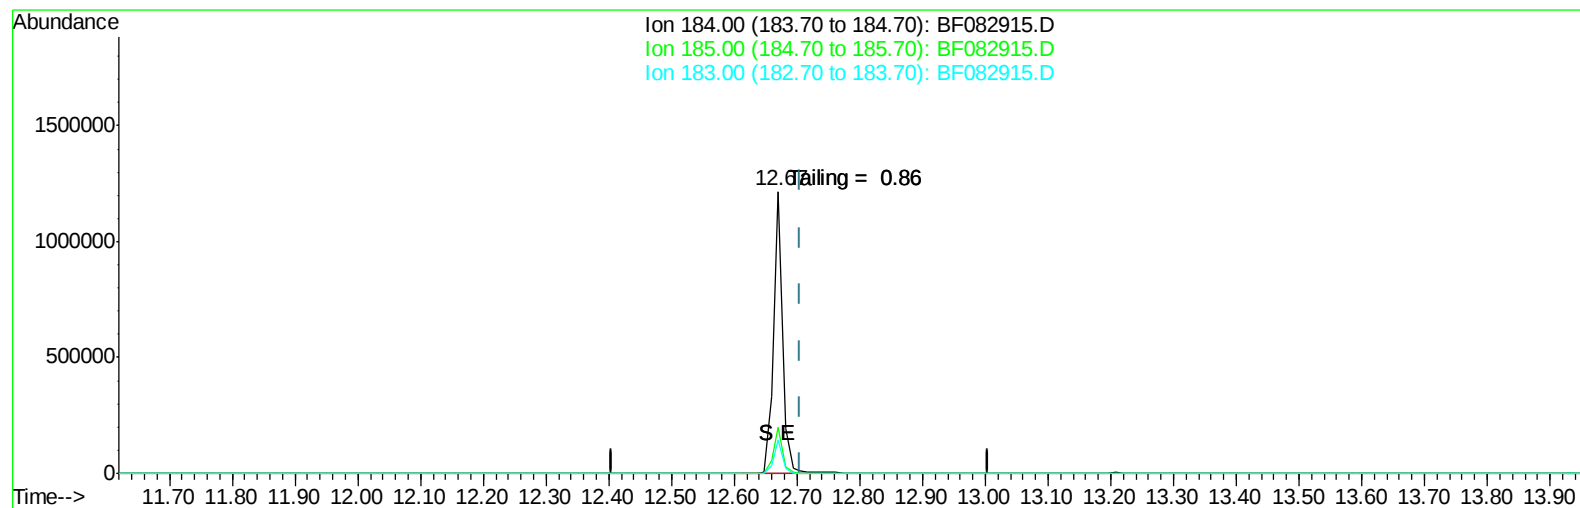

TIC: BF082915.D

(76) Benzidine

12.671min (-0.034) 0.00ng

response 1245711

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	16.20
183.00	12.00	11.70
0.00	0.00	0.00