

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111315\
 Data File : BF082896.D
 Acq On : 13 Nov 2015 14:37
 Operator : UM/IZ
 Sample : G4366-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.979	249	253	261	rVB	1897377	3263702	45.72%	5.028%
2	5.401	287	290	293	rBV	4733222	5570741	78.04%	8.582%
3	6.441	378	381	383	rBV	5811589	6647937	93.13%	10.241%
4	6.567	389	392	394	rBV	5860270	5706228	79.94%	8.791%
5	6.796	410	412	414	rBV	2092264	1704899	23.88%	2.626%
6	6.956	423	426	428	rBV	5034205	4437887	62.17%	6.837%
7	7.367	458	462	464	rBV	3202919	4292467	60.13%	6.613%
8	8.087	522	525	527	rBV	2382038	2322959	32.54%	3.579%
9	9.173	616	620	622	rBV	4791459	6888410	96.50%	10.612%
10	9.562	651	654	656	rBV	1520594	1319690	18.49%	2.033%
11	9.836	676	678	681	rVB	2234194	2645087	37.05%	4.075%
12	10.625	744	747	750	rBV2	3578485	4401501	61.66%	6.781%
13	10.762	757	759	763	rBV2	63488	97213	1.36%	0.150%
14	11.196	794	797	799	rBV2	63361	106116	1.49%	0.163%
15	11.322	805	808	810	rVV	3128256	2717587	38.07%	4.187%
16	11.859	853	855	860	rVB4	39090	74063	1.04%	0.114%
17	12.911	944	947	950	rBV	5148540	7138313	100.00%	10.997%
18	13.391	987	989	992	rBV	62609	83827	1.17%	0.129%
19	13.574	1003	1005	1006	rVB	97292	80097	1.12%	0.123%
20	13.962	1036	1039	1041	rVV	2820006	2999994	42.03%	4.622%
21	15.391	1160	1164	1166	rBV	1880914	2413588	33.81%	3.718%


Sum of corrected areas: 64912306

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111315\
Data File : BF082896.D
Acq On : 13 Nov 2015 14:37
Operator : UM/IZ
Sample : G4366-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

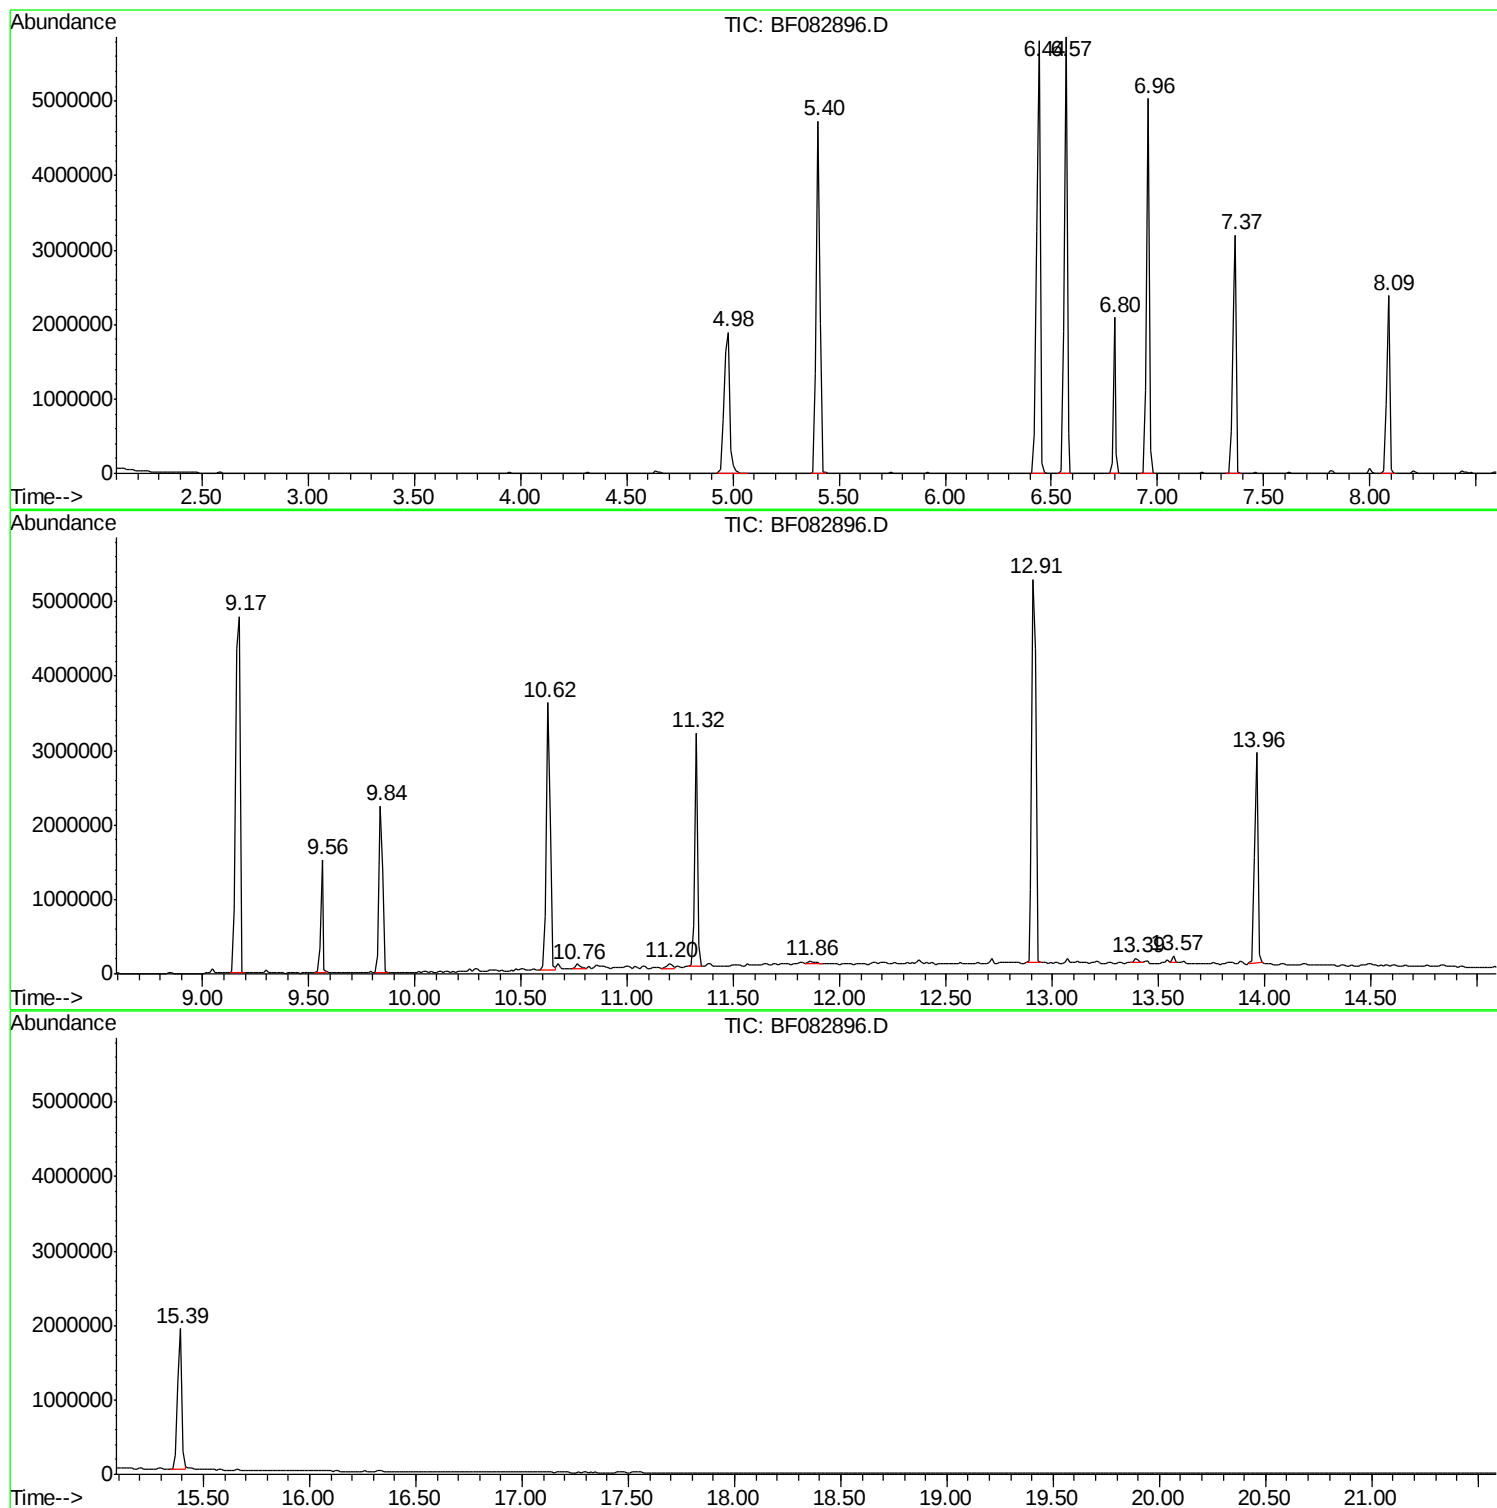

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111315\
Data File : BF082896.D
Acq On : 13 Nov 2015 14:37
Operator : UM/IZ
Sample : G4366-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-1










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.98	38.29 ng	3263700	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

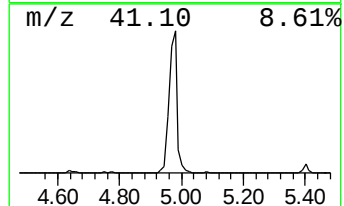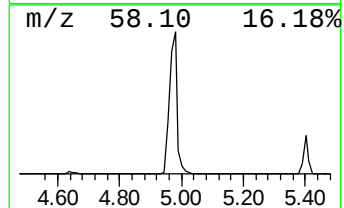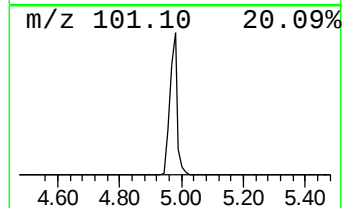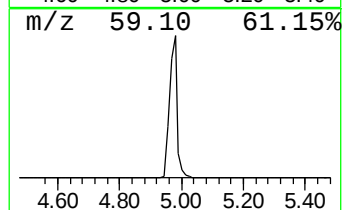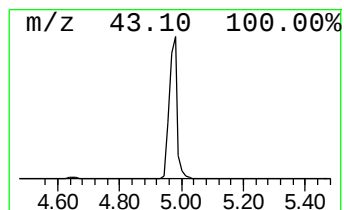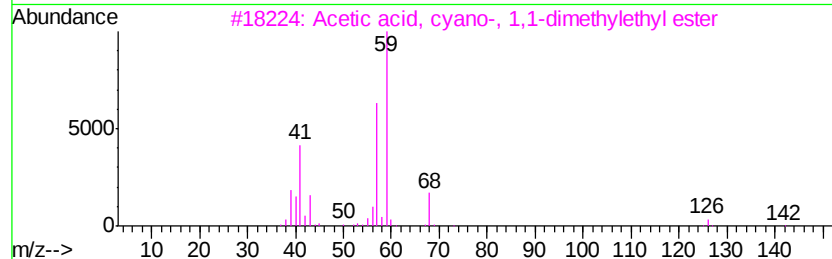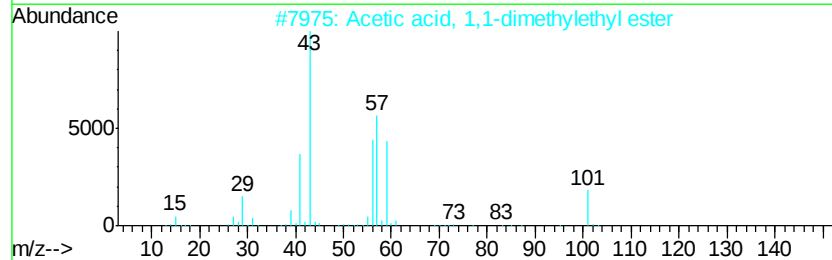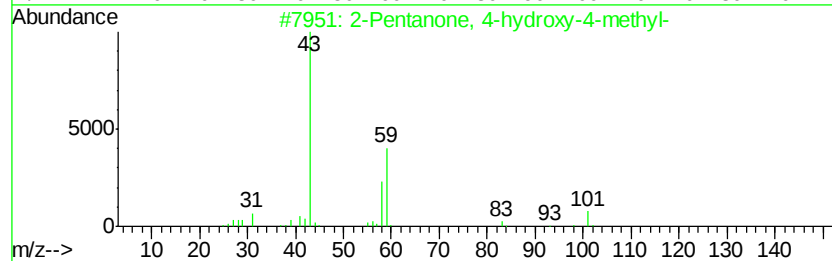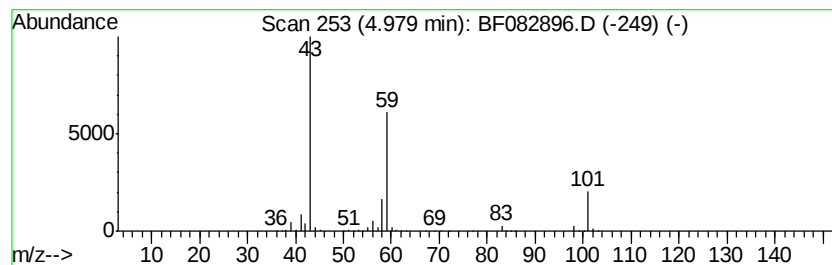

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111315\
Data File : BF082896.D
Acq On : 13 Nov 2015 14:37
Operator : UM/IZ
Sample : G4366-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.57 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.57	66.94 ng	5706230	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		2-Cyclohexen-1-one	96	C6H8O	000930-68-7	10
4		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
5		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10

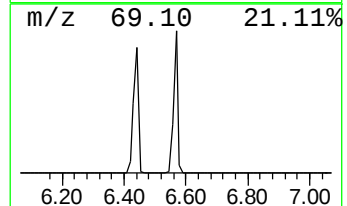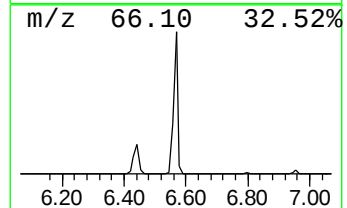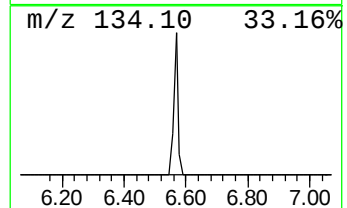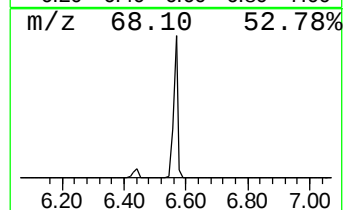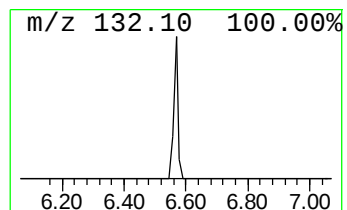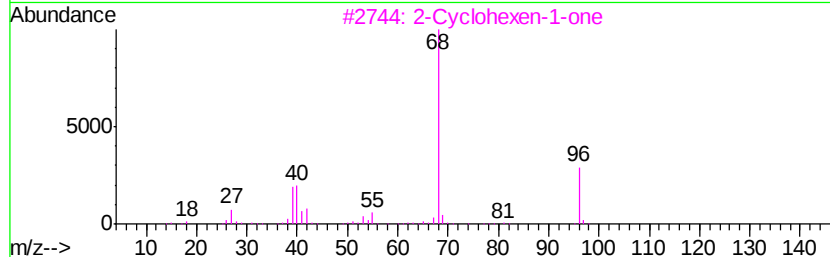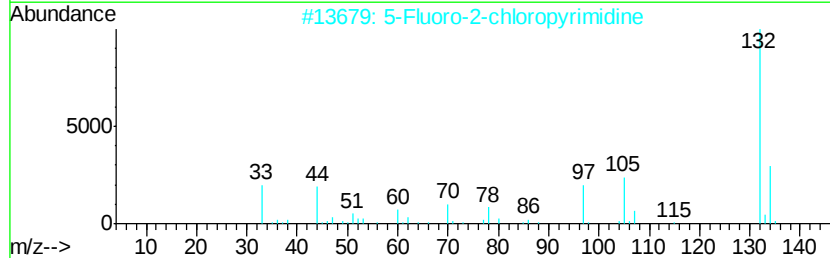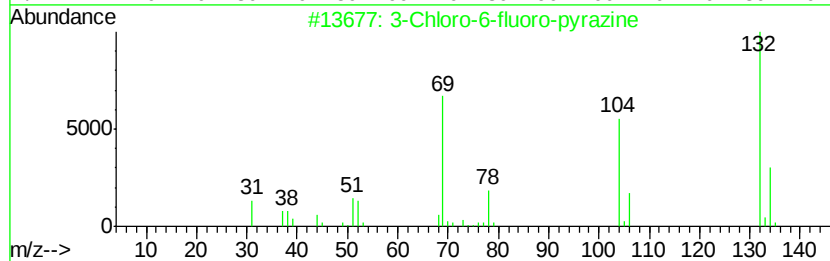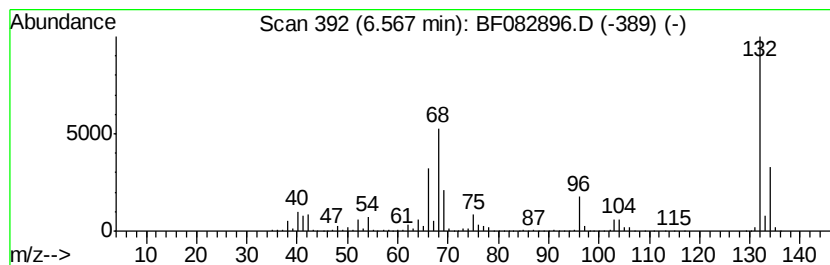

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111315\
Data File : BF082896.D
Acq On : 13 Nov 2015 14:37
Operator : UM/IZ
Sample : G4366-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.98	38.3	ng	3263700	1	6.80	1704900	20.0
unknown6.57	6.57	66.9	ng	5706230	1	6.80	1704900	20.0