


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111315\
 Data File : BF082892.D
 Acq On : 13 Nov 2015 11:37
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 07 02:32:49 2015

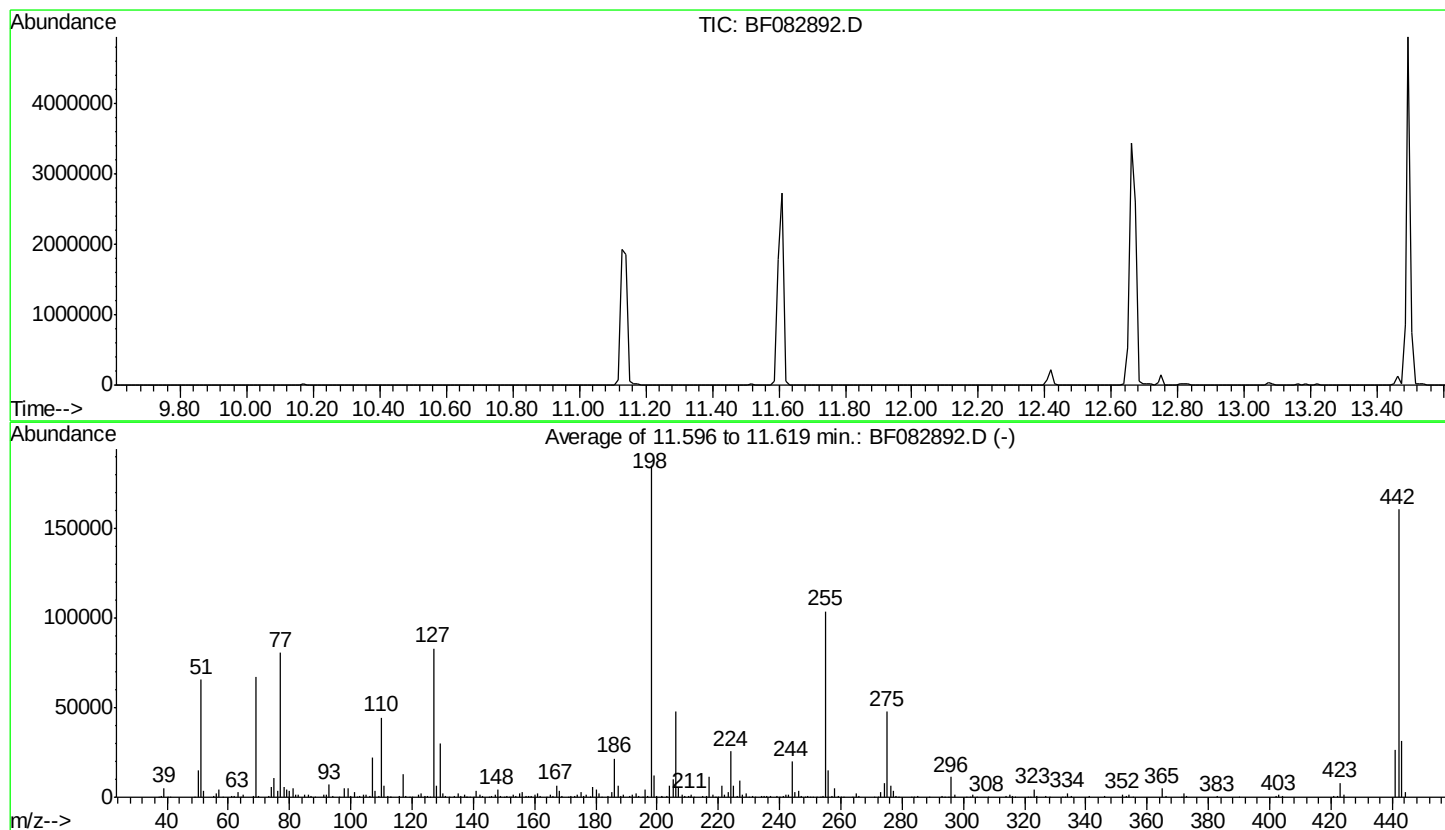

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	65589	PASS
68	69	0.00	2	1.4	947	PASS
69	198	0.00	100	36.3	67122	PASS
70	69	0.00	2	0.6	393	PASS
127	198	10	80	44.8	82834	PASS
197	198	0.00	2	0.6	1084	PASS
198	198	100	100	100.0	184861	PASS
199	198	5	9	6.6	12181	PASS
275	198	10	60	25.7	47587	PASS
365	198	1	100	2.6	4718	PASS
441	442	0.01	24	16.6	26678	PASS
442	198	50	100	86.7	160328	PASS
443	442	15	24	19.5	31305	PASS