


Data Path : Z:\HPCHEM1\BNA F\DATA\BF111315\
 Data File : BF082915.D
 Acq On : 14 Nov 2015 00:52
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 07 02:32:49 2015

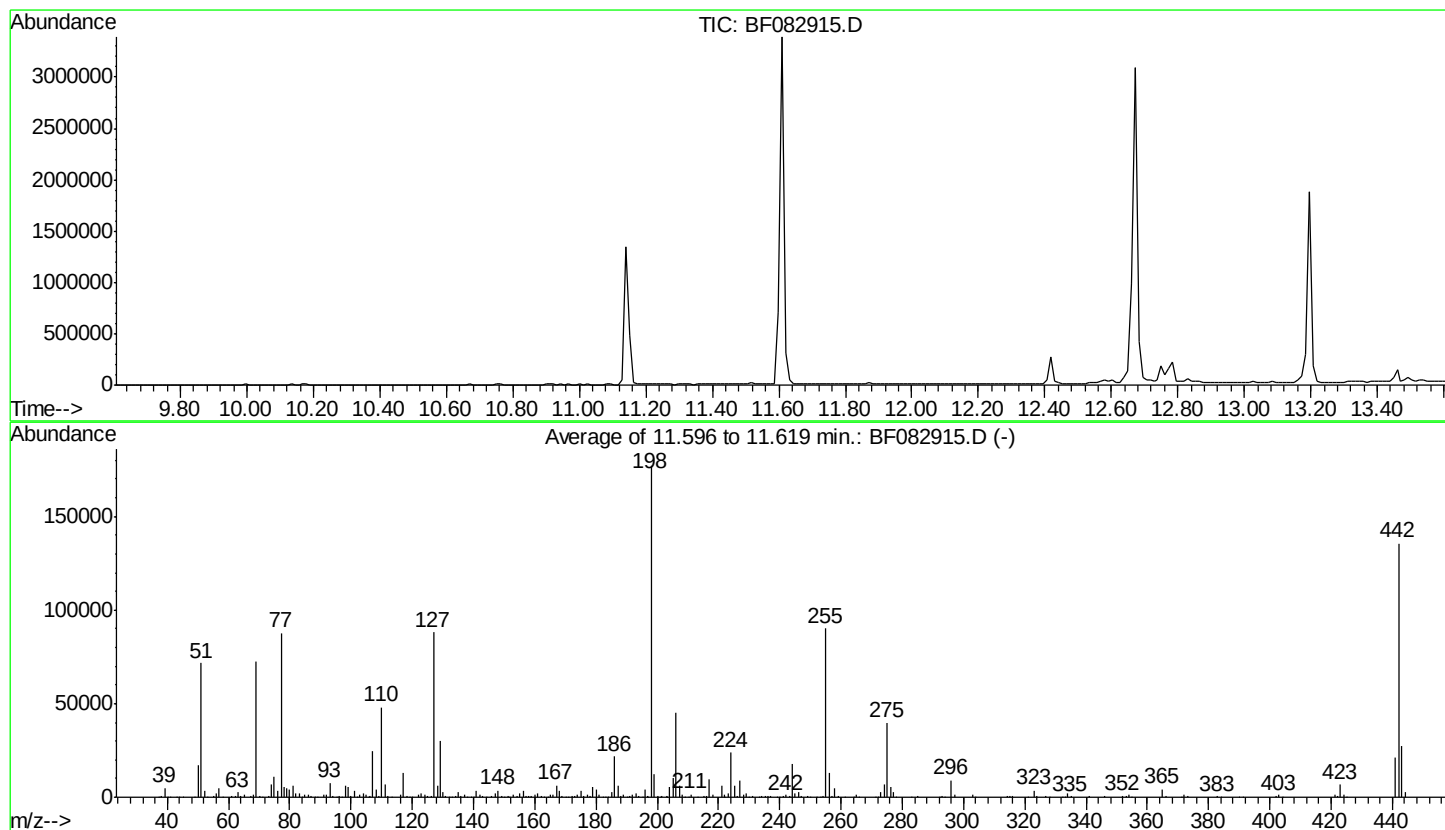

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	71761	PASS
68	69	0.00	2	1.6	1153	PASS
69	198	0.00	100	40.8	72186	PASS
70	69	0.00	2	0.6	444	PASS
127	198	10	80	49.7	88044	PASS
197	198	0.00	2	0.4	756	PASS
198	198	100	100	100.0	177106	PASS
199	198	5	9	6.9	12152	PASS
275	198	10	60	22.4	39742	PASS
365	198	1	100	2.4	4315	PASS
441	442	0.01	24	15.8	21376	PASS
442	198	50	100	76.5	135554	PASS
443	442	15	24	20.0	27176	PASS