

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111321\  
 Data File : BF126178.D  
 Acq On : 13 Nov 2021 20:24  
 Operator : JU/CG  
 Sample : M4654-04  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PARKINGLOT-TOP-U-SP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126178.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.040       | 498           | 502         | 512          | rVB      | 29026          | 38430         | 1.46%           | 0.234%        |
| 2         | 5.445       | 566           | 571         | 574          | rBV      | 3047309        | 2628113       | 100.00%         | 15.993%       |
| 3         | 6.457       | 738           | 743         | 746          | rBV      | 1980521        | 1777308       | 67.63%          | 10.816%       |
| 4         | 6.828       | 803           | 806         | 810          | rBV      | 596992         | 490299        | 18.66%          | 2.984%        |
| 5         | 7.392       | 897           | 902         | 905          | rBV      | 1332361        | 1168336       | 44.46%          | 7.110%        |
| 6         | 8.016       | 1005          | 1008        | 1021         | rBV      | 124068         | 132188        | 5.03%           | 0.804%        |
| 7         | 8.110       | 1021          | 1024        | 1028         | rBV      | 681312         | 615618        | 23.42%          | 3.746%        |
| 8         | 9.192       | 1203          | 1208        | 1211         | rBV      | 2880050        | 2277438       | 86.66%          | 13.859%       |
| 9         | 9.310       | 1224          | 1228        | 1231         | rVB      | 43175          | 37465         | 1.43%           | 0.228%        |
| 10        | 9.869       | 1319          | 1323        | 1326         | rBV      | 930835         | 736981        | 28.04%          | 4.485%        |
| 11        | 10.657      | 1453          | 1457        | 1460         | rBV      | 1502544        | 1379223       | 52.48%          | 8.393%        |
| 12        | 11.351      | 1572          | 1575        | 1578         | rBV      | 792551         | 668031        | 25.42%          | 4.065%        |
| 13        | 12.563      | 1779          | 1781        | 1785         | rVB      | 40494          | 34572         | 1.32%           | 0.210%        |
| 14        | 12.792      | 1812          | 1820        | 1823         | rBV2     | 34293          | 38982         | 1.48%           | 0.237%        |
| 15        | 12.939      | 1841          | 1845        | 1848         | rBV      | 2626093        | 2227788       | 84.77%          | 13.557%       |
| 16        | 13.857      | 1995          | 2001        | 2011         | rBV4     | 49131          | 115002        | 4.38%           | 0.700%        |
| 17        | 13.992      | 2017          | 2024        | 2027         | rBV      | 912082         | 791665        | 30.12%          | 4.818%        |
| 18        | 14.851      | 2167          | 2170        | 2175         | rBV      | 39832          | 41986         | 1.60%           | 0.256%        |
| 19        | 15.033      | 2196          | 2201        | 2203         | rBV4     | 25837          | 39612         | 1.51%           | 0.241%        |
| 20        | 15.115      | 2211          | 2215        | 2219         | rBV2     | 37320          | 45235         | 1.72%           | 0.275%        |
| 21        | 15.457      | 2267          | 2273        | 2277         | rBV      | 771419         | 893194        | 33.99%          | 5.435%        |
| 22        | 15.498      | 2277          | 2280        | 2285         | rVB4     | 38217          | 53522         | 2.04%           | 0.326%        |
| 23        | 15.933      | 2349          | 2354        | 2359         | rBV2     | 38627          | 57951         | 2.21%           | 0.353%        |
| 24        | 16.433      | 2434          | 2439        | 2446         | rBV2     | 32083          | 59441         | 2.26%           | 0.362%        |
| 25        | 17.027      | 2535          | 2540        | 2544         | rVB4     | 23810          | 44386         | 1.69%           | 0.270%        |
| 26        | 17.727      | 2654          | 2659        | 2664         | rVB7     | 18339          | 40027         | 1.52%           | 0.244%        |




Sum of corrected areas: 16432793

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111321\  
Data File : BF126178.D  
Acq On : 13 Nov 2021 20:24  
Operator : JU/CG  
Sample : M4654-04  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PARKINGLOT-TOP-U-SP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

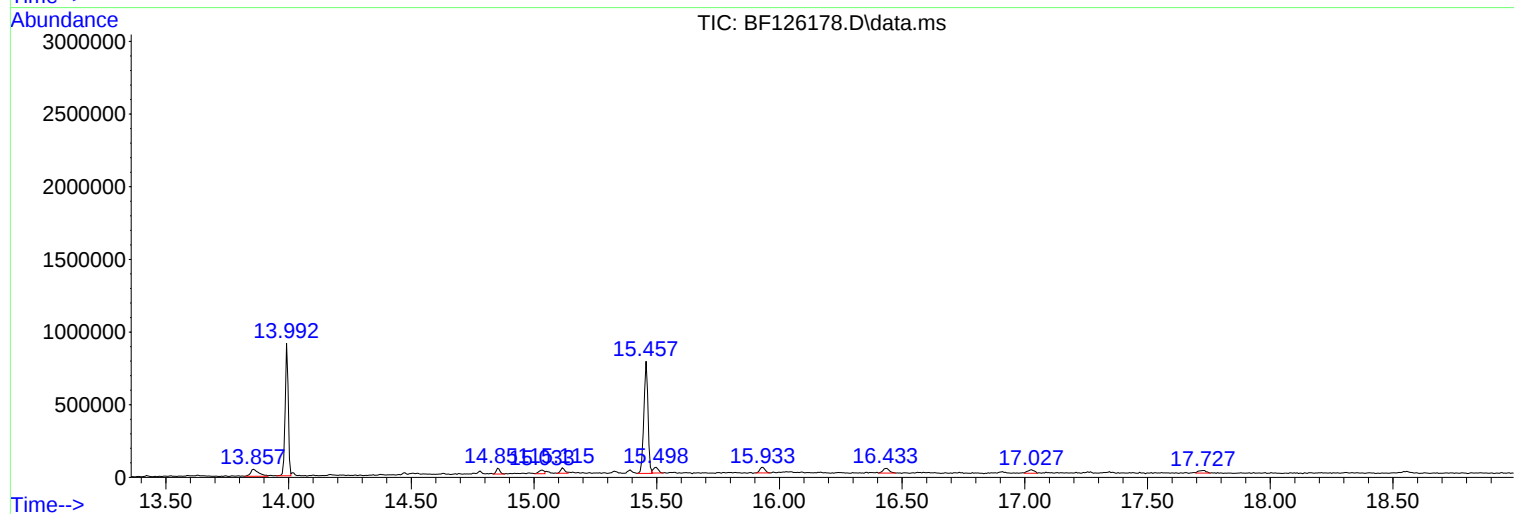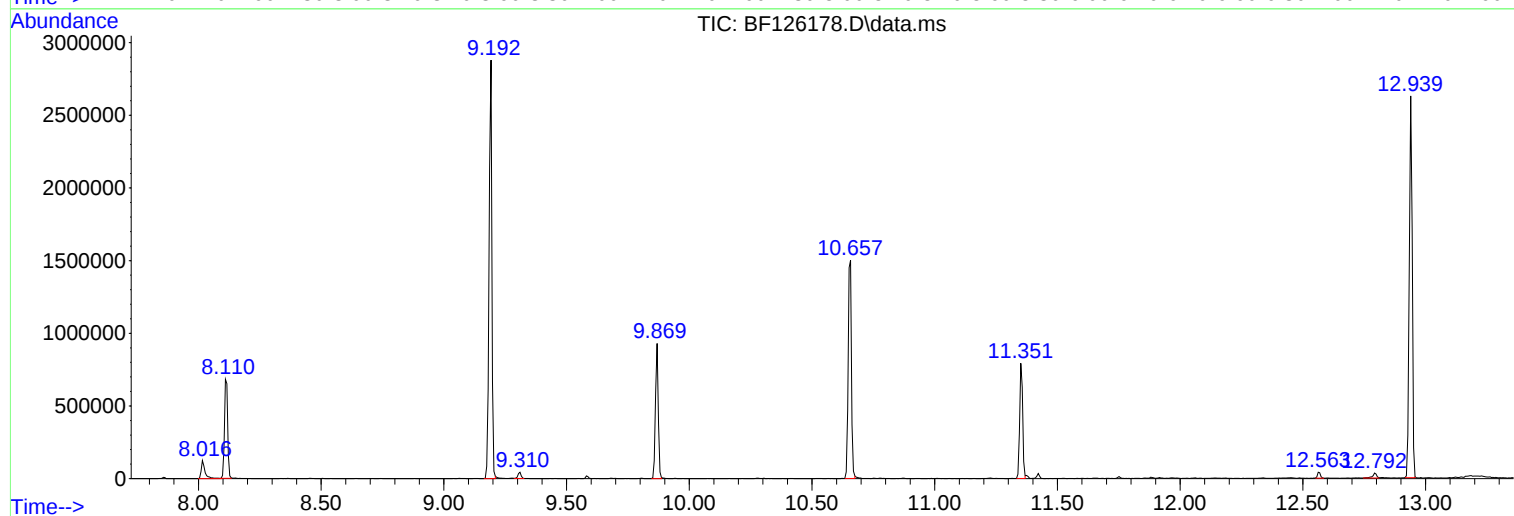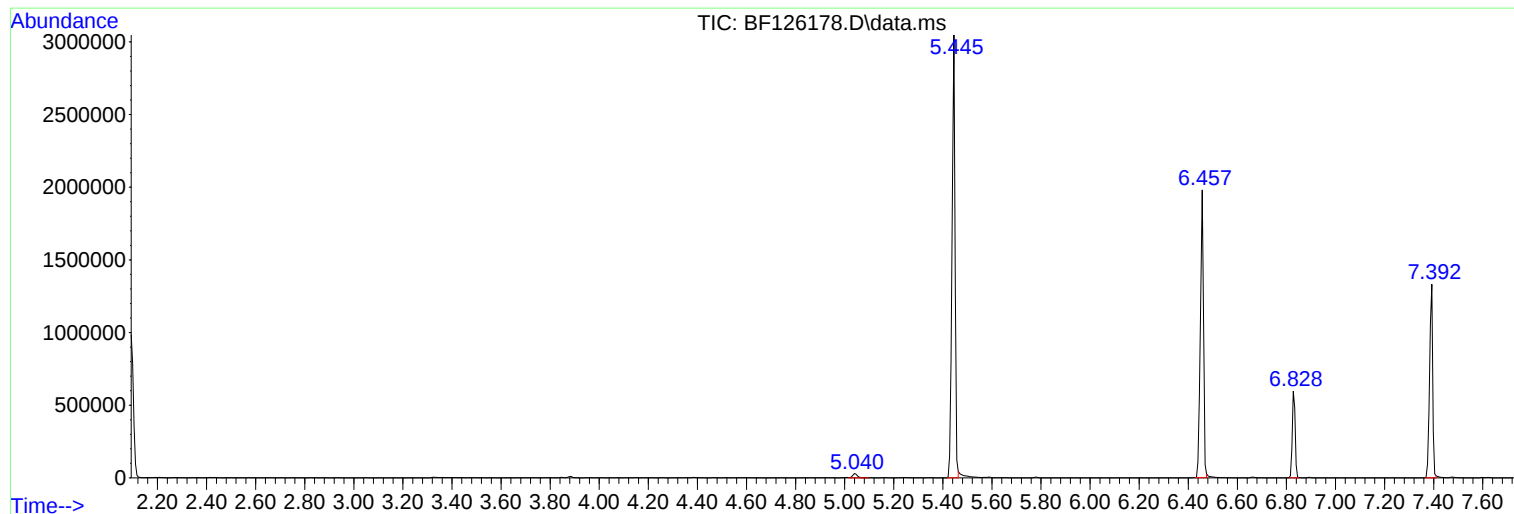

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111321\  
Data File : BF126178.D  
Acq On : 13 Nov 2021 20:24  
Operator : JU/CG  
Sample : M4654-04  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PARKINGLOT-TOP-U-SP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111321\  
Data File : BF126178.D  
Acq On : 13 Nov 2021 20:24  
Operator : JU/CG  
Sample : M4654-04  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PARKINGLOT-TOP-U-SP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |