


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111321\
 Data File : BF126165.D
 Acq On : 13 Nov 2021 11:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 14:29:48 2021

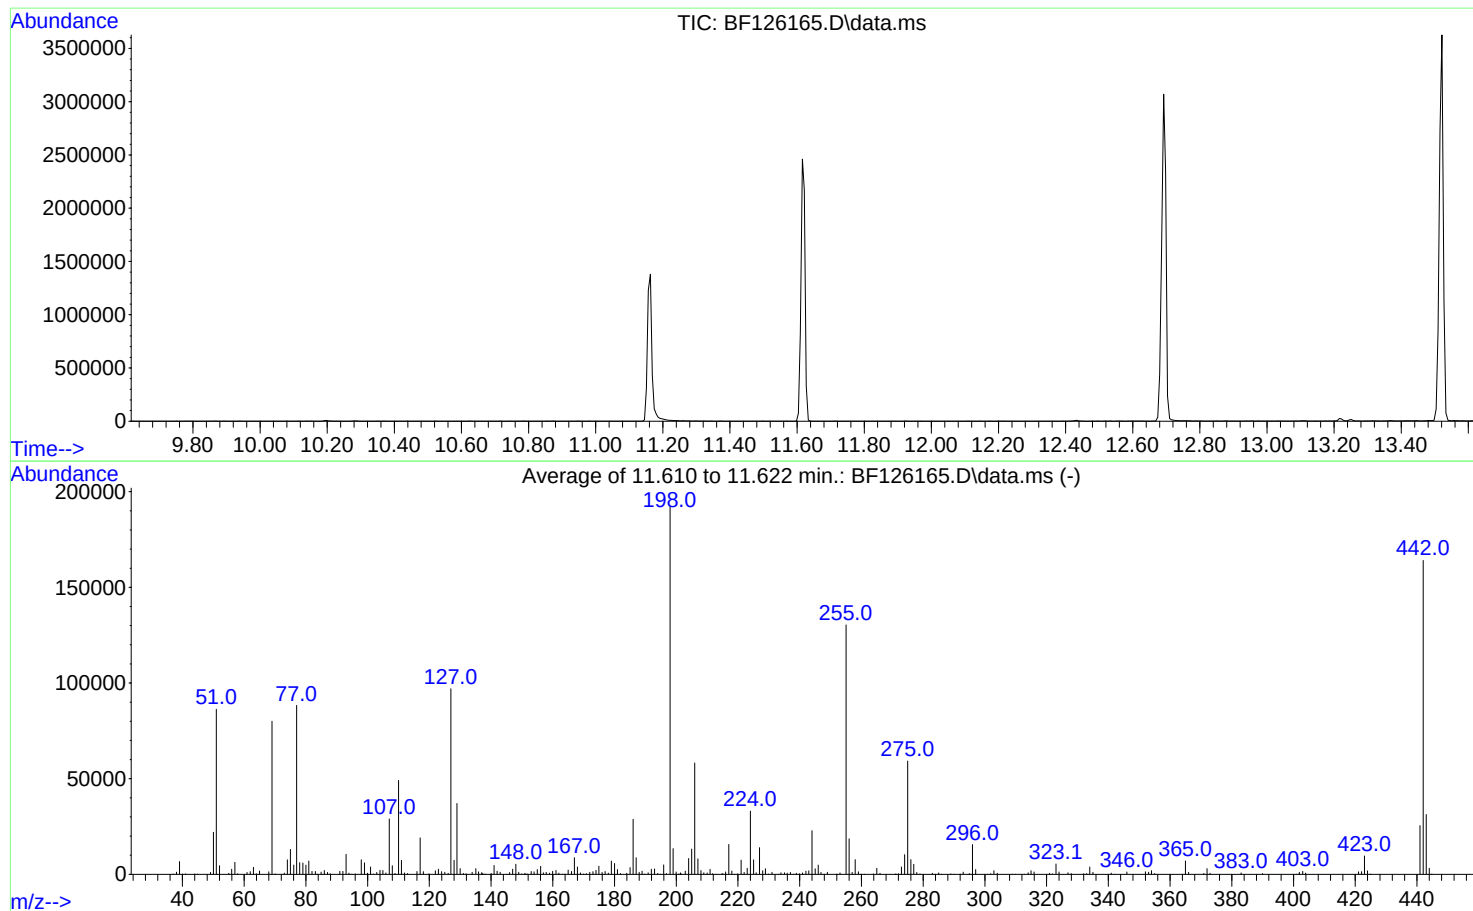

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	86339	PASS
68	69	0.00	2	1.7	1328	PASS
69	198	0.00	100	41.6	80048	PASS
70	69	0.00	2	0.4	284	PASS
127	198	10	80	50.5	97016	PASS
197	198	0.00	2	0.2	432	PASS
198	198	100	100	100.0	192264	PASS
199	198	5	9	7.0	13475	PASS
275	198	10	60	30.8	59171	PASS
365	198	1	100	3.6	7014	PASS
441	198	0.01	100	13.3	25502	PASS
442	442	50	100	100.0	164088	PASS
443	442	15	24	19.1	31299	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2021	BNA_F	<u>BF126165.D</u>
Compound Name	Response	Retention Time
DDT	592911	13.521
DDD	8544	13.216
DDE	181	12.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8725	601636	1.45

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111321\
Data File : BF126165.D
Acq On : 13 Nov 2021 11:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 22 04:30:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 14:29:48 2021
Response via : Initial Calibration

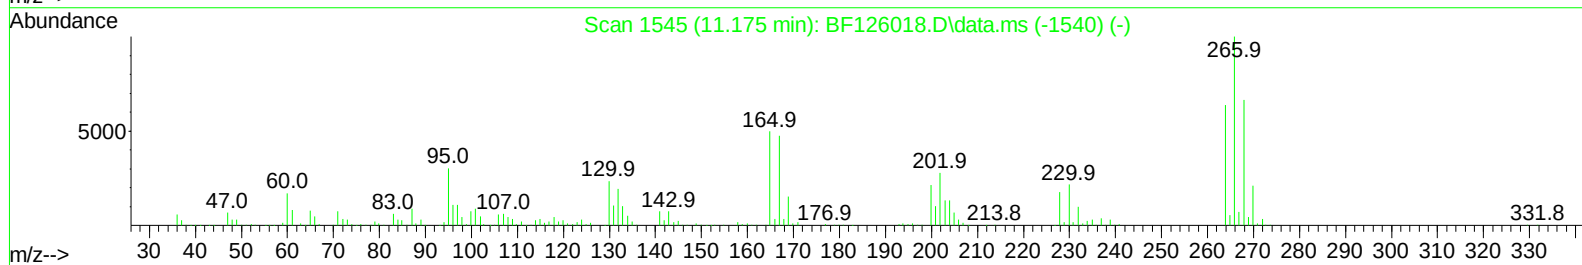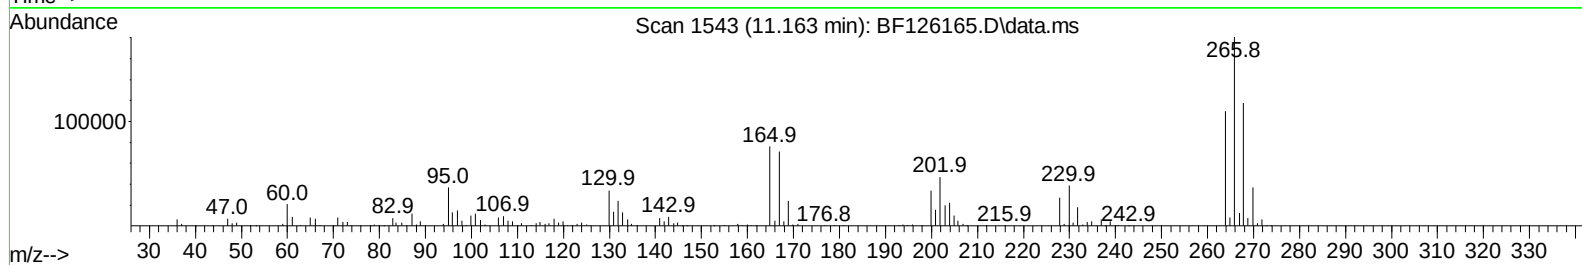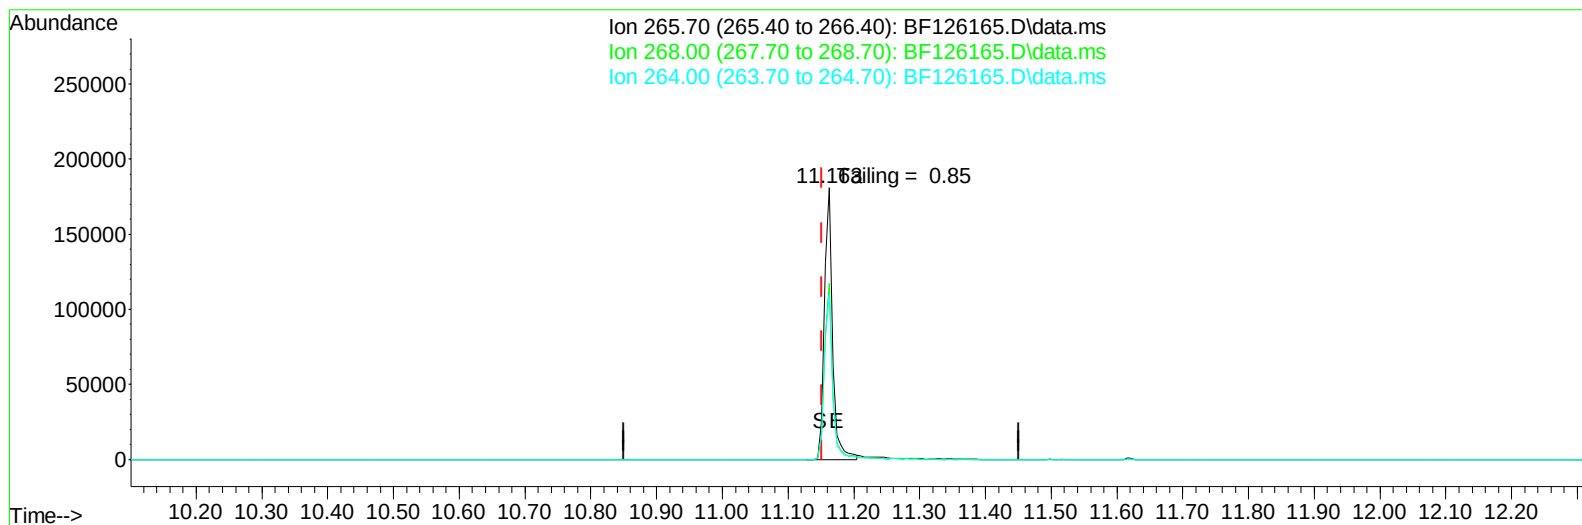

TIC: BF126165.D\data.ms

(70) Pentachlorophenol (C)

11.163min (+ 0.012) 21452.23 ng




response 162790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.04
264.00	69.90	60.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111321\
Data File : BF126165.D
Acq On : 13 Nov 2021 11:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 22 04:30:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 14:29:48 2021
Response via : Initial Calibration

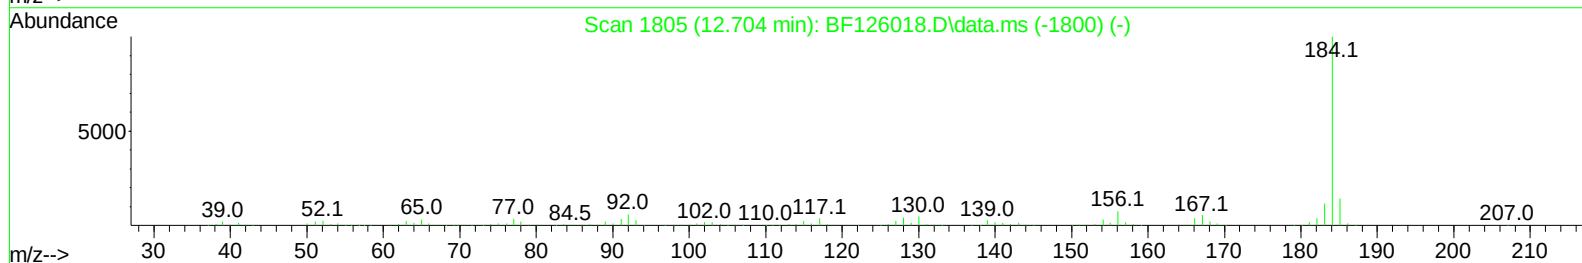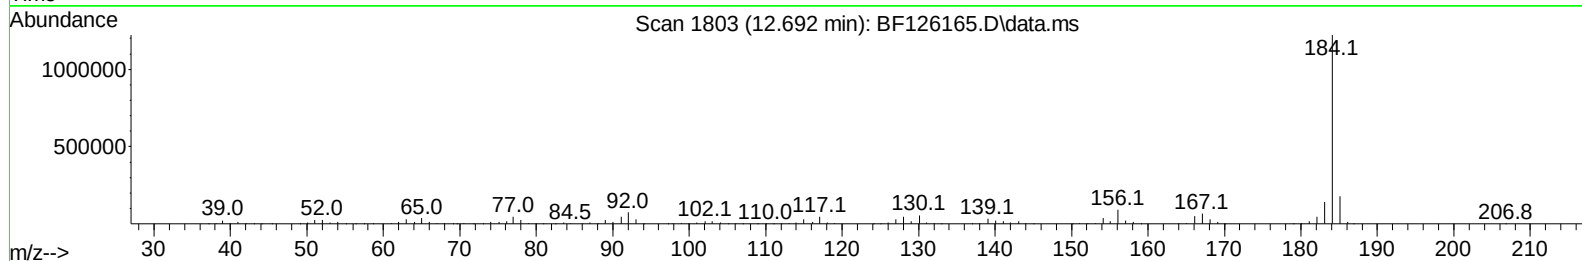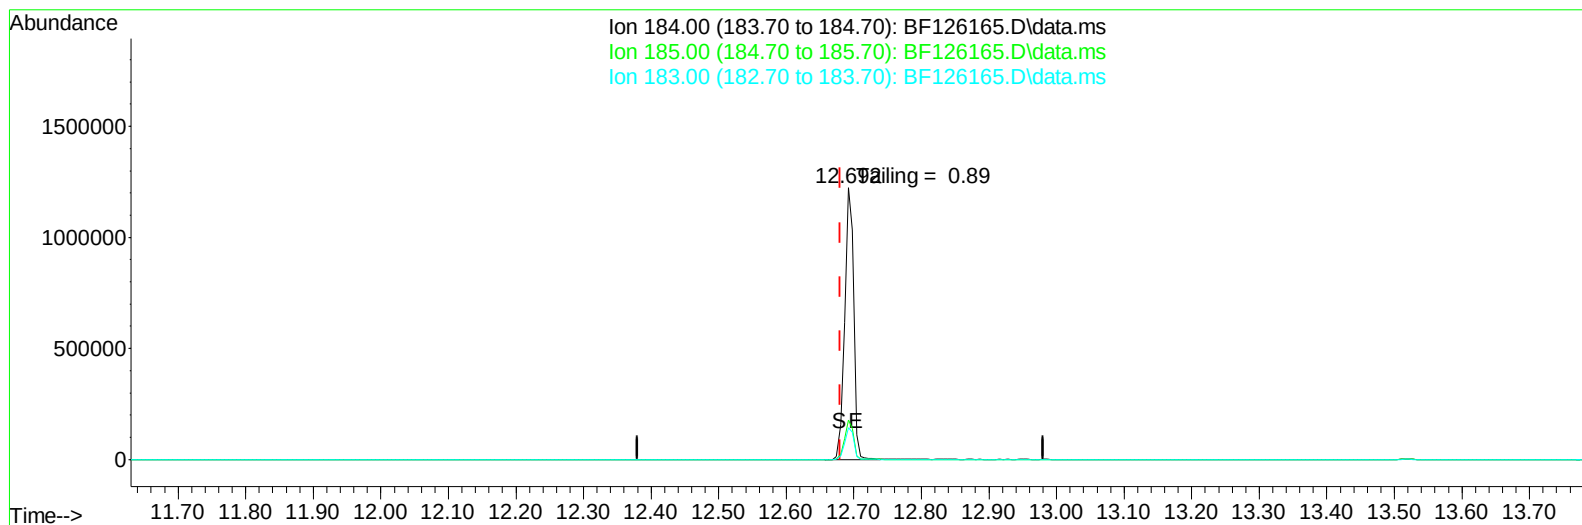

TIC: BF126165.D\data.ms

(77) Benzidine

12.692min (+ 0.012) 0.00 ng

response 1127105

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.55
183.00	10.10	11.64
0.00	0.00	0.00