

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
 Data File : BF075504.D
 Acq On : 14 Nov 2014 20:05
 Operator : TP / JJ
 Sample : PB80327TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB80327TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.624	44	47	50	rVB	6713677	7955183	100.00%	31.977%
2	1.830	63	65	74	rVV	330569	643856	8.09%	2.588%
3	1.967	74	77	84	rVV	773992	1166036	14.66%	4.687%
4	2.070	84	86	98	rVB	47652	121544	1.53%	0.489%
5	5.339	370	372	379	rBV	373737	460658	5.79%	1.852%
6	5.841	413	416	418	rBV	1282228	1332472	16.75%	5.356%
7	7.087	523	525	528	rBV	1064374	1268419	15.94%	5.099%
8	7.259	537	540	542	rVB	1419977	1321663	16.61%	5.313%
9	7.544	563	565	568	rBV	414632	522475	6.57%	2.100%
10	7.739	579	582	584	rBV	1063634	988355	12.42%	3.973%
11	8.242	623	626	628	rBV	829311	801794	10.08%	3.223%
12	9.133	701	704	706	rBV	784282	760126	9.56%	3.055%
13	10.470	819	821	824	rBV	1150046	1426347	17.93%	5.733%
14	11.316	892	895	897	rVB	626099	816130	10.26%	3.281%
15	12.288	978	980	983	rVB	824323	870408	10.94%	3.499%
16	13.156	1054	1056	1059	rBV	766822	823649	10.35%	3.311%
17	15.157	1228	1231	1233	rBV	1560141	1613005	20.28%	6.484%
18	16.460	1342	1345	1347	rBV	735446	963352	12.11%	3.872%
19	18.208	1495	1498	1501	rBV	818107	1022475	12.85%	4.110%


Sum of corrected areas: 24877947

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
Data File : BF075504.D
Acq On : 14 Nov 2014 20:05
Operator : TP / JJ
Sample : PB80327TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB80327TB

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

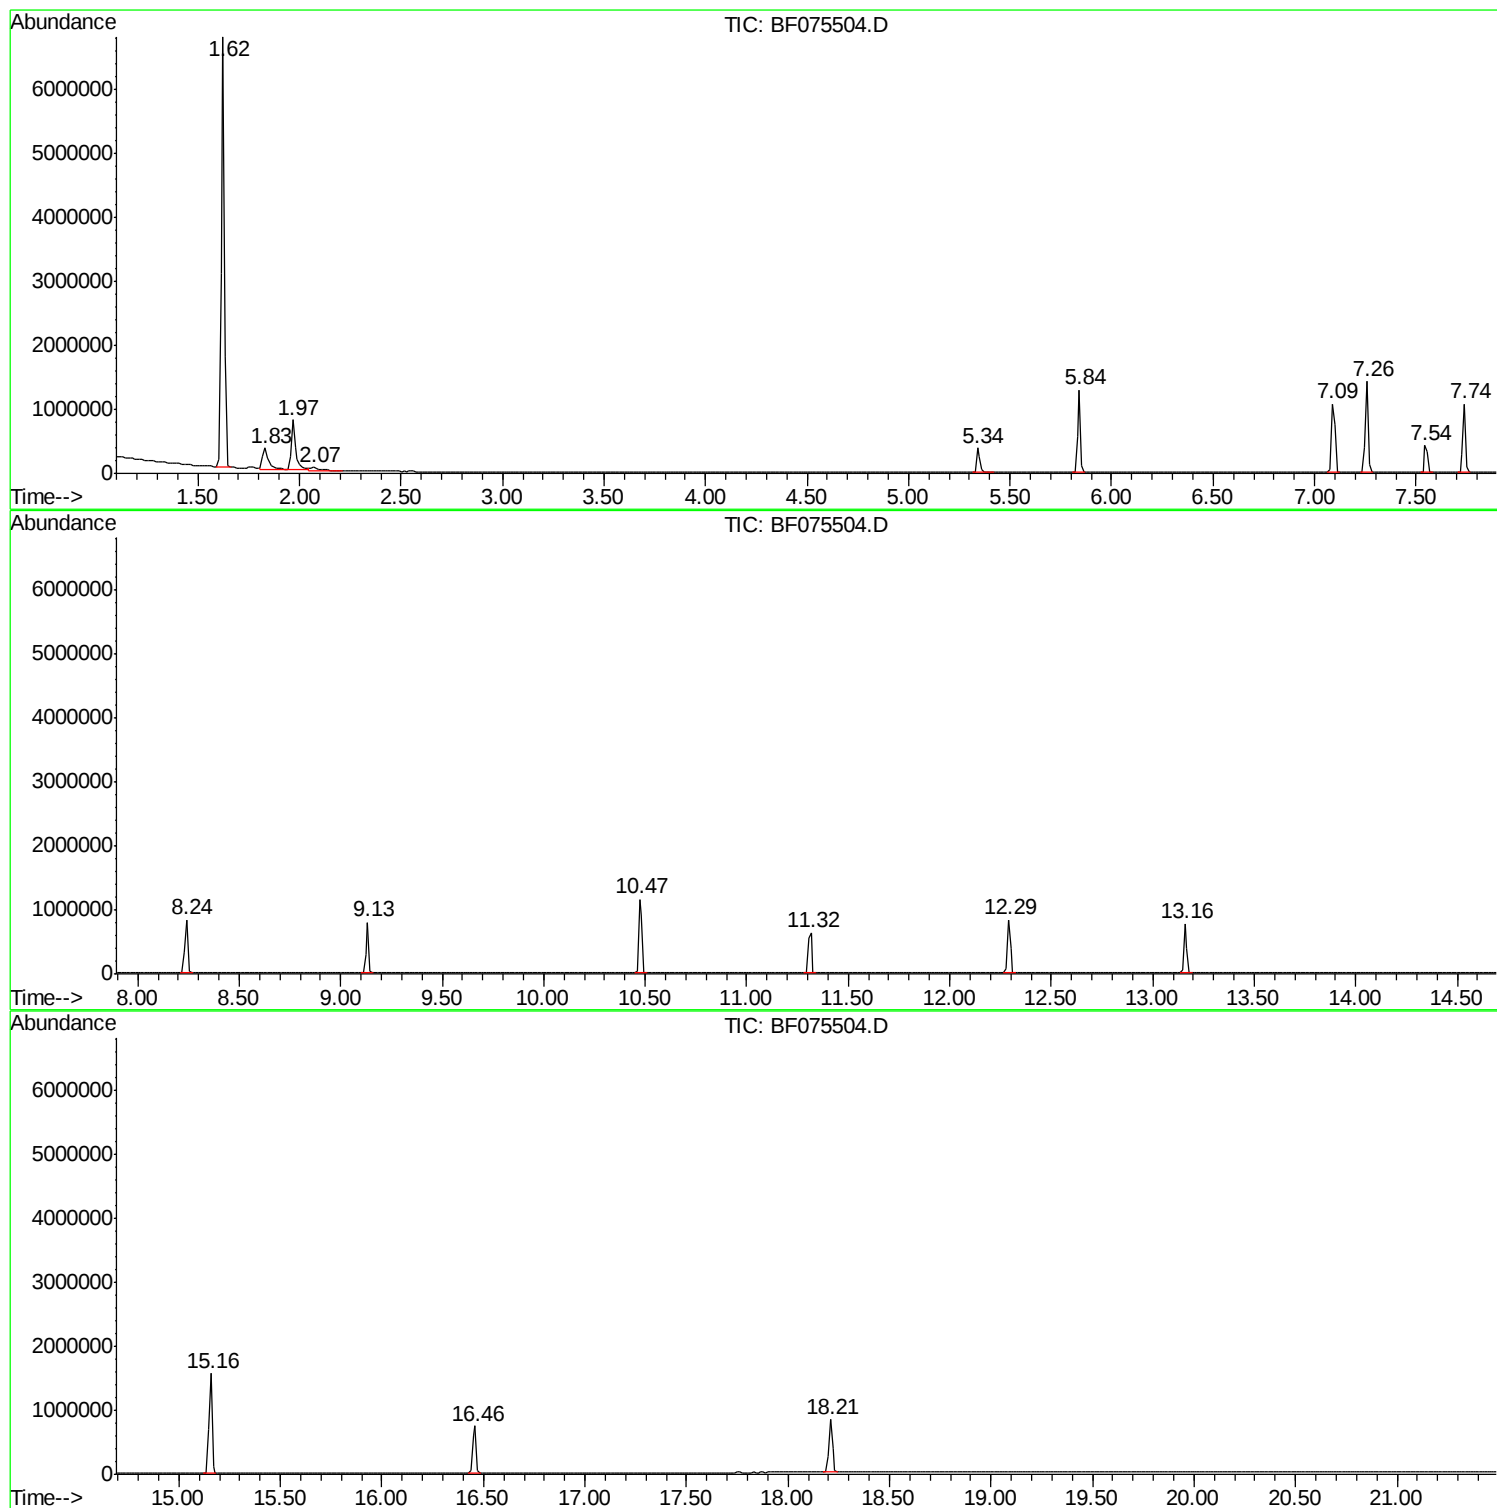

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
Data_File : BF075504.D
Acq_On : 14 Nov 2014 20:055
Operator : TP / JJJ
Sample : PB80327TBB
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB80327TB

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
