

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111414\
Data File : BF075541.D
Acq On : 15 Nov 2014 14:53
Operator : TP / JJ
Sample : F4614-01 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EFFWW

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.722	450	493	495	rBV	12678250	293224112	100.00%	98.966%
2	15.122	1225	1228	1230	rVV2	1760192	3062424	1.04%	1.034%




Sum of corrected areas: 296286536

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
Data File : BF075541.D
Acq On : 15 Nov 2014 14:53
Operator : TP / JJ
Sample : F4614-01 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EFFWW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

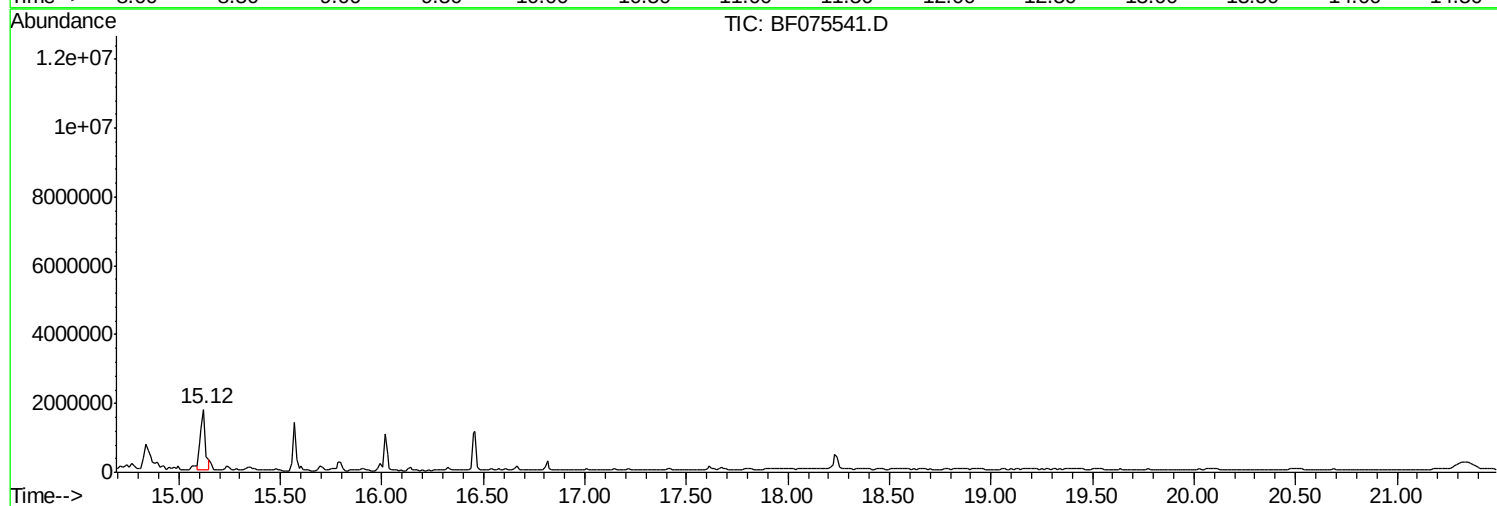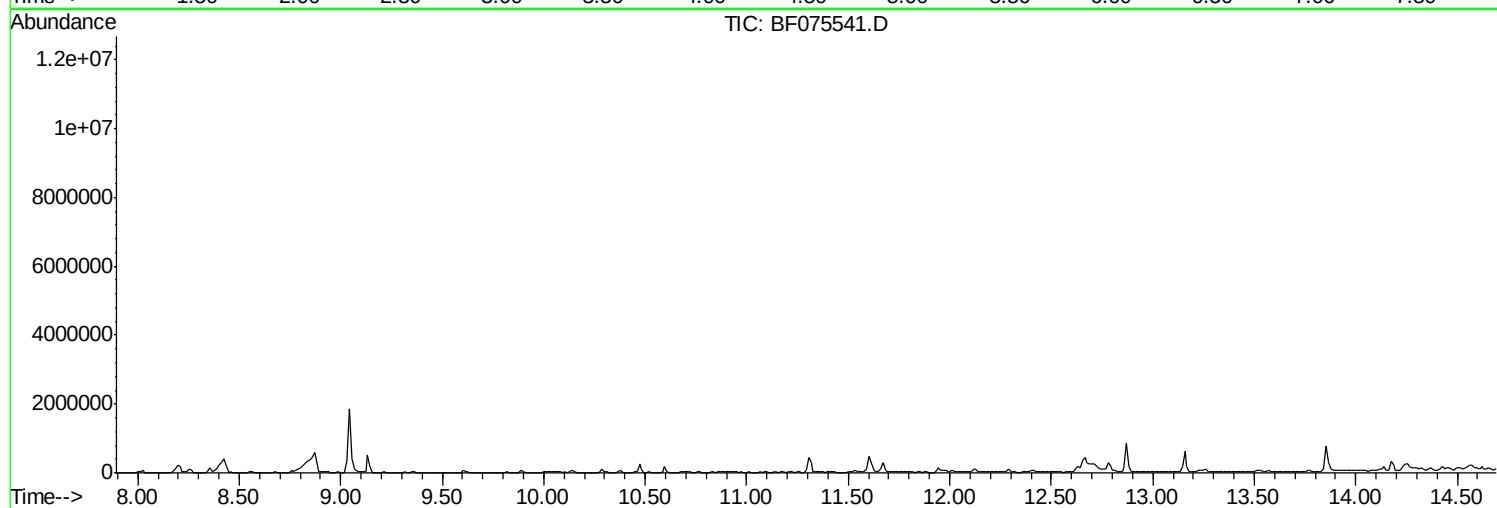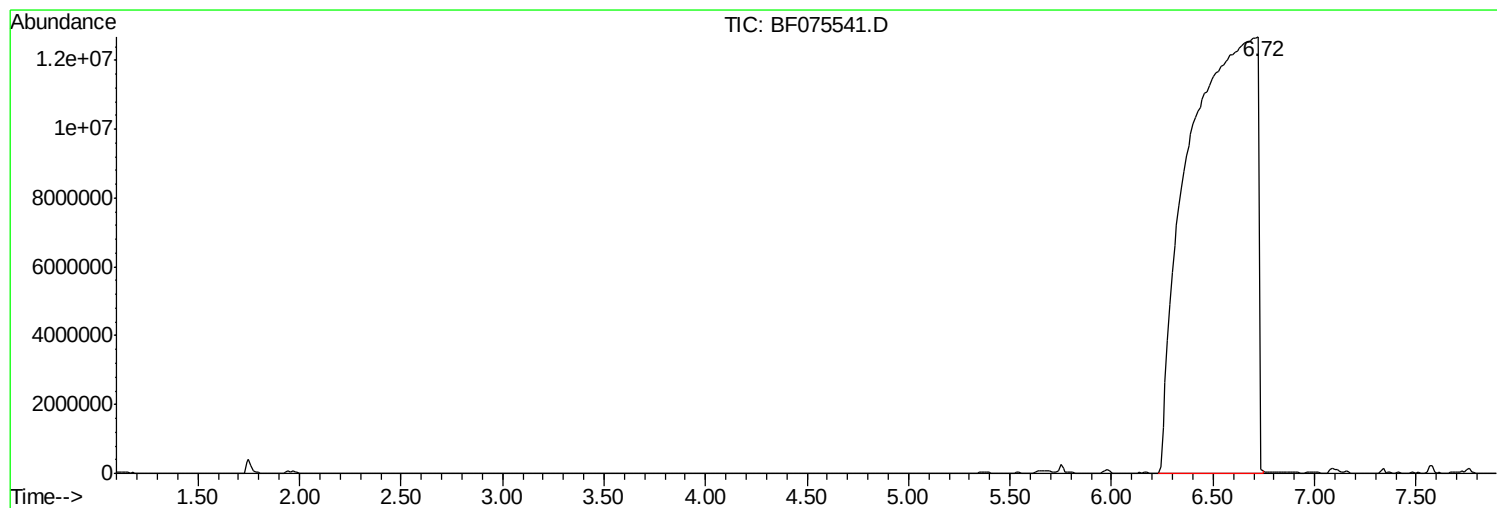

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
Data File : BF075541.D
Acq On : 15 Nov 2014 14:53
Operator : TP / JJ
Sample : F4614-01 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
EFFWW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-butoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.72	20.00 ng	293224000	1,4-Dichlorobenzene-d4	7.58
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1		Ethanol, 2-butoxy-	118 C6H14O2	000111-76-2 78
2		3,3-Dimethylbutane-2-ol	102 C6H14O	000464-07-3 64
3		Propane, 1-methoxy-2,2-dimethyl-	102 C6H14O	001118-00-9 64
4		Ethylene glycol monoisobutyl ether	118 C6H14O2	004439-24-1 36
5		1-Butene, 4-butoxy-	128 C8H16O	034061-76-2 32

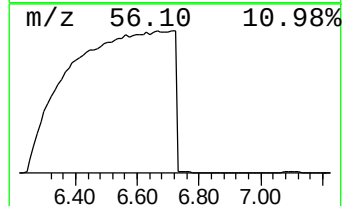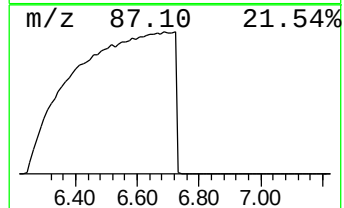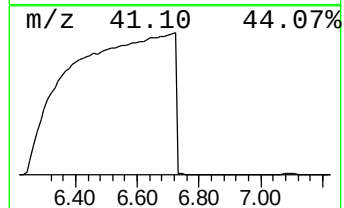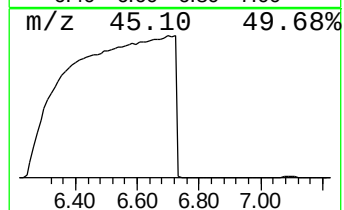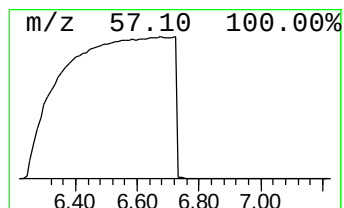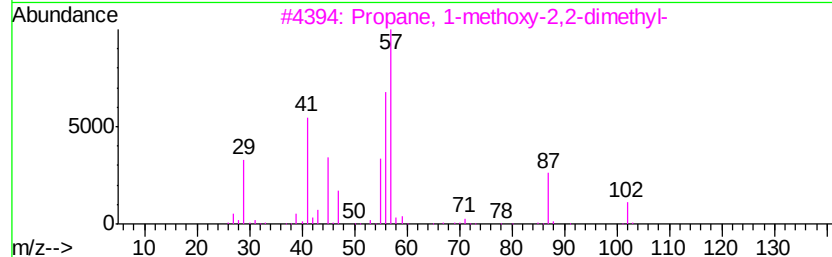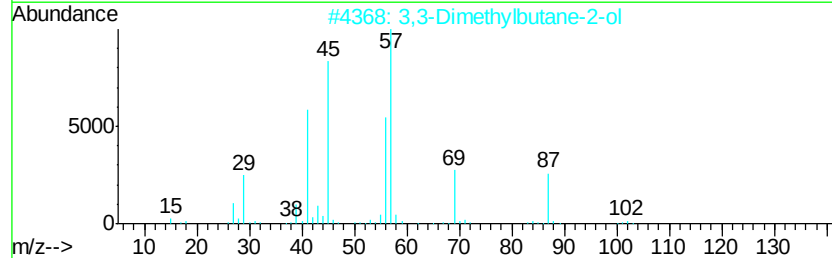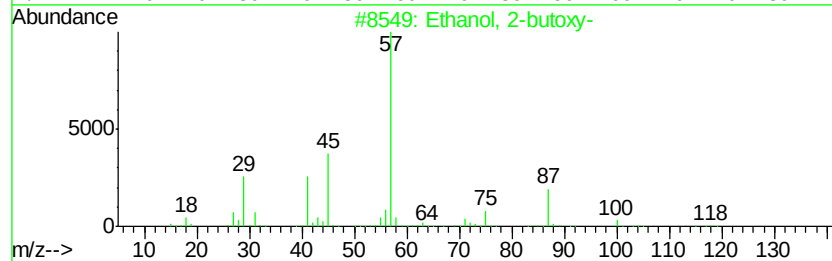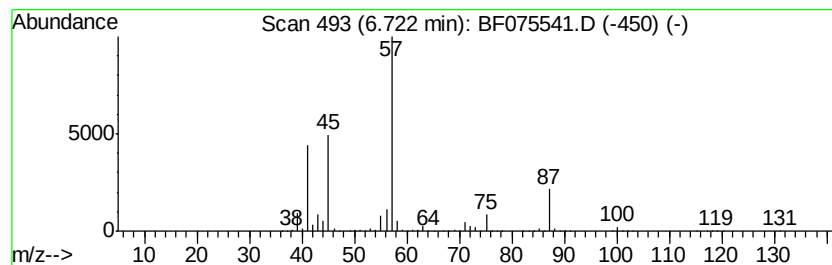

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
Data File : BF075541.D
Acq On : 15 Nov 2014 14:53
Operator : TP / JJ
Sample : F4614-01 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EFFWW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-butoxy-	6.72	20.0	ng	293224000	1	7.58	293224000	20.0