

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111414\
 Data File : BF075606.D
 Acq On : 17 Nov 2014 3:43
 Operator : TP / JJ
 Sample : F4695-01DL 2X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-75(5-7)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	43	46	48	rBV	682311	954130	17.73%	2.699%
2	1.761	56	59	62	rVB	47084	61340	1.14%	0.173%
3	1.967	73	77	84	rBV	210158	312897	5.81%	0.885%
4	5.350	370	373	377	rBV	104779	159278	2.96%	0.451%
5	5.853	415	417	419	rBV	289210	293547	5.46%	0.830%
6	7.110	525	527	529	rBV	268091	316151	5.88%	0.894%
7	7.270	538	541	543	rBV	240388	314555	5.85%	0.890%
8	7.339	545	547	549	rBV	111467	101427	1.88%	0.287%
9	7.556	564	566	568	rBV	170769	158851	2.95%	0.449%
10	7.625	570	572	574	rBV	74713	63605	1.18%	0.180%
11	7.739	580	582	584	rBV	248661	223496	4.15%	0.632%
12	7.899	594	596	598	rVB	115624	100710	1.87%	0.285%
13	7.956	598	601	603	rBV	189164	223141	4.15%	0.631%
14	8.036	607	608	611	rBV	56778	67823	1.26%	0.192%
15	8.128	614	616	618	rBV	131437	153500	2.85%	0.434%
16	8.162	618	619	621	rVB	149042	106422	1.98%	0.301%
17	8.219	621	624	625	rBV	323024	314009	5.84%	0.888%
18	8.242	625	626	630	rVB	220566	208703	3.88%	0.590%
19	8.356	634	636	638	rBV	54488	63398	1.18%	0.179%
20	8.402	638	640	641	rBV	99210	96336	1.79%	0.272%
21	8.505	647	649	651	rBV	360696	359194	6.68%	1.016%
22	8.539	651	652	654	rVB	629784	489591	9.10%	1.385%
23	8.653	660	662	663	rBV	85970	69393	1.29%	0.196%
24	8.688	663	665	666	rVB	50980	68530	1.27%	0.194%
25	8.722	666	668	670	rBV2	160794	244633	4.55%	0.692%
26	8.813	673	676	678	rBV2	390537	522960	9.72%	1.479%
27	8.859	678	680	682	rVV	221067	204589	3.80%	0.579%
28	8.905	682	684	689	rVV3	115539	207843	3.86%	0.588%
29	8.985	689	691	693	rVB	216141	185065	3.44%	0.523%
30	9.133	702	704	705	rVV	322479	309470	5.75%	0.875%
31	9.168	705	707	710	rVV2	574792	894620	16.63%	2.530%
32	9.259	713	715	717	rVB	117102	131876	2.45%	0.373%
33	9.465	732	733	736	rBV2	43610	70588	1.31%	0.200%
34	9.625	745	747	750	rVB	43488	62810	1.17%	0.178%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
 Data File : BF075606.D
 Acq On : 17 Nov 2014 3:43
 Operator : TP / JJ
 Sample : F4695-01DL 2X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-75(5-7)DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.842	764	766	767 rBV	83984	95369	1.77%	0.270%
36	9.888	767	770	773 rBV	60764	87909	1.63%	0.249%
37	10.025	779	782	783 rBV	172459	175447	3.26%	0.496%
38	10.139	790	792	795 rBV	81318	110842	2.06%	0.314%
39	10.242	797	801	802 rBV	87763	112894	2.10%	0.319%
40	10.265	802	803	805 rVV2	77223	105747	1.97%	0.299%
41	10.299	805	806	808 rVV	59723	82944	1.54%	0.235%
42	10.345	808	810	813 rVV	177263	203982	3.79%	0.577%
43	10.402	813	815	816 rVV	119803	172588	3.21%	0.488%
44	10.425	816	817	819 rVV	173623	190235	3.54%	0.538%
45	10.482	819	822	824 rVV	344180	401148	7.45%	1.135%
46	10.528	824	826	827 rVV	42766	67964	1.26%	0.192%
47	10.596	830	832	835 rVV	1357572	1481760	27.54%	4.191%
48	10.654	835	837	838 rVV	131700	196470	3.65%	0.556%
49	10.745	842	845	846 rVV2	69267	136082	2.53%	0.385%
50	10.791	846	849	851 rVV2	62029	142764	2.65%	0.404%
51	10.825	851	852	854 rVV	79611	120372	2.24%	0.340%
52	10.916	857	860	861 rVV	258238	394127	7.32%	1.115%
53	10.996	864	867	868 rVV2	429849	687237	12.77%	1.944%
54	11.019	868	869	872 rVV	306561	366788	6.82%	1.037%
55	11.076	872	874	875 rVB	168342	232948	4.33%	0.659%
56	11.214	883	886	888 rVB3	50598	110072	2.05%	0.311%
57	11.259	888	890	892 rVV	1719868	1637922	30.44%	4.633%
58	11.317	892	895	900 rVV2	384140	615890	11.45%	1.742%
59	11.397	900	902	903 rVV2	46871	69752	1.30%	0.197%
60	11.431	903	905	907 rVV2	48490	75123	1.40%	0.212%
61	11.477	907	909	911 rVB	71153	63212	1.17%	0.179%
62	11.545	911	915	917 rBV	188133	312474	5.81%	0.884%
63	11.579	917	918	920 rVV	144257	158085	2.94%	0.447%
64	11.625	920	922	923 rVV	111251	142789	2.65%	0.404%
65	11.659	923	925	927 rVB	298104	297081	5.52%	0.840%
66	11.705	927	929	934 rVB	161026	196699	3.66%	0.556%
67	11.819	936	939	941 rVB2	45971	75258	1.40%	0.213%
68	11.888	942	945	947 rVV	914011	908339	16.88%	2.569%
69	11.922	947	948	953 rVV2	66337	137604	2.56%	0.389%
70	12.002	953	955	960 rVB6	27523	84383	1.57%	0.239%
71	12.162	965	969	970 rBV	128758	211809	3.94%	0.599%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
 Data File : BF075606.D
 Acq On : 17 Nov 2014 3:43
 Operator : TP / JJ
 Sample : F4695-01DL 2X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-75(5-7)DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.219	972	974	976	rVB	76300	98694	1.83%	0.279%
73	12.265	976	978	979	rBV	50264	55442	1.03%	0.157%
74	12.299	979	981	984	rVB2	258163	281531	5.23%	0.796%
75	12.471	994	996	1001	rVB	188731	283589	5.27%	0.802%
76	13.168	1054	1057	1058	rBV	283294	269506	5.01%	0.762%
77	13.191	1058	1059	1062	rVB	71915	84226	1.57%	0.238%
78	13.705	1101	1104	1106	rBV	1461088	1778388	33.05%	5.030%
79	13.900	1119	1121	1123	rBV	152945	159963	2.97%	0.452%
80	14.563	1176	1179	1180	rBV	4620292	5381136	100.00%	15.220%
81	14.585	1180	1181	1185	rVV	3157337	4671479	86.81%	13.213%
82	14.688	1188	1190	1193	rVB	720015	914427	16.99%	2.586%
83	14.963	1211	1214	1216	rBV	158422	176059	3.27%	0.498%
84	15.157	1229	1231	1234	rVB	303456	368495	6.85%	1.042%
85	15.420	1253	1254	1257	rBV3	28648	57044	1.06%	0.161%
86	15.500	1257	1261	1267	rVB4	74043	149045	2.77%	0.422%
87	15.603	1267	1270	1271	rBV	77303	105788	1.97%	0.299%
88	15.626	1271	1272	1275	rVV2	74877	124908	2.32%	0.353%
89	15.683	1275	1277	1281	rVV2	64878	110005	2.04%	0.311%
90	15.786	1284	1286	1289	rVV2	37909	78144	1.45%	0.221%
91	15.866	1291	1293	1296	rVB3	42349	69963	1.30%	0.198%
92	16.128	1313	1316	1320	rVB3	78549	142984	2.66%	0.404%
93	16.460	1342	1345	1350	rBV3	294192	625307	11.62%	1.769%
94	17.751	1455	1458	1464	rBV	65451	157505	2.93%	0.445%
95	18.083	1484	1487	1489	rBV	44740	59523	1.11%	0.168%
96	18.151	1490	1493	1496	rVB	42594	68325	1.27%	0.193%
97	18.220	1496	1499	1501	rBV	221913	306898	5.70%	0.868%


Sum of corrected areas: 35354964

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
Data File : BF075606.D
Acq On : 17 Nov 2014 3:43
Operator : TP / JJ
Sample : F4695-01DL 2X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-75(5-7)DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

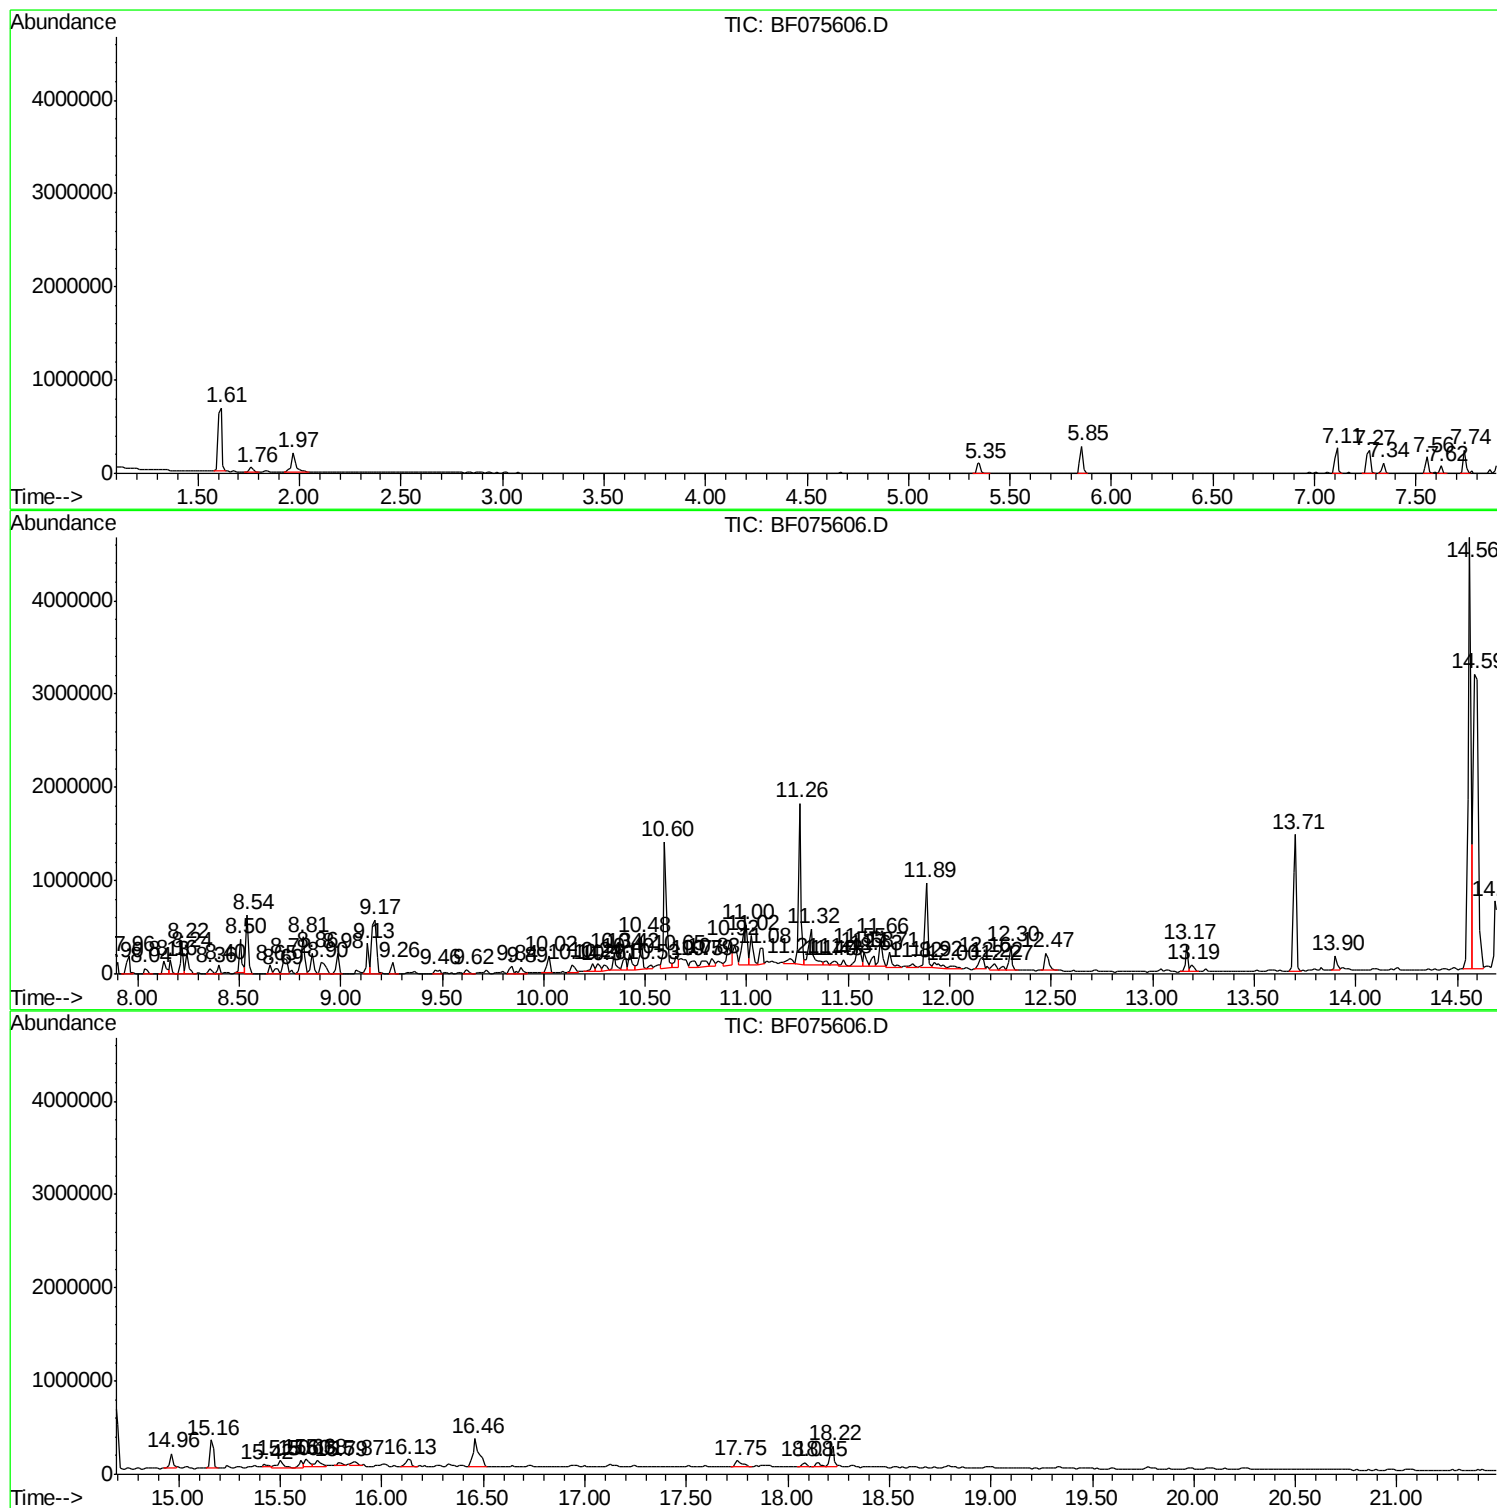

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF111414\
Data_File : BE075606.D
Acq_On : 17 Nov 2014 3:433
Operator : TP / JJJ
Sample : F4695-01DL_2XX
Misc :
ALS_Vial : 33 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-75(5-7)DL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
