


Data Path : Z:\HPCHEM1\BNA F\Data\BF111414\
 Data File : BF075497.D
 Acq On : 14 Nov 2014 16:29
 Operator : TP / JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 12 18:46:55 2014

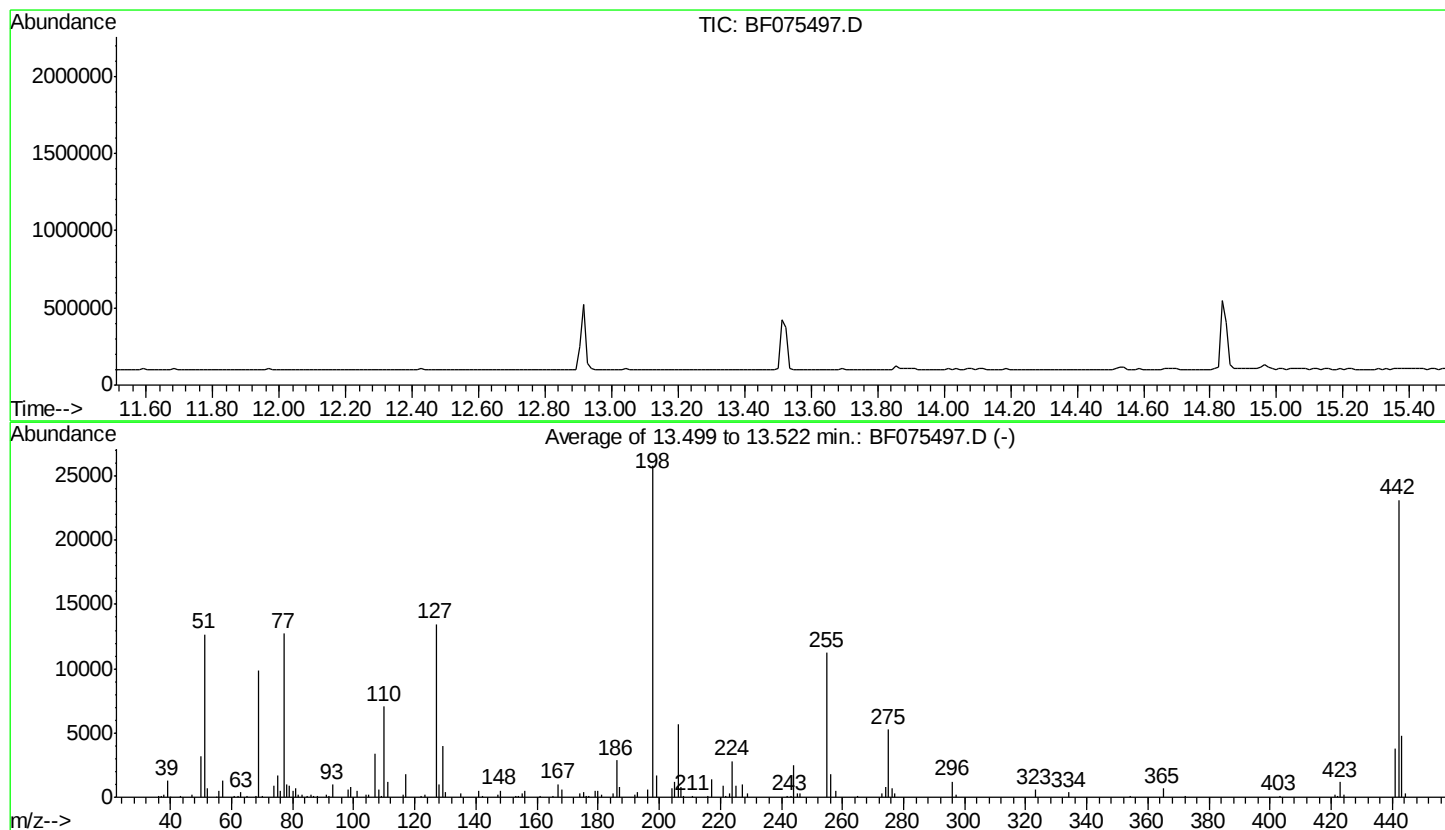

AutoFind: Scans 1086, 1087, 1088; Background Corrected with Scan 1083

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	12696	PASS
68	69	0.00	2	1.4	142	PASS
69	198	0.00	100	38.2	9859	PASS
70	69	0.00	2	1.1	111	PASS
127	198	10	80	52.3	13494	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25804	PASS
199	198	5	9	6.7	1740	PASS
275	198	10	60	20.4	5272	PASS
365	198	1	100	2.6	676	PASS
441	442	0.01	24	16.2	3747	PASS
442	198	50	100	89.6	23110	PASS
443	442	15	24	20.8	4796	PASS