


Data Path : Z:\HPCHEM1\BNA F\Data\BF111414\
 Data File : BF075521.D
 Acq On : 15 Nov 2014 4:34
 Operator : TP / JJ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 12 18:46:55 2014

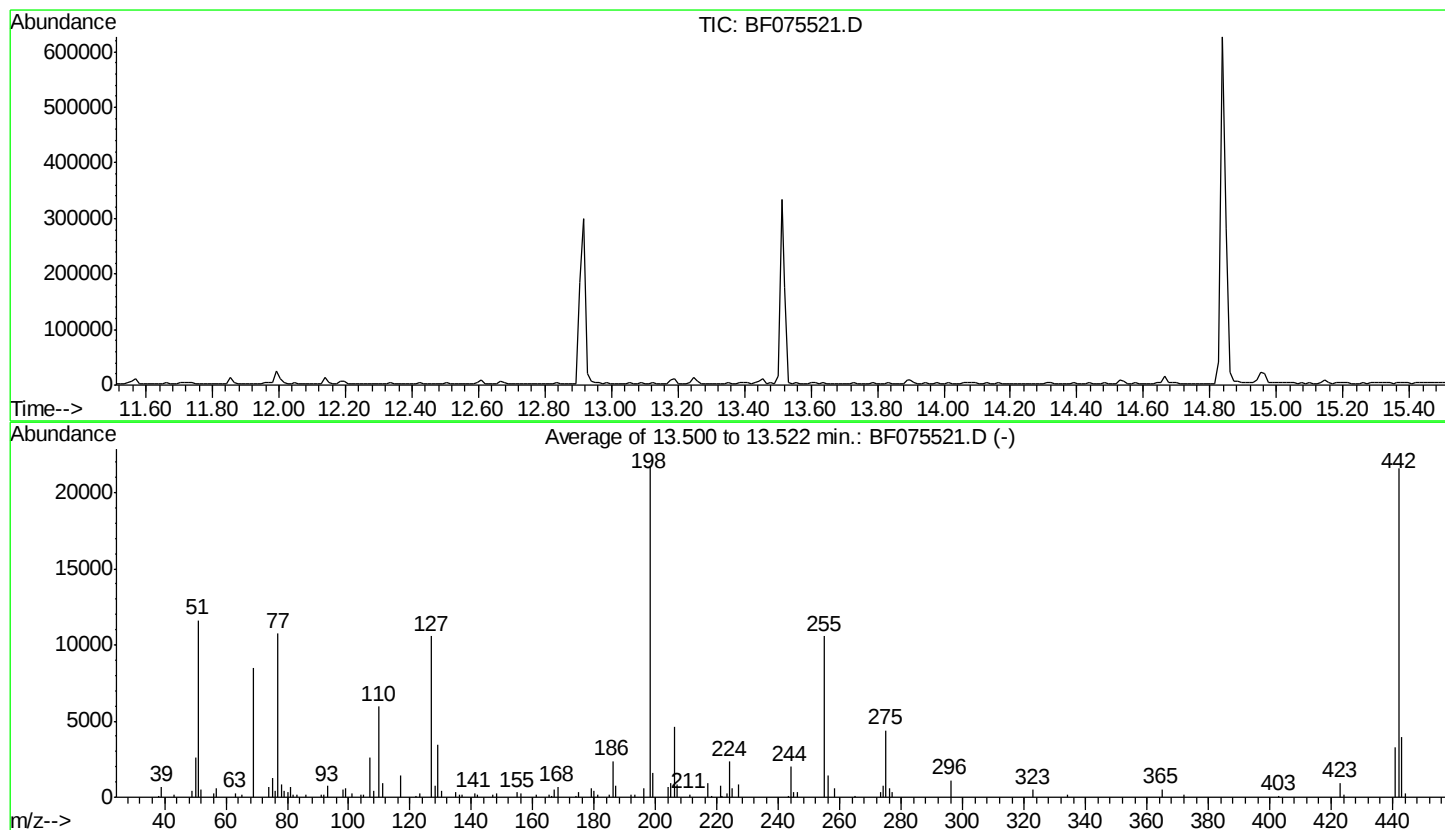

AutoFind: Scans 1086, 1087, 1088; Background Corrected with Scan 1083

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	11638	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.8	8451	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	10559	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21767	PASS
199	198	5	9	7.4	1606	PASS
275	198	10	60	20.3	4412	PASS
365	198	1	100	2.3	508	PASS
441	442	0.01	24	15.1	3257	PASS
442	198	50	100	99.1	21563	PASS
443	442	15	24	18.1	3910	PASS