


Data Path : Z:\HPCHEM1\BNA_F\Data\BF111414\
 Data File : BF075546.D
 Acq On : 15 Nov 2014 17:14
 Operator : TP / JJ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111214.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 12 18:46:55 2014

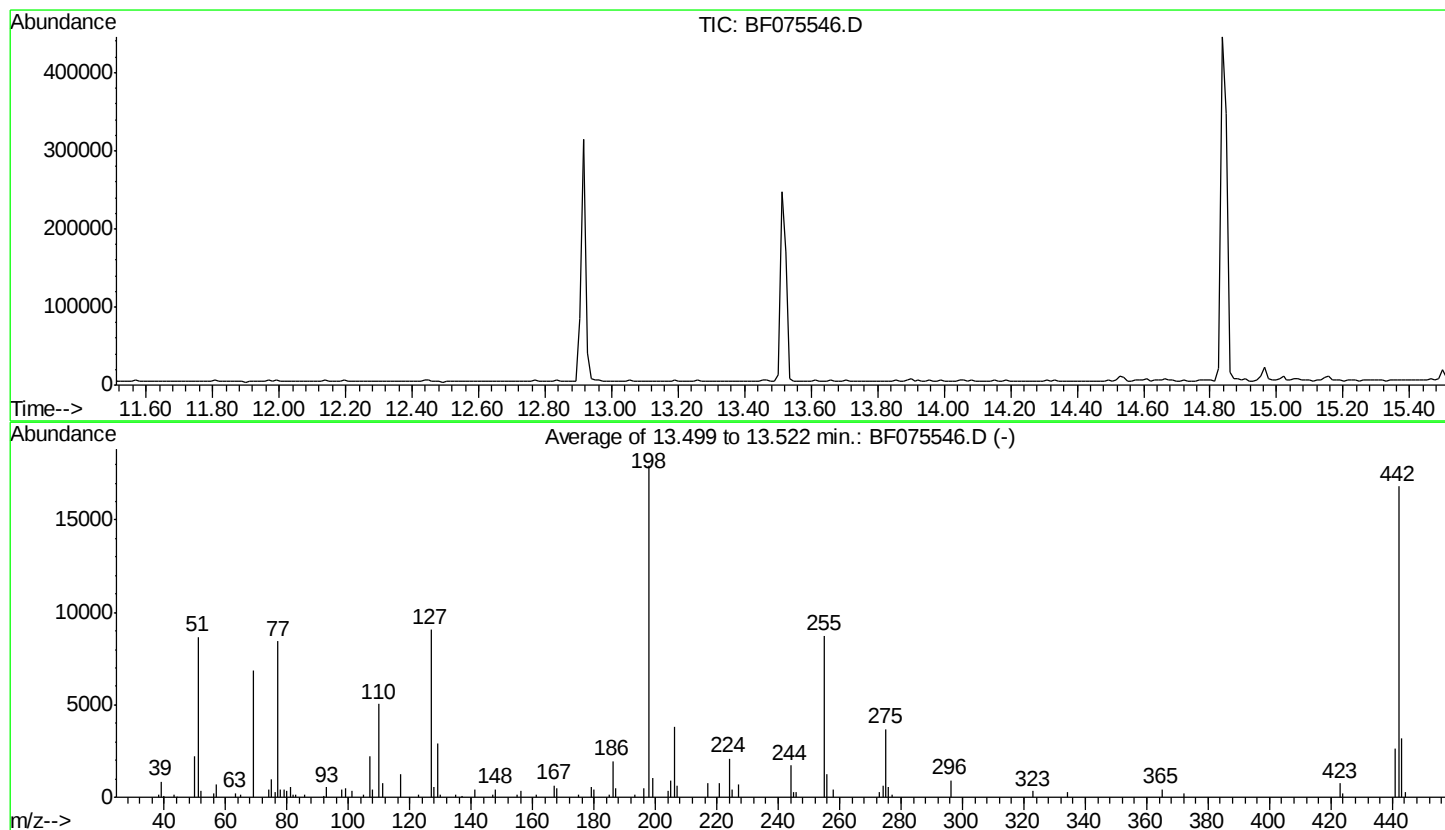

AutoFind: Scans 1086, 1087, 1088; Background Corrected with Scan 1083

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	8663	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.1	6836	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	9055	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17940	PASS
199	198	5	9	6.0	1069	PASS
275	198	10	60	20.5	3673	PASS
365	198	1	100	2.3	418	PASS
441	442	0.01	24	15.8	2650	PASS
442	198	50	100	93.7	16811	PASS
443	442	15	24	18.9	3174	PASS