
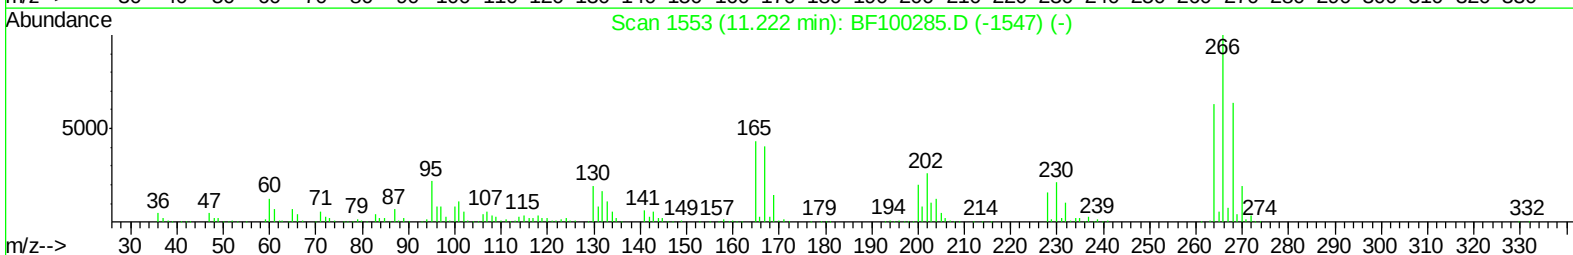
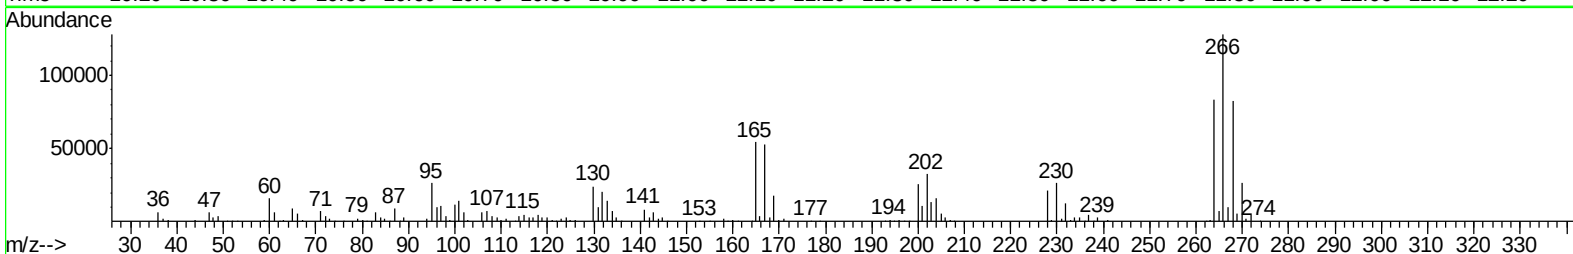


Data File : BF100536.D
Acq On : 14 Nov 2017 11:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 07:49:12 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 14 14:17:16 2017
Response via : Initial Calibration

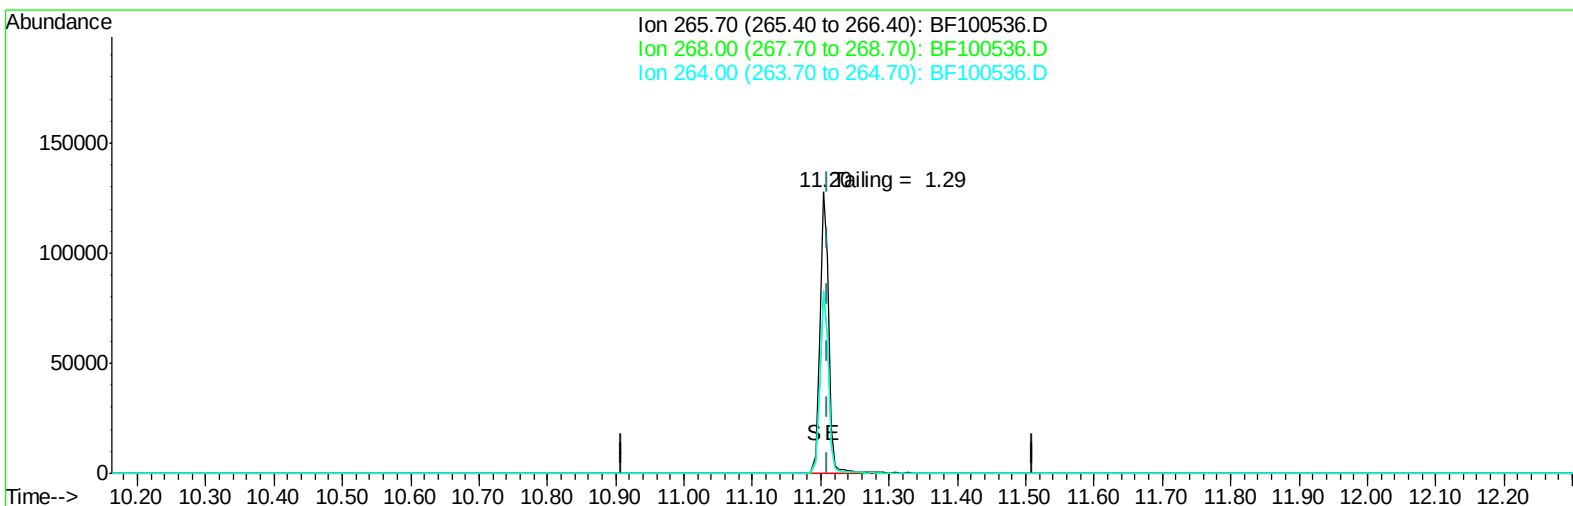

TIC: BF100536.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 135484.35ng

response 116546

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.62
264.00	61.90	64.93
0.00	0.00	0.00

Data File : BF100536.D
Acq On : 14 Nov 2017 11:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 07:49:12 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 14 14:17:16 2017
Response via : Initial Calibration

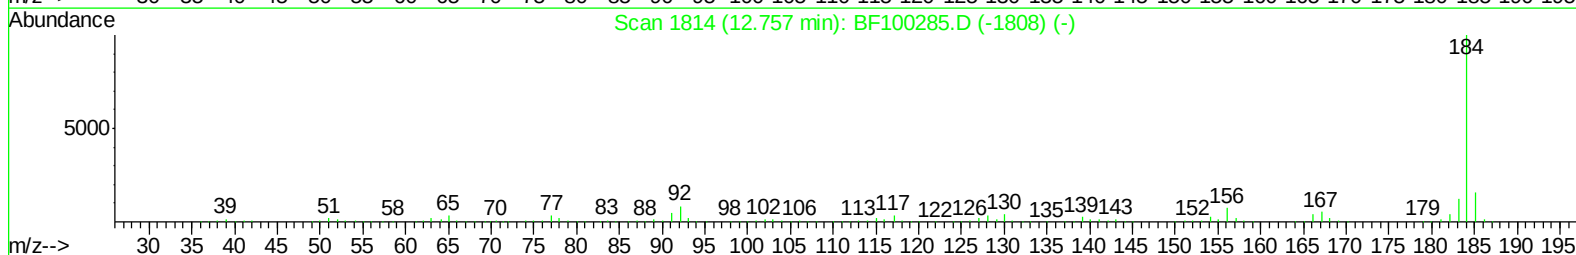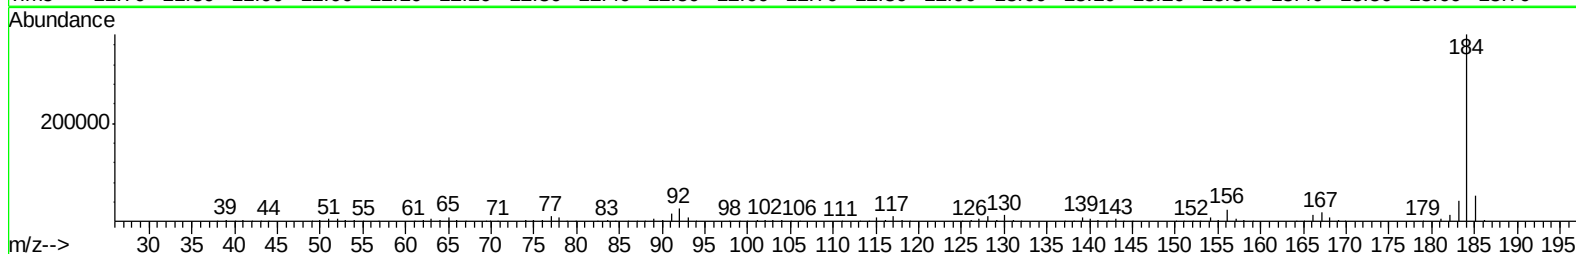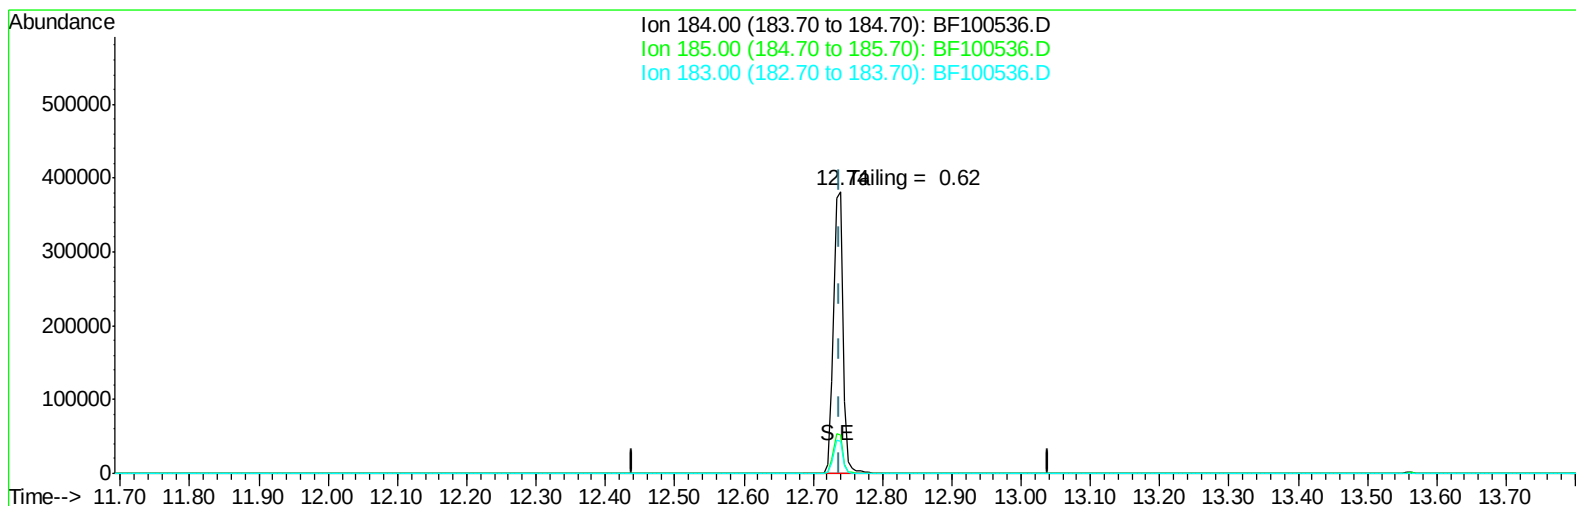

TIC: BF100536.D

(76) Benzidine

12.739min (-0.000) 0.00ng

response 361856

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.75
183.00	11.60	11.33
0.00	0.00	0.00