

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111417\
 Data File : BF100544.D
 Acq On : 14 Nov 2017 15:58
 Operator : SJ/JU
 Sample : I6301-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-02-110917-A

Manual Integrations
 APPROVED

SOHIL
 11/15/2017 12:30:06 PM

Quant Time: Nov 14 16:33:13 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 14 14:17:16 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	134294	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	495554	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	195715	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	312255	20.00	ng	0.00
75) Chrysene-d12	14.04	240	267568	20.00	ng	0.00
86) Perylene-d12	15.52	264	192967	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	780931	93.22	ng	0.01
7) Phenol-d6	6.51	99	955565	92.50	ng	0.00
23) Nitrobenzene-d5	7.45	82	580805	77.49	ng	0.00
41) 2,4,6-Tribromophenol	10.71	330	173415	86.95	ng	0.00
44) 2-Fluorobiphenyl	9.24	172	887576	69.06	ng	0.00
78) Terphenyl-d14	12.99	244	626069	53.76	ng	0.00
Target Compounds						
10) Phenol	6.52	94	41756	3.850	ng	96
49) Dimethylphthalate	9.63	163	168000	11.243	ng	98
74) Fluoranthene	12.62	202	81117	4.655	ng	98
77) Pyrene	12.85	202	75229	3.944	ng	99
80) Benzo(a)anthracene	14.03	228	47908	2.973	ng	93
82) Chrysene	14.07	228	44497	2.852	ng	96
87) Benzo(b)fluoranthene	15.09	252	46470m	4.065	ng	
89) Benzo(a)pyrene	15.46	252	32012	3.159	ng	# 89
91) Benzo(g,h,i)perylene	17.45	276	17345	2.138	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF111417\
Data File : BF100544.D
Acq On : 14 Nov 2017 15:58
Operator : SJ/JU
Sample : I6301-01
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
JC-02-110917-A

Manual Integrations
APPROVED

SOHIL
11/15/2017 12:30:06 PM

Quant Time: Nov 14 16:33:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 14 14:17:16 2017
Response via : Initial Calibration

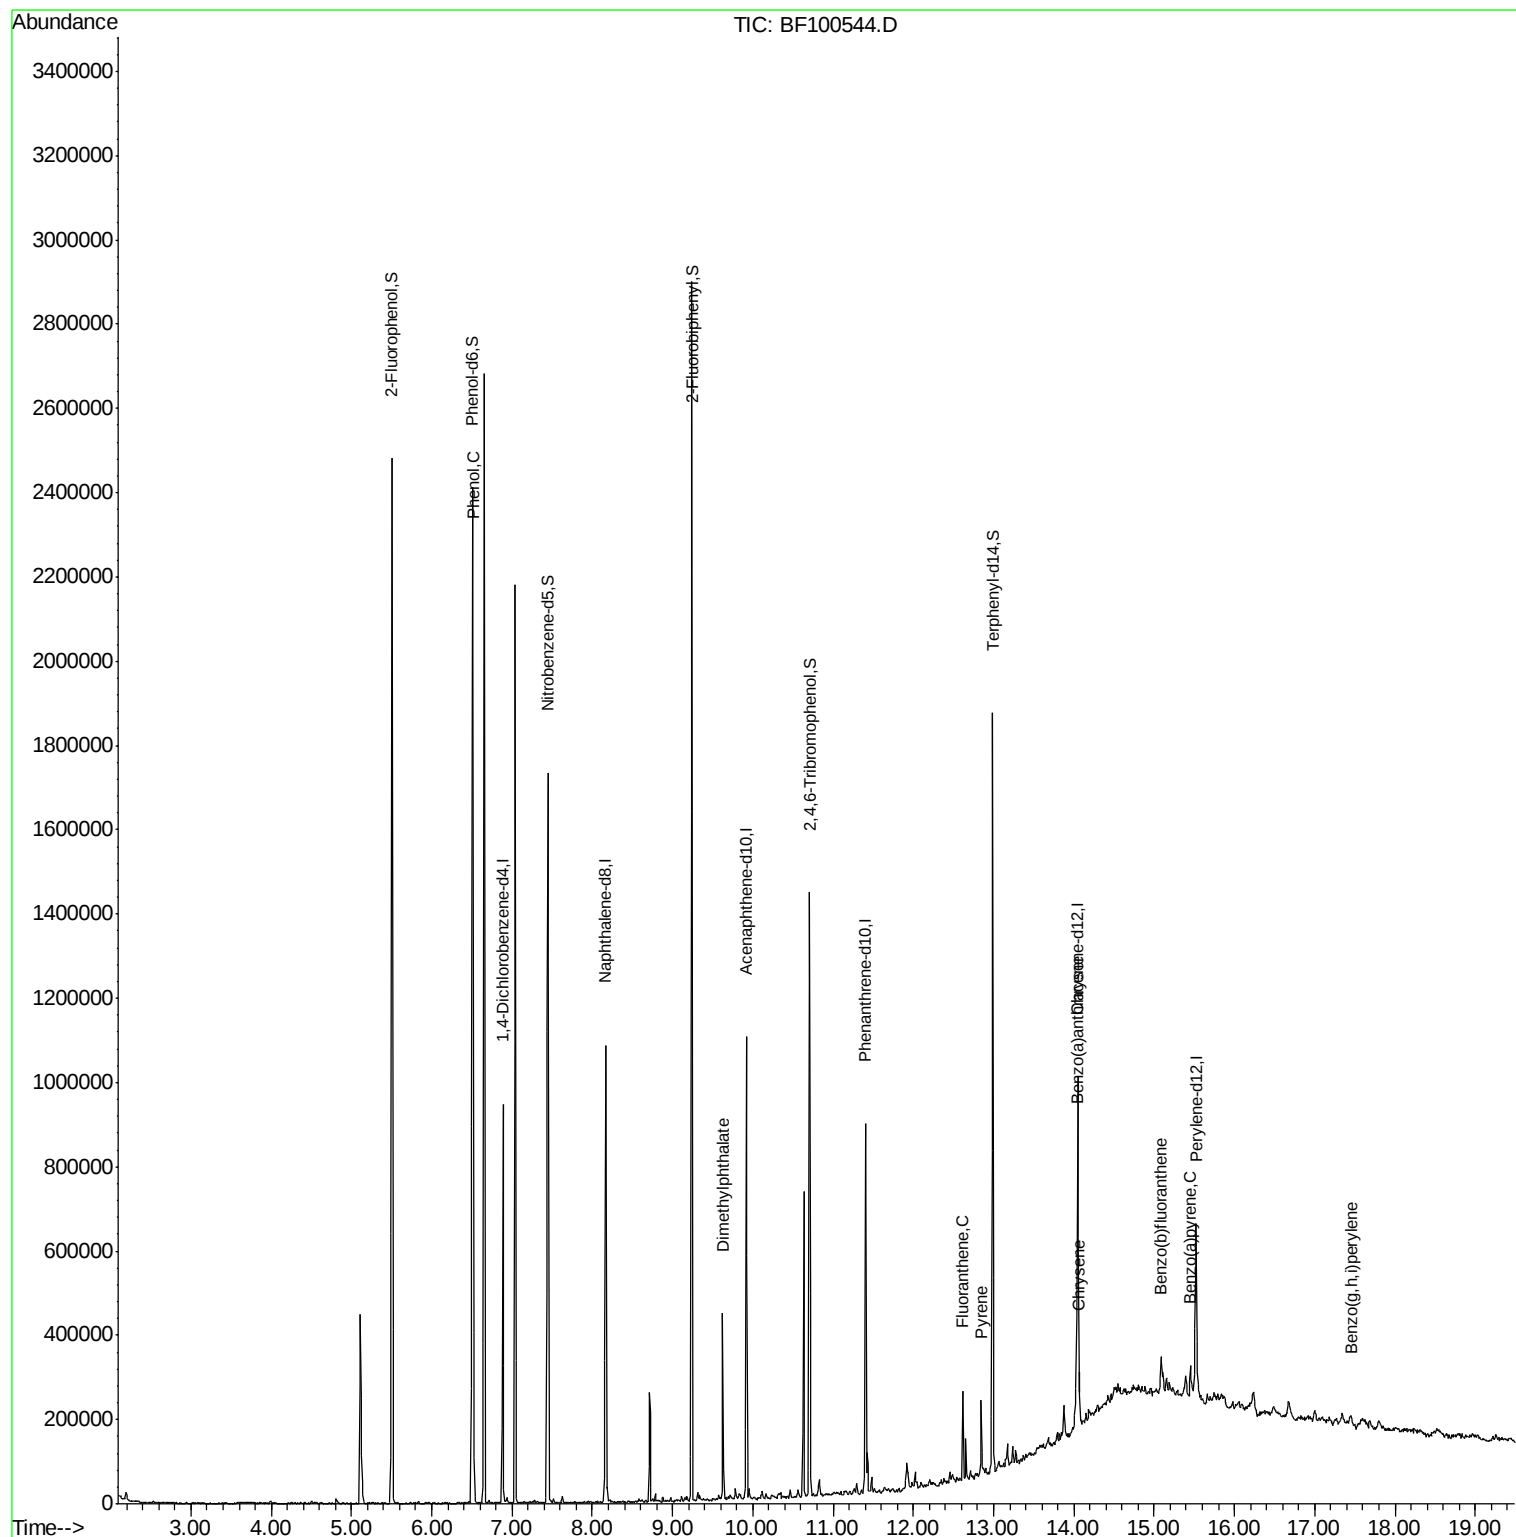



#1





1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.89 min Scan# 816
Delta R.T. 0.00 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Instrument :
BNA_F
ClientSampleId :
JC-02-110917-A

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.6	124.6	186.8
115	57.4	50.1	75.1

Manual Integrations
APPROVED




SOHIL
11/15/2017 12:30:06 PM

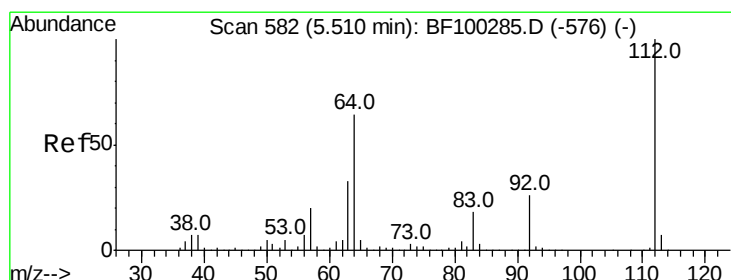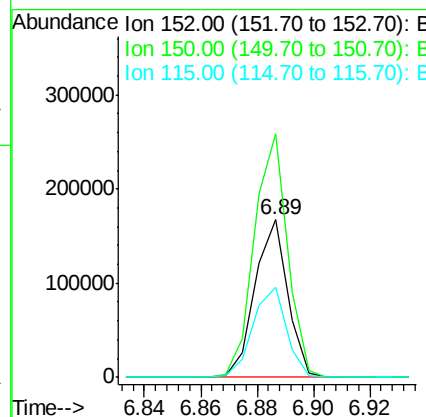

#5

2-Fluorophenol
Concen: 93.215 ng
RT: 5.51 min Scan# 582
Delta R.T. 0.01 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.5	47.9	71.9
63	29.7	23.7	35.5

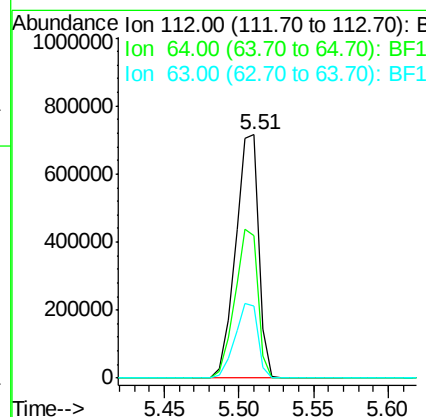



#7

Phenol-d6

Concen: 92.496 ng

RT: 6.51 min Scan# 752

Delta R.T. 0.00 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58

Instrument :

BNA_F





ClientSampleId :

JC-02-110917-A

Tot Ion:	99	Resp:	955565
Ion Ratio	Lower	Upper	
99	100		
42	20.1	14.5	21.7
71	33.6	25.4	38.0

Manual Integrations
APPROVED

SOHIL
11/15/2017 12:30:06 PM

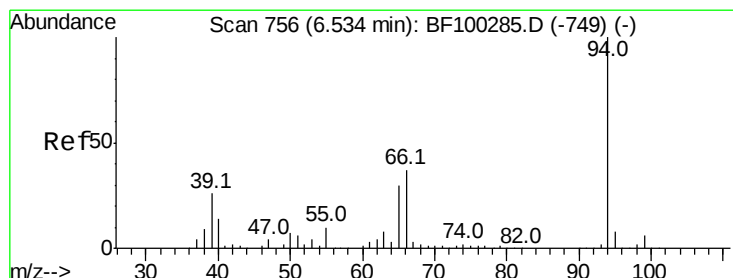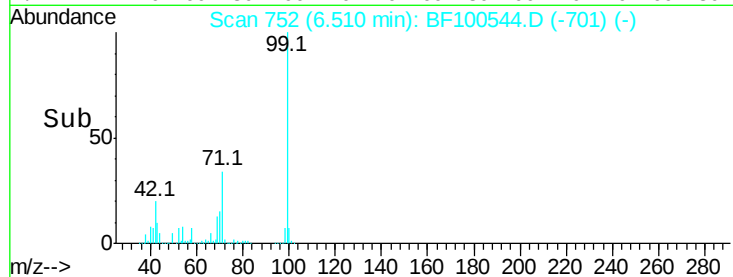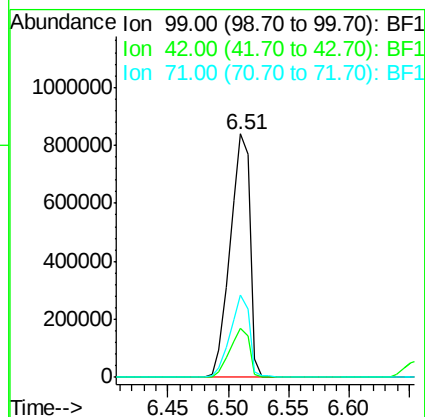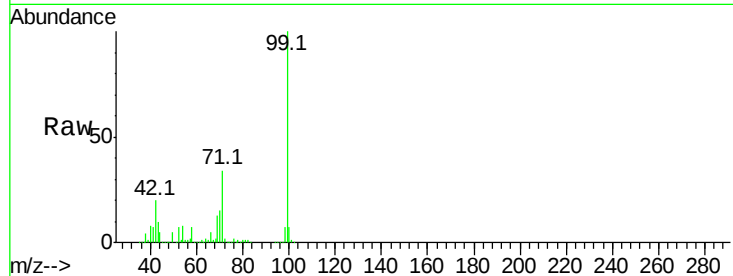

#10

Phenol

Concen: 3.850 ng




RT: 6.52 min Scan# 754

Delta R.T. 0.00 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58

Tgt Ion:	94	Resp:	41756
Ion Ratio	Lower	Upper	
94	100		
65	29.9	7.9	47.9
66	38.4	16.2	56.2

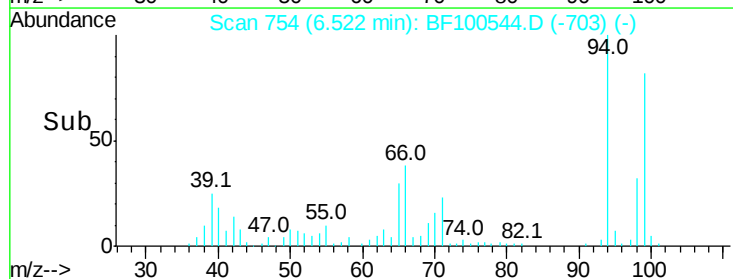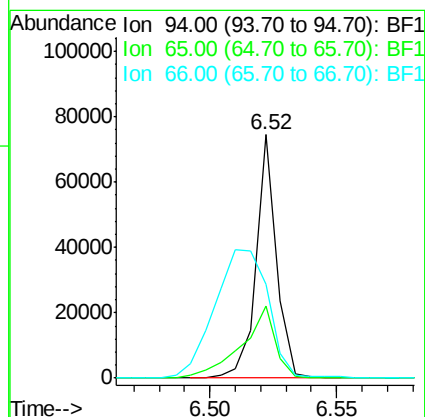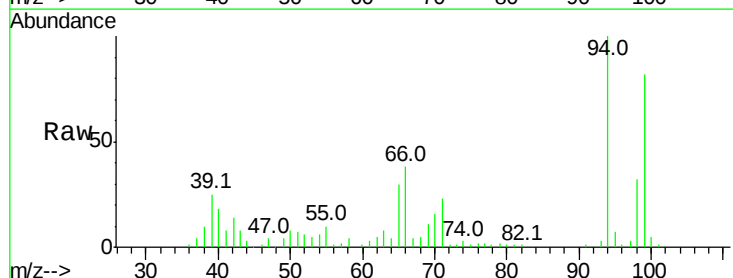







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.17 min Scan# 1034
Delta R.T. 0.00 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Instrument :
BNA_F
ClientSampleId :
JC-02-110917-A

Tot Ion	Ratio	Resp	Lower	Upper
136	100	495554		
137	10.6	8.9	13.3	
54	7.9	6.6	9.8	
68	5.9	5.0	7.4	




Manual Integrations
APPROVED


SOHIL
11/15/2017 12:30:06 PM

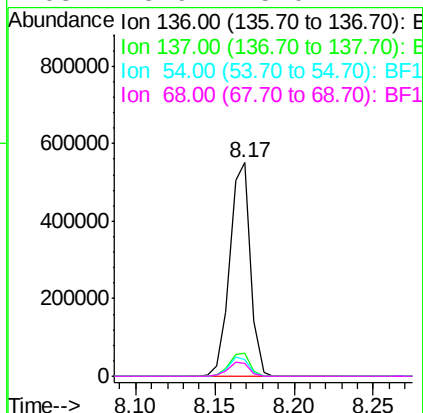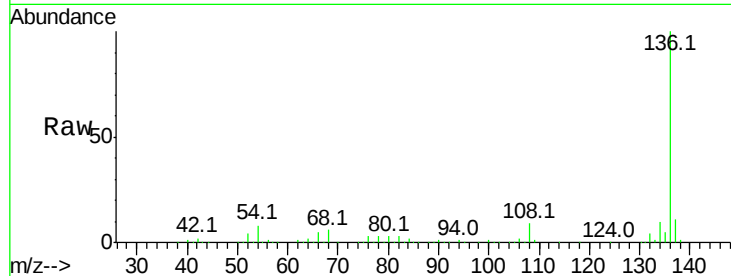

#23
Nitrobenzene-d5
Concen: 77.487 ng
RT: 7.45 min Scan# 911
Delta R.T. -0.01 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Tgt Ion	Ratio	Resp	Lower	Upper
82	100	580805		
128	45.1	36.1	54.1	
54	54.4	41.4	62.2	

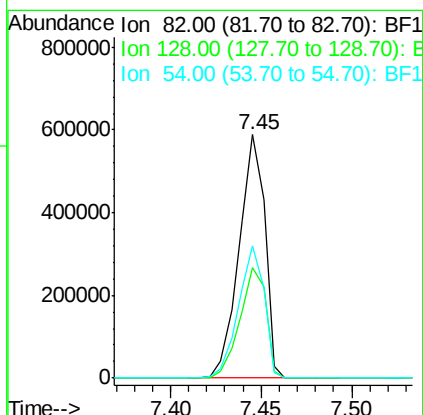

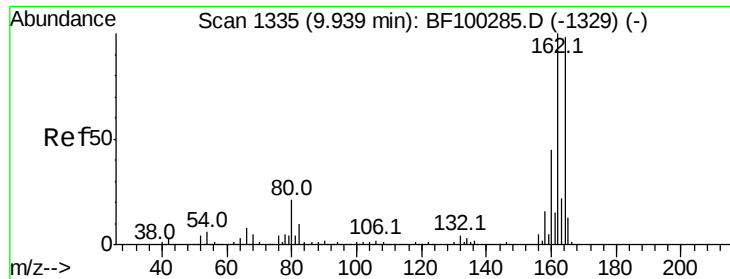





#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.92 min Scan# 1332
 Delta R.T. 0.00 min
 Lab File: BF100544.D
 Acq: 14 Nov 2017 15:58

Instrument :
 BNA_F
 ClientSampleId :
 JC-02-110917-A

Tot Ion	Ratio	Resp	Lower	Upper
164	100	195715		
162	104.8	86.1	129.1	
160	48.5	38.3	57.5	




Manual Integrations
 APPROVED

SOHIL
 11/15/2017 12:30:06 PM

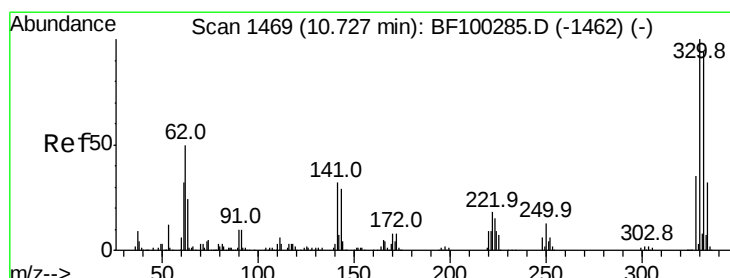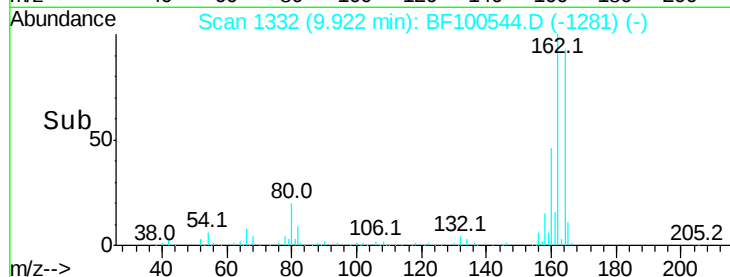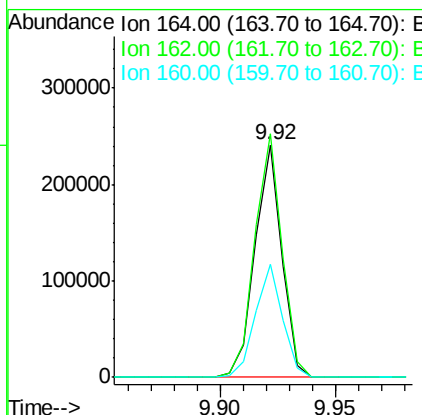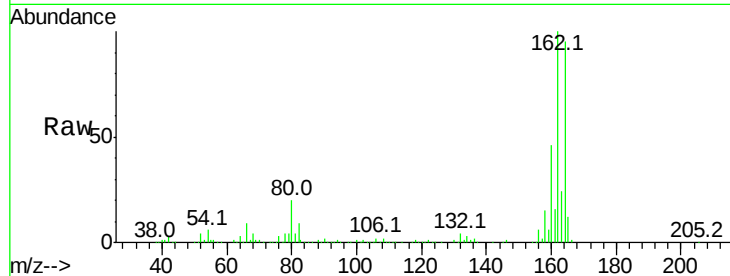

#41
 2,4,6-Tribromophenol
 Concen: 86.954 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. 0.00 min
 Lab File: BF100544.D
 Acq: 14 Nov 2017 15:58

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	173415		
332	93.8	77.0	115.6	
141	30.3	29.9	44.9	

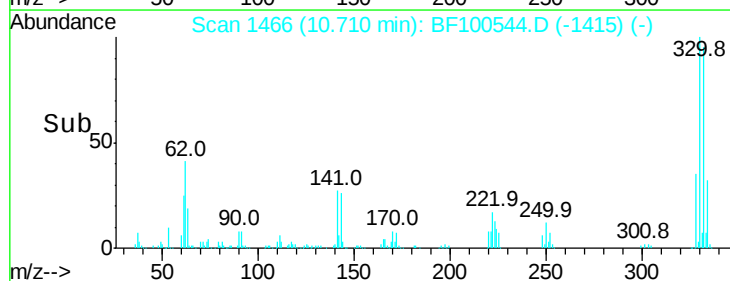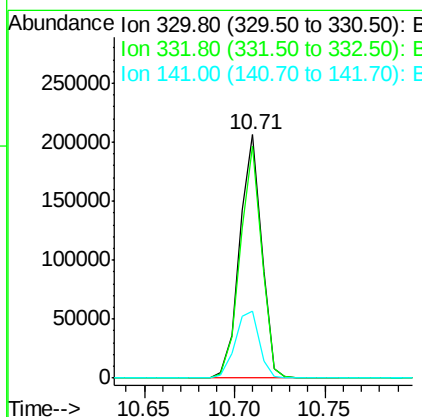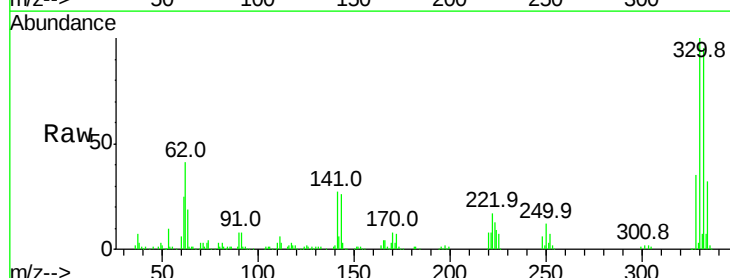




#44
2-Fluorobiphenyl
Concen: 69.056 ng
RT: 9.24 min Scan# 1216
Delta R.T. -0.01 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Instrument :
BNA_F
ClientSampled :
JC-02-110917-A




Tot Ion	Ratio	Resp	Lower	Upper
172	100	887576		
171	36.2		29.7	44.5
170	23.7		19.6	29.4

Manual Integrations
APPROVED

SOHIL
11/15/2017 12:30:06 PM

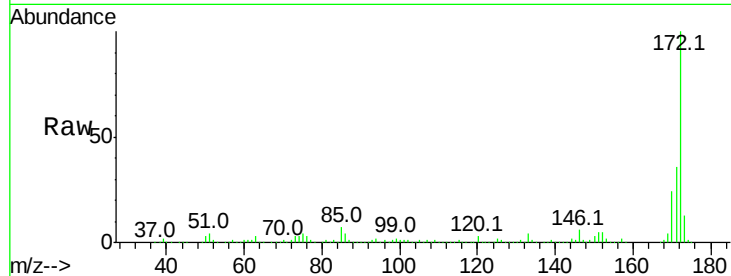


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

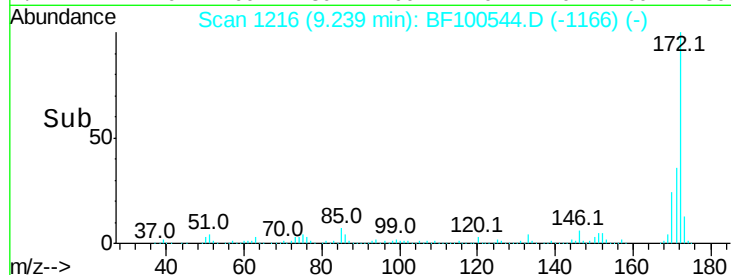
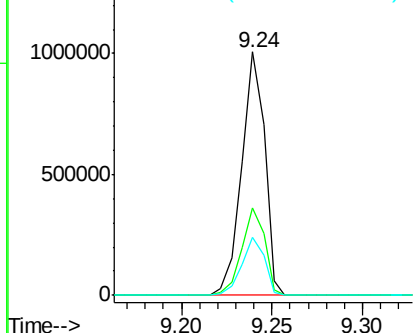


#49
Dimethylphthalate
Concen: 11.243 ng
RT: 9.63 min Scan# 1283
Delta R.T. -0.01 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	168000		
194	3.7		2.7	4.1
164	9.4		8.2	12.2



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

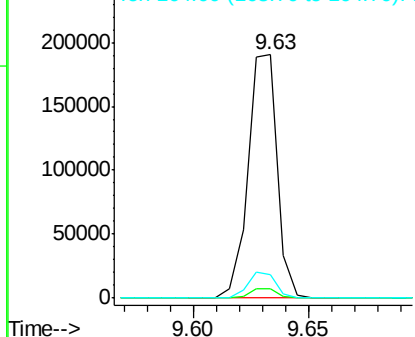







#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. -0.01 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Instrument :
BNA_F
ClientSampleId :
JC-02-110917-A

Tot Ion	Ratio	Resp Lower	Upper
188	100		
94	10.7	8.5	12.7
80	11.5	9.2	13.8




Manual Integrations
APPROVED


SOHIL
11/15/2017 12:30:06 PM

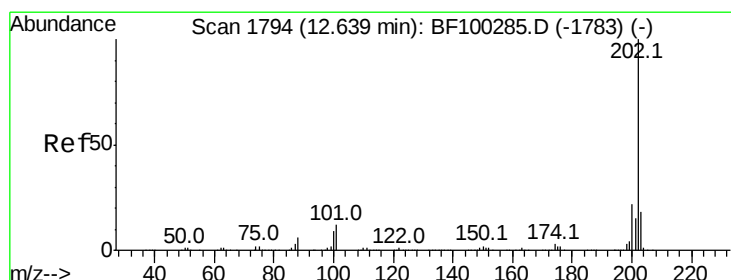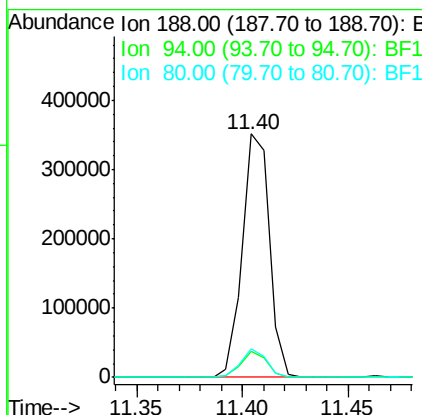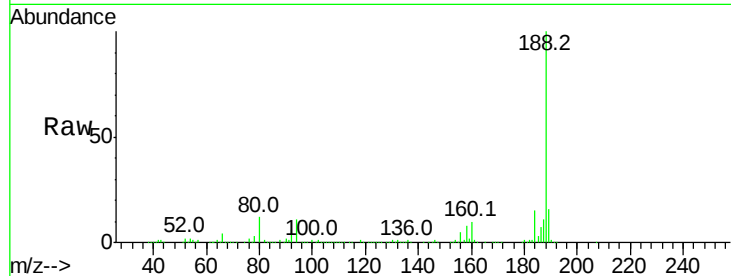

#74
Fluoranthene
Concen: 4.655 ng
RT: 12.62 min Scan# 1790
Delta R.T. -0.01 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Tgt Ion	Ratio	Resp Lower	Upper
202	100		
101	12.9	0.0	34.1
203	17.4	0.0	38.1

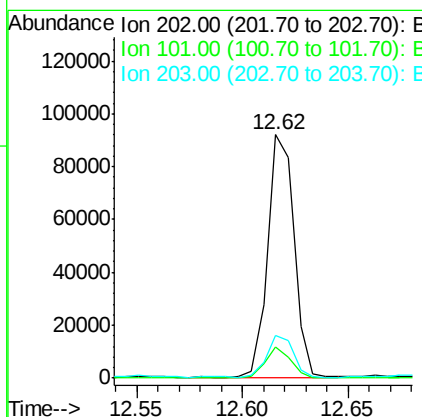

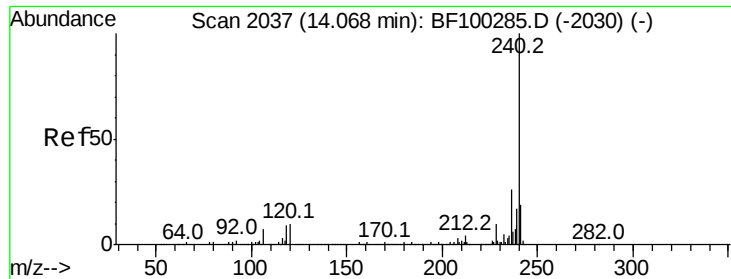

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.04 min Scan# 2033

Delta R.T. -0.01 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58

Instrument :

BNA_F


ClientSampleId :

JC-02-110917-A

Tot Ion	Ratio	Resp	Lower	Upper
240	100	267568		
120	10.8		9.5	14.3
236	24.6		20.7	31.1

Manual Integrations
APPROVED




SOHIL
11/15/2017 12:30:06 PM

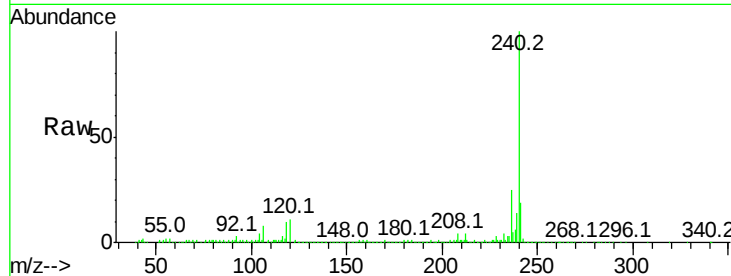

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

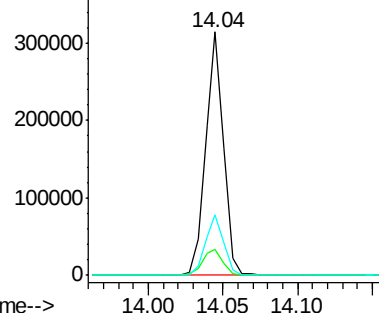

#77

Pyrene

Concen: 3.944 ng


RT: 12.85 min Scan# 1829

Delta R.T. -0.01 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58



Tgt Ion	Ratio	Resp	Lower	Upper
202	100	75229		
200	21.3		17.4	26.2
203	18.4		14.3	21.5




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

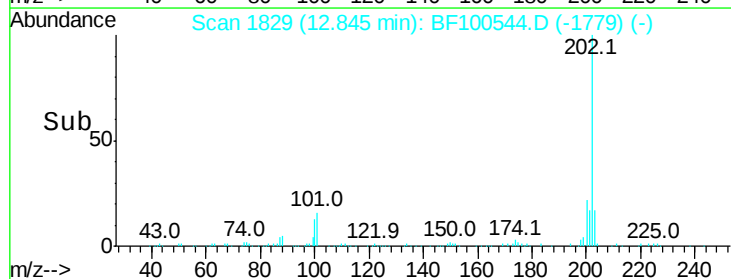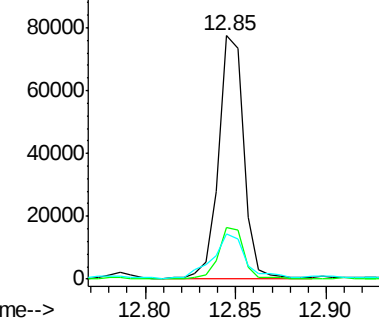

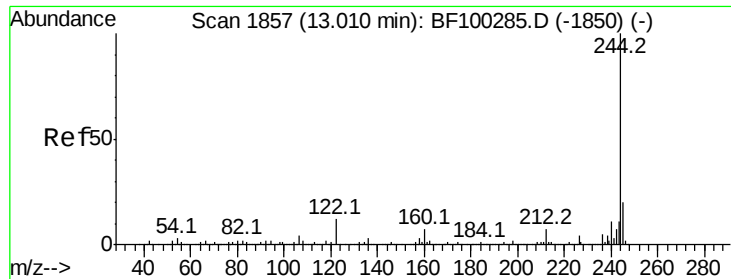

#78

Terphenyl-d14

Concen: 53.763 ng

RT: 12.99 min Scan# 1854

Delta R.T. 0.00 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58

Instrument :

BNA_F





ClientSampleId :

JC-02-110917-A

Tot Ion:	244	Resp:	626069
Ion Ratio	Lower	Upper	
244	100		
212	6.5	5.4	8.0
122	9.8	11.0	16.4

Manual Integrations
APPROVED

SOHIL
11/15/2017 12:30:06 PM

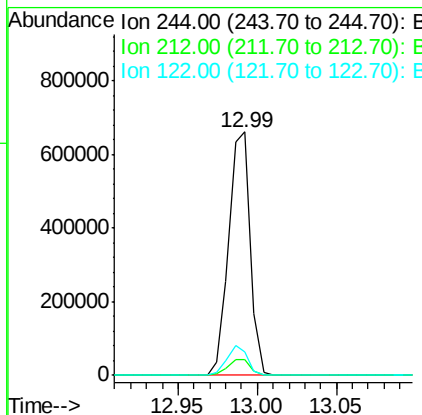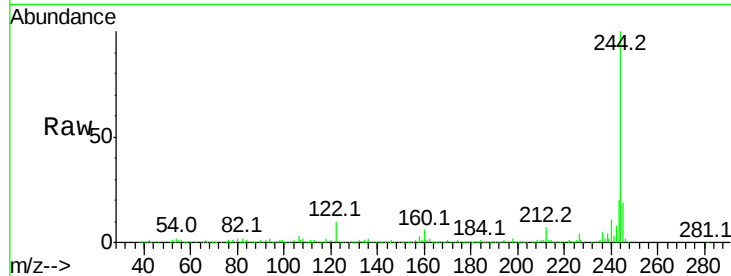

#80

Benzo(a)anthracene

Concen: 2.973 ng




RT: 14.03 min Scan# 2031


Delta R.T. -0.01 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58

Tgt Ion:	228	Resp:	47908
Ion Ratio	Lower	Upper	
228	100		
226	33.3	22.6	33.8
229	21.0	15.8	23.6

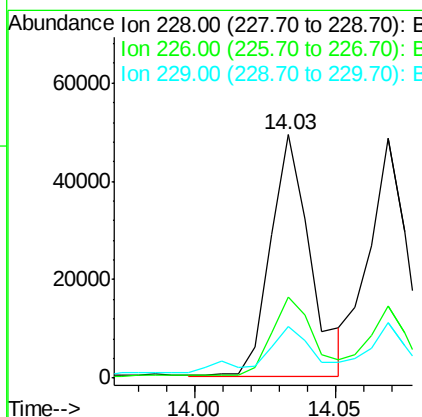

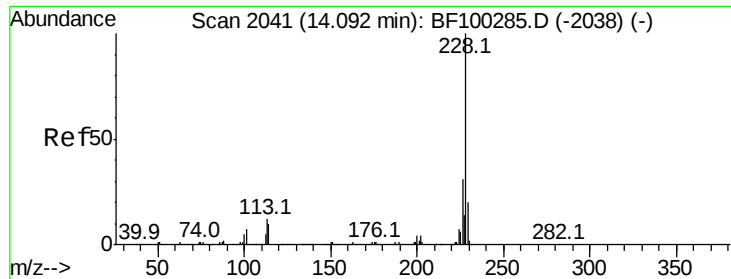





#82
Chrysene
Concen: 2.852 ng
RT: 14.07 min Scan# 2037
Delta R.T. -0.01 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Instrument :
BNA_F
ClientSampleId :
JC-02-110917-A

Tot Ion	Ratio	Lower	Upper
228	100		
226	29.9	25.0	37.6
229	23.3	16.2	24.4




Manual Integrations
APPROVED


SOHIL
11/15/2017 12:30:06 PM

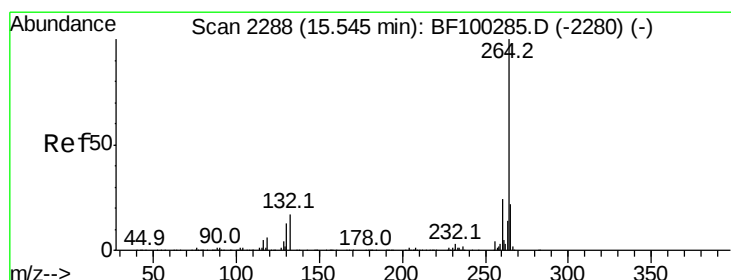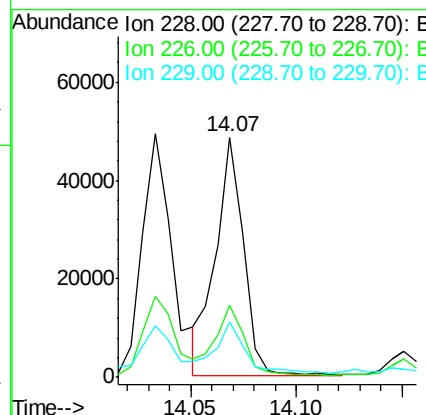

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.52 min Scan# 2284
Delta R.T. 0.00 min
Lab File: BF100544.D
Acq: 14 Nov 2017 15:58

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.2	28.8
265	20.9	17.5	26.3

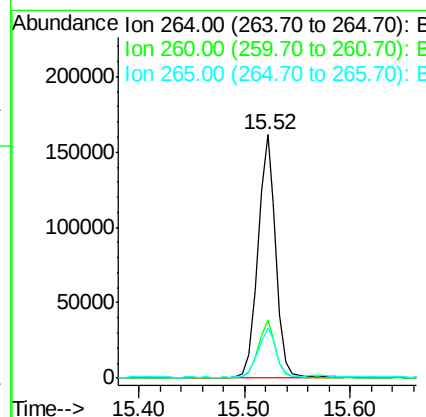

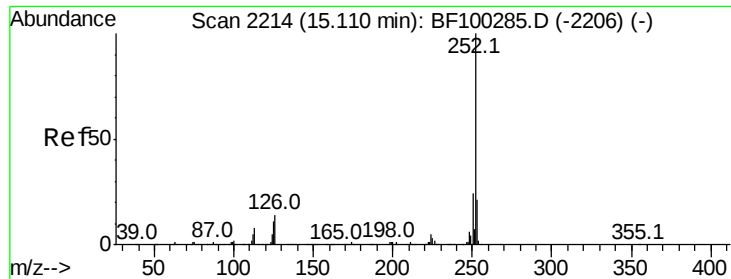

#87

Benzo(b)fluoranthene

Concen: 4.065 ng/mL

RT: 15.09 min Scan# 2210

Delta R.T. -0.01 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58

Instrument :

BNA_F





ClientSampleId :

JC-02-110917-A

Tot Ion:	252	Resp:	46470
Ion Ratio	Lower	Upper	
252	100		
253	24.7	17.0	25.6
125	17.8	9.0	13.6

Manual Integrations
APPROVED

SOHIL
11/15/2017 12:30:06 PM

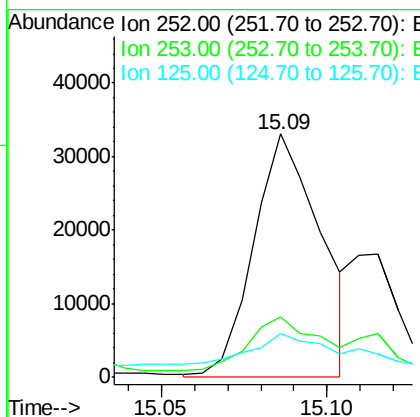

#89

Benzo(a)pyrene

Concen: 3.159 ng/mL




RT: 15.46 min Scan# 2273




Delta R.T. -0.01 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58

Tgt Ion:	252	Resp:	32012
Ion Ratio	Lower	Upper	
252	100		
253	24.8	17.1	25.7
125	19.4	9.8	14.6

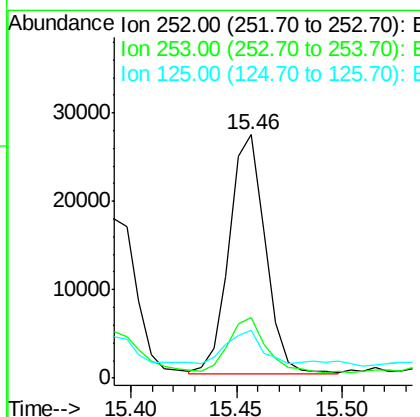

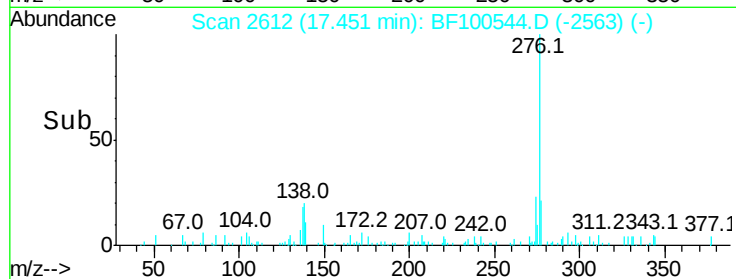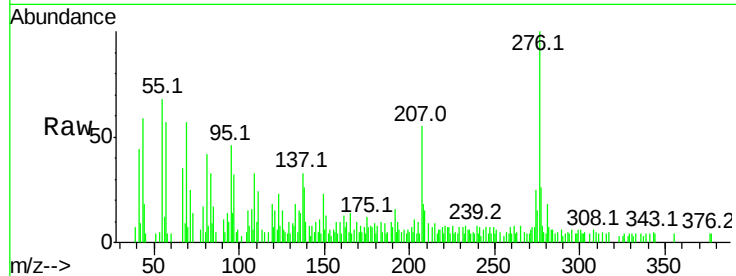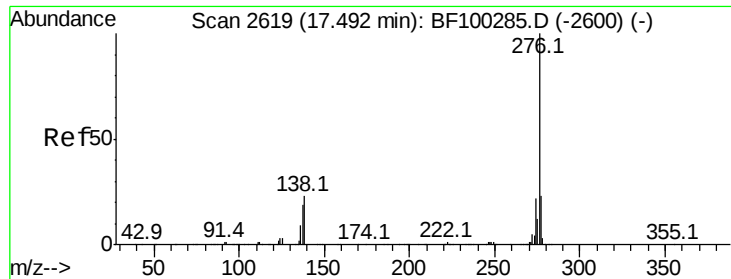

#91

Benzo(a,h,i)perylene

Concen: 2.138 ng

RT: 17.45 min Scan# 2612

Delta R.T. -0.01 min

Lab File: BF100544.D

Acq: 14 Nov 2017 15:58

Instrument :

BNA_F

ClientSampleId :

JC-02-110917-A

Tot Ion: 276 Resp: 17345

Ion Ratio Lower Upper

276 100

277 26.0 17.9 26.9

138 26.0 21.8 32.8

Manual Integrations
APPROVED

SOHIL
11/15/2017 12:30:06 PM

