

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF111417\
 Data File : BF100559.D
 Acq On : 14 Nov 2017 22:44
 Operator : SJ/JU
 Sample : I6388-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 3N-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.222	19	23	32	rVB2	16645	29861	1.05%	0.125%
2	5.116	511	515	524	rBV	654076	833753	29.32%	3.478%
3	5.510	577	582	585	rBV	2744327	2734152	96.14%	11.404%
4	6.510	746	752	760	rBV	2506049	2844028	100.00%	11.862%
5	6.657	772	777	780	rBV	2562376	2684872	94.40%	11.199%
6	6.886	812	816	819	rVB	843811	735627	25.87%	3.068%
7	7.039	838	842	846	rBV	2330332	2151081	75.64%	8.972%
8	7.445	905	911	914	rBV	1716973	1709690	60.12%	7.131%
9	8.163	1029	1033	1037	rBV	950116	905617	31.84%	3.777%
10	9.239	1211	1216	1219	rBV	3022180	2809517	98.79%	11.719%
11	9.627	1279	1282	1285	rBV	160967	120034	4.22%	0.501%
12	9.921	1327	1332	1335	rBV	989516	839250	29.51%	3.501%
13	10.710	1461	1466	1469	rBV	1355023	1283076	45.11%	5.352%
14	11.404	1581	1584	1587	rBV	842957	748545	26.32%	3.122%
15	12.804	1819	1822	1825	rBV	36886	29337	1.03%	0.122%
16	12.992	1849	1854	1857	rBV	2234306	2139424	75.23%	8.924%
17	13.874	2001	2004	2015	rBV2	44007	58407	2.05%	0.244%
18	14.015	2024	2028	2029	rBV	59832	52150	1.83%	0.218%
19	14.045	2029	2033	2036	rVB	739135	704774	24.78%	2.940%
20	15.515	2278	2283	2292	rBV	407896	561847	19.76%	2.343%


Sum of corrected areas: 23975042

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111417\
Data File : BF100559.D
Acq On : 14 Nov 2017 22:44
Operator : SJ/JU
Sample : I6388-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
3N-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

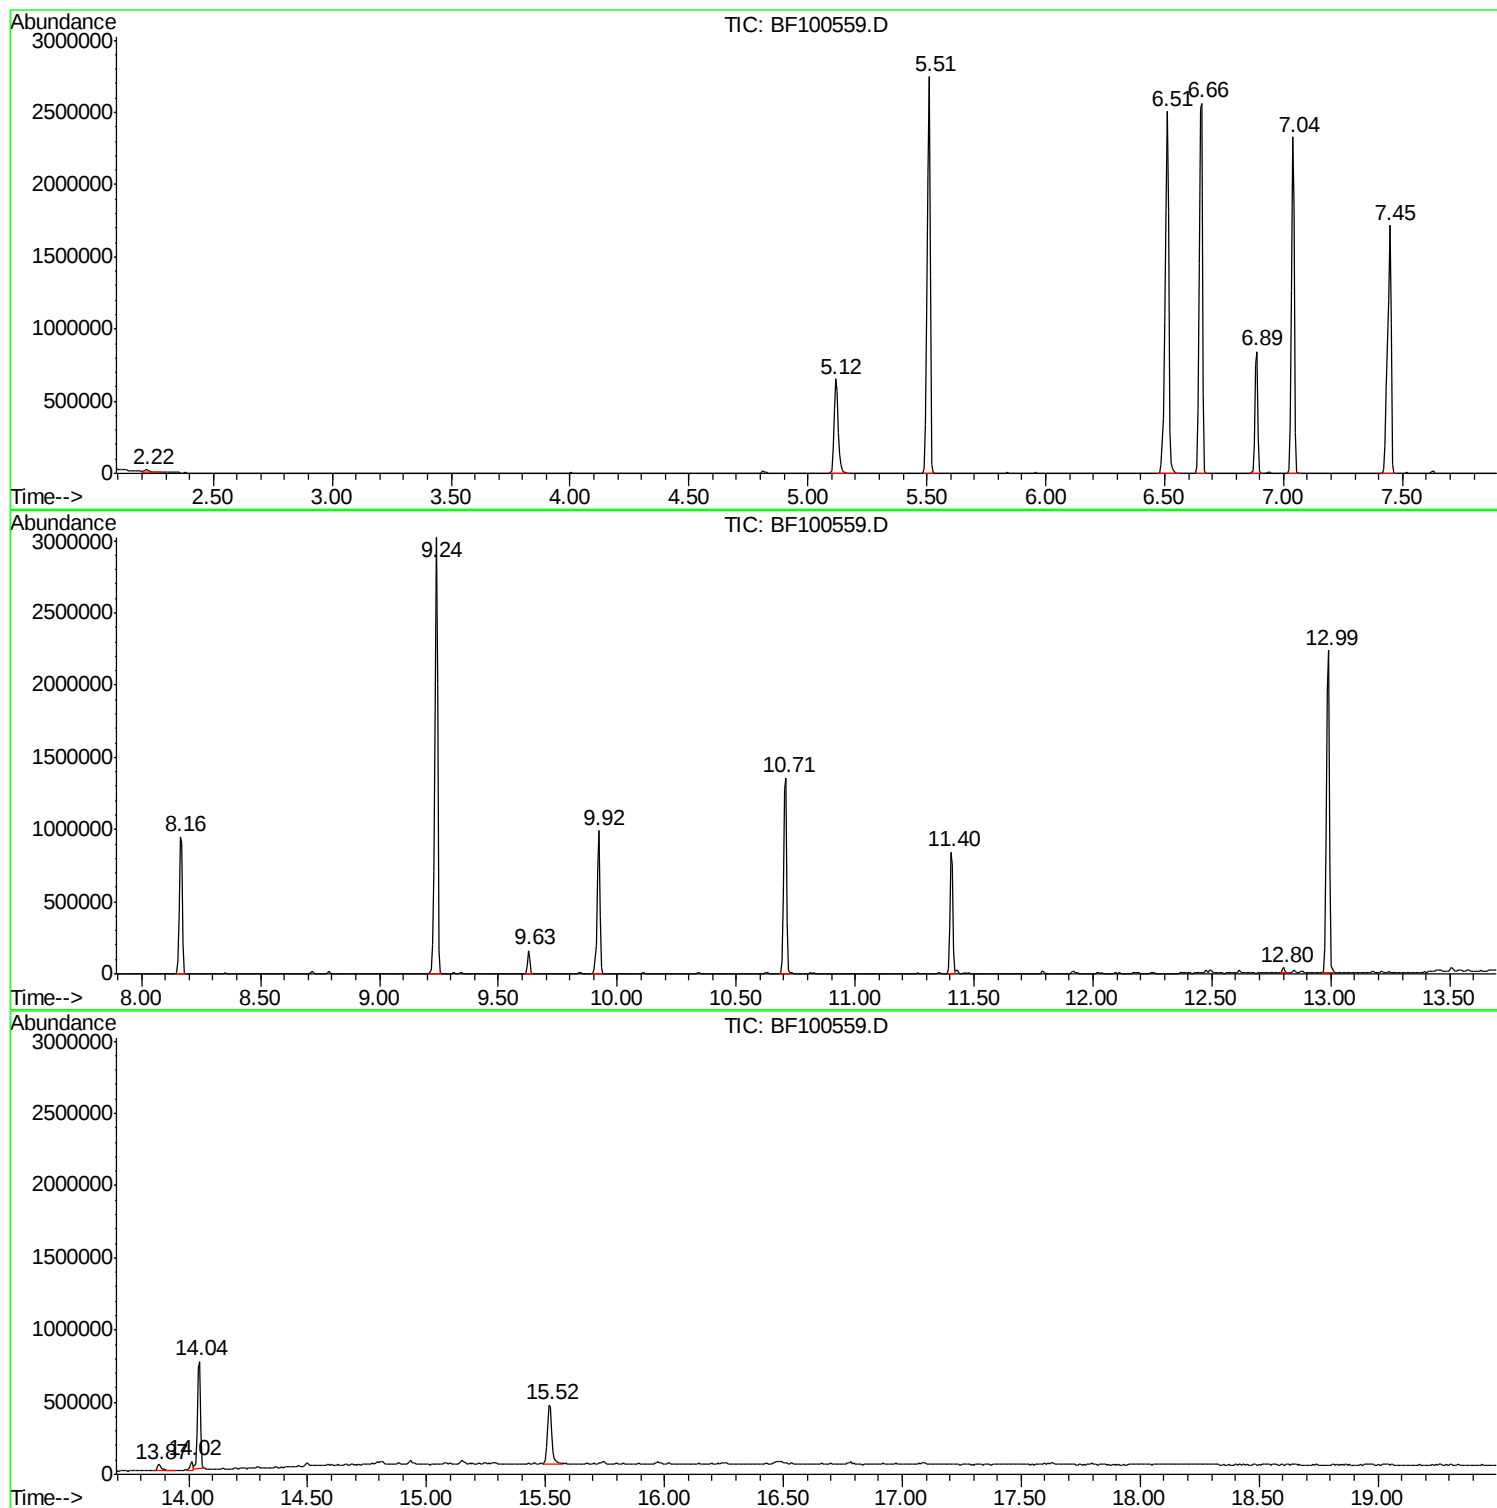

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111417\
Data File : BF100559.D
Acq On : 14 Nov 2017 22:44
Operator : SJ/JU
Sample : I6388-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
3N-1









Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.12	22.67 ng	833753	1,4-Dichlorobenzene-d4	6.89

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
3			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	23
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

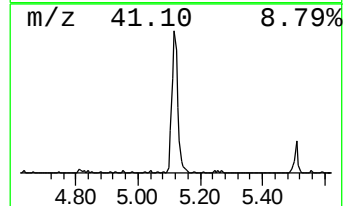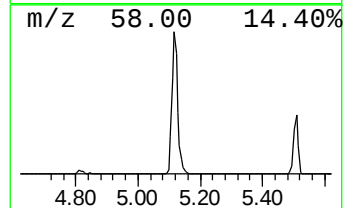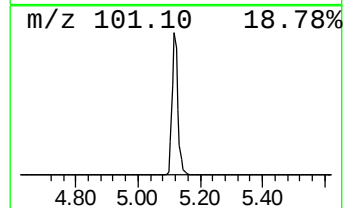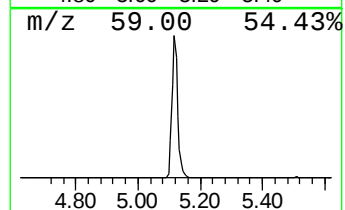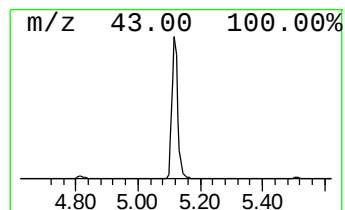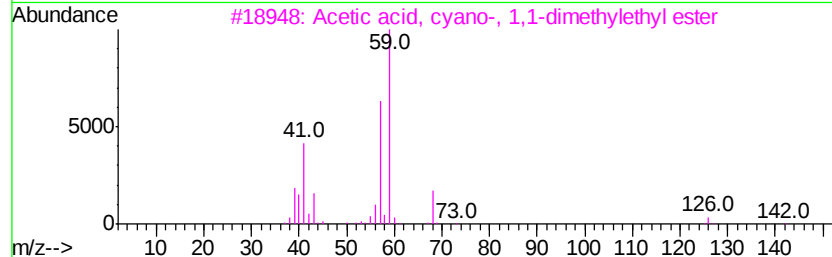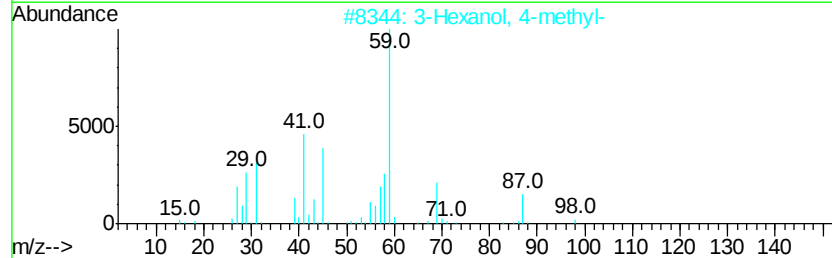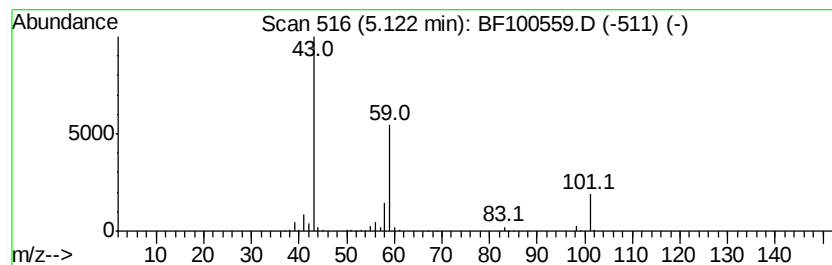

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF111417\
Data File : BF100559.D
Acq On : 14 Nov 2017 22:44
Operator : SJ/JU
Sample : I6388-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
3N-1







Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	73.00 ng	2684870	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

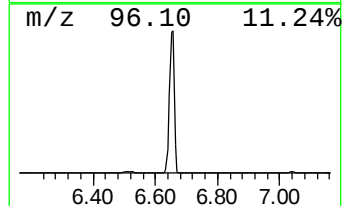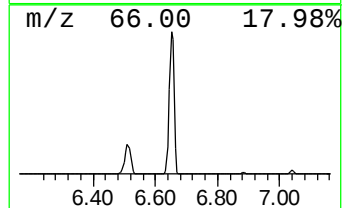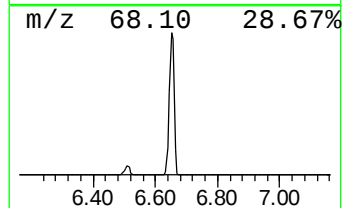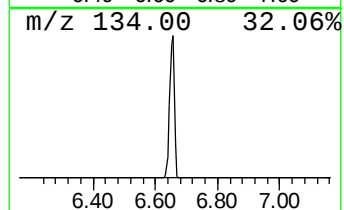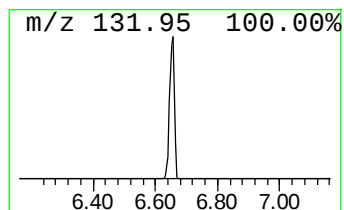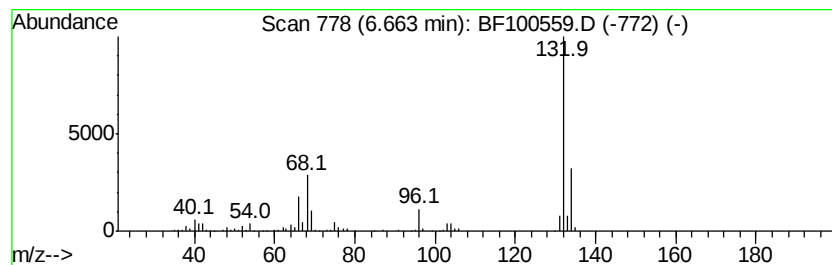

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF111417\
Data File : BF100559.D
Acq On : 14 Nov 2017 22:44
Operator : SJ/JU
Sample : I6388-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
3N-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.12	22.7	ng	833753	1	6.89	735627	20.0
unknown6.66	6.66	73.0	ng	2684870	1	6.89	735627	20.0