


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111417\
 Data File : BF100536.D
 Acq On : 14 Nov 2017 11:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 14 14:17:16 2017

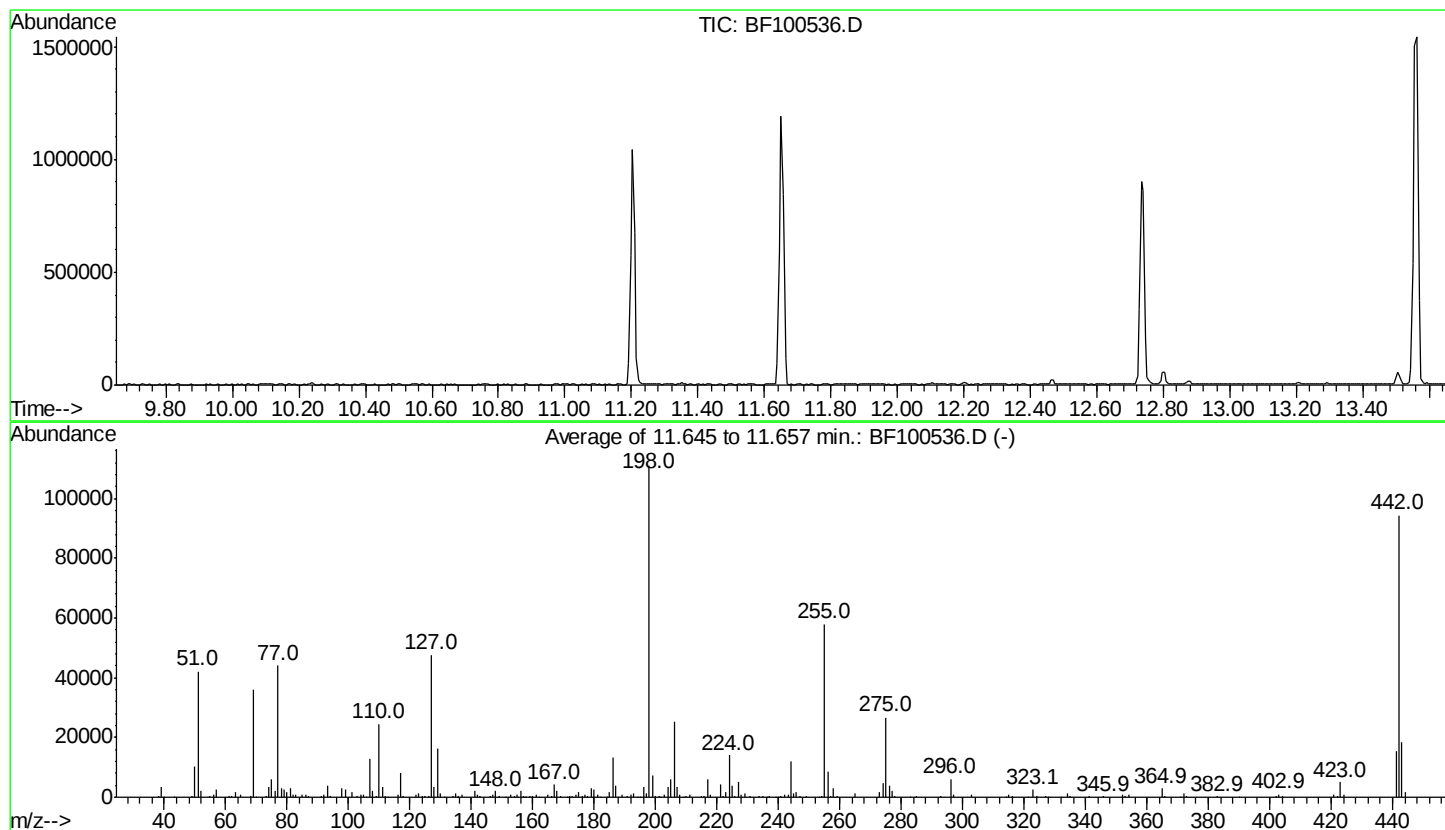

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	42146	PASS
68	69	0.00	2	1.7	604	PASS
69	198	0.00	100	32.4	35949	PASS
70	69	0.00	2	0.3	109	PASS
127	198	10	80	42.9	47656	PASS
197	198	0.00	2	1.0	1118	PASS
198	198	100	100	100.0	110997	PASS
199	198	5	9	6.5	7248	PASS
275	198	10	60	24.1	26780	PASS
365	198	1	100	2.6	2862	PASS
441	443	0.01	100	83.0	15402	PASS
442	198	50	100	84.9	94280	PASS
443	442	15	24	19.7	18550	PASS